

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF083121\
 Data File : BF125281.D
 Acq On : 31 Aug 2021 9:43
 Operator : JU/CG
 Sample : PB138819BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB138819BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF125281.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.281	21	33	39	rVB	98762	143161	2.63%	0.403%
2	5.551	583	589	592	rBV	4634685	4895131	89.90%	13.772%
3	6.545	753	758	761	rBV	4028961	4765713	87.52%	13.408%
4	6.916	817	821	824	rBV	1333338	1118069	20.53%	3.146%
5	7.475	911	916	920	rBV	2779937	3129835	57.48%	8.806%
6	8.198	1034	1039	1051	rBV	1535970	1468764	26.97%	4.132%
7	9.269	1216	1221	1240	rBV	5433800	5445325	100.00%	15.320%
8	9.951	1332	1337	1349	rBV	1841160	1620534	29.76%	4.559%
9	10.739	1466	1471	1488	rBV	3236205	3546249	65.12%	9.977%
10	11.439	1586	1590	1598	rBV	1773786	1621810	29.78%	4.563%
11	13.027	1855	1860	1863	rBV	5963817	5443023	99.96%	15.314%
12	14.080	2035	2039	2048	rBV	1225087	1249993	22.96%	3.517%
13	15.580	2289	2294	2306	rBV	655324	1095660	20.12%	3.083%

Sum of corrected areas: 35543267

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF083121\
Data File : BF125281.D
Acq On : 31 Aug 2021 9:43
Operator : JU/CG
Sample : PB138819BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB138819BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.281	2.56 ng	143161	1,4-Dichlorobenzene-d4	6.916

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2			3-Pentanol, 2,4-dimethyl-	116	C7H16O	000600-36-2	43
3			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40
4			3-Pentanol, 3-methyl-	102	C6H14O	000077-74-7	32
5			2-Methyl-5-hexen-3-ol	114	C7H14O	032815-70-6	32

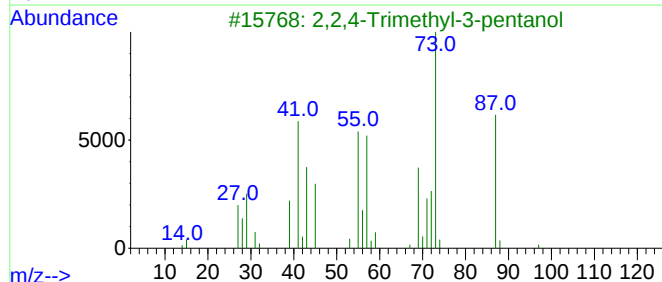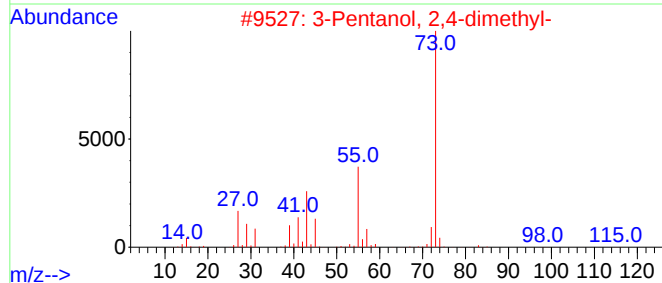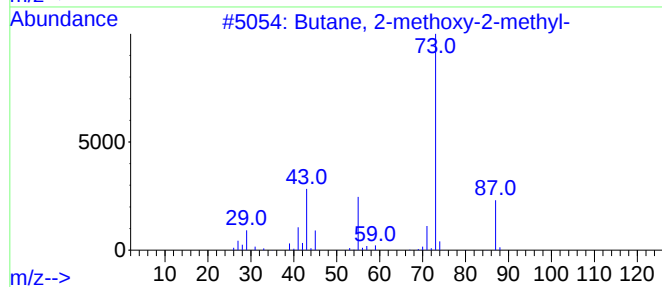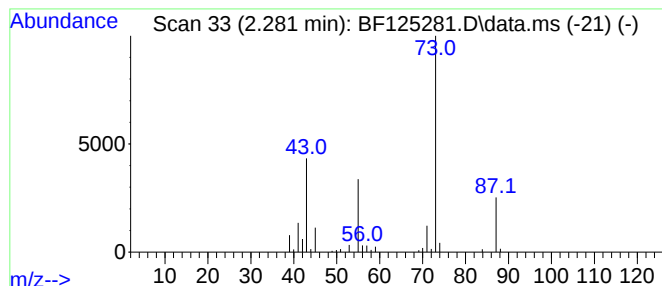

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF083121\
Data File : BF125281.D
Acq On : 31 Aug 2021 9:43
Operator : JU/CG
Sample : PB138819BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB138819BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.281	2.6	ng	143161	1	6.916	1118070	20.0