

Data Path : Z:\HPCHEM1\BNA F\DATA\BF090115\
 Data File : BF081335.D
 Acq On : 2 Sep 2015 7:25
 Operator : UM/IZ
 Sample : G3480-15
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Sep 02 07:50:18 2015
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF090115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 01 17:35:35 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.55	152	202816	20.00	ng	0.16
21) Naphthalene-d8	7.68	136	242146	20.00	ng	0.00
38) Acenaphthene-d10	9.42	164	118007	20.00	ng	0.00
63) Phenanthrene-d10	10.88	188	219779	20.00	ng	0.00
75) Chrysene-d12	13.49	240	159220	20.00	ng	-0.01
86) Perylene-d12	14.80	264	123560	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	4.94	112	414502	31.71	ng	0.01
7) Phenol-d6	6.06	99	667124	38.55	ng	0.00
23) Nitrobenzene-d5	6.96	82	351722	70.08	ng	-0.01
41) 2,4,6-Tribromophenol	10.20	330	113266	107.80	ng	0.00
44) 2-Fluorobiphenyl	8.76	172	602519	65.43	ng	0.00
78) Terphenyl-d14	12.47	244	488048	71.35	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propylamine	6.96	70	47415	4.03	ng	# 63
49) Dimethylphthalate	9.16	163	142853	15.58	ng	# 97
56) 2,4-Dinitrotoluene	9.42	165	14970	5.65	ng	# 31
66) 4-Bromophenyl-phenylether	10.19	248	7892	3.55	ng	# 1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF090115\
Data File : BF081335.D
Acq On : 2 Sep 2015 7:25
Operator : UM/IZ
Sample : G3480-15
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Sep 02 07:50:18 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF090115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 01 17:35:35 2015
Response via : Initial Calibration

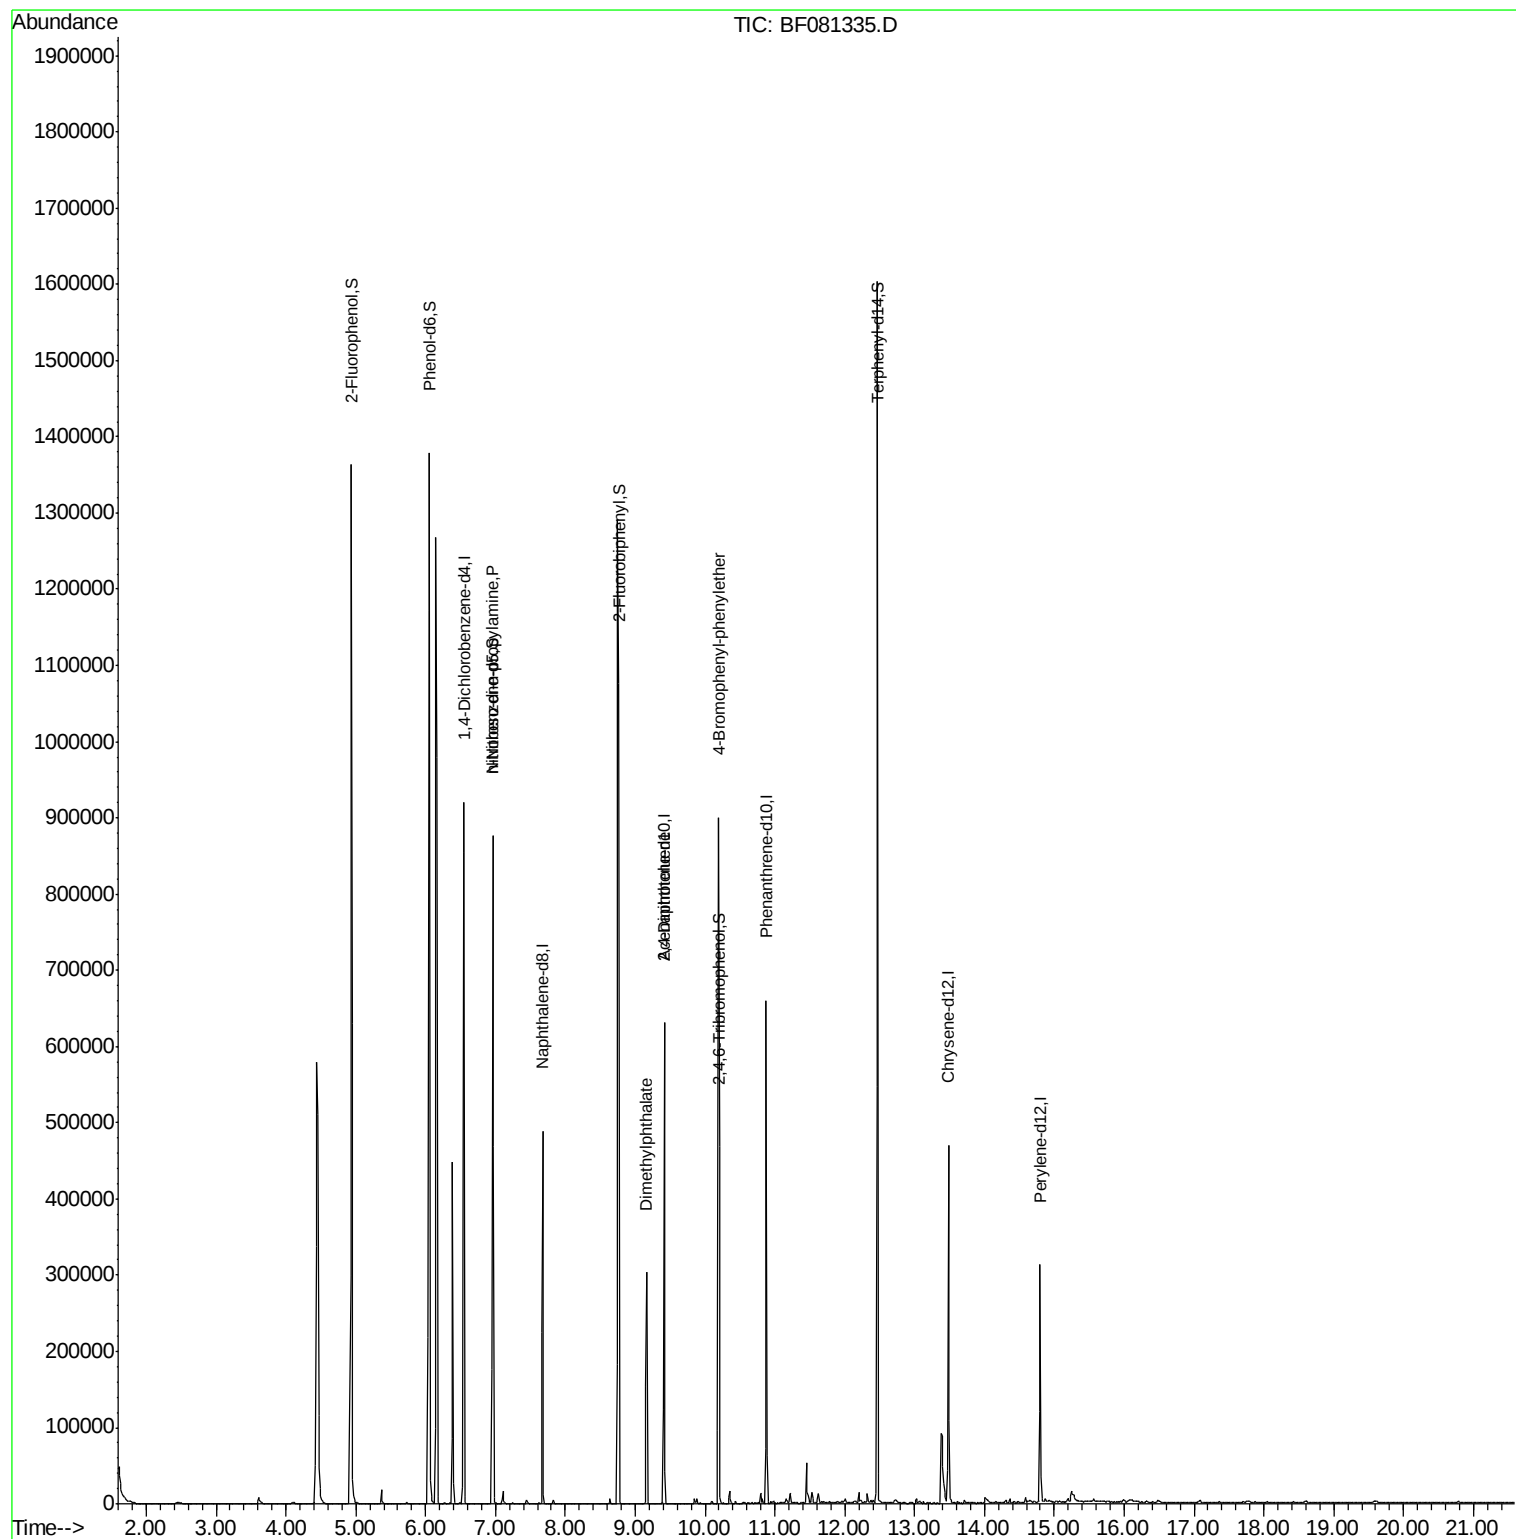







#1
 1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 6.55 min Scan# 434
 Delta R.T. 0.16 min
 Lab File: BF081335.D
 Acq: 2 Sep 2015 7:25

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:152 Resp: 202816
 Ion Ratio Lower Upper
 152 100
 150 154.2 124.7 187.1
 115 58.4 39.0 58.4

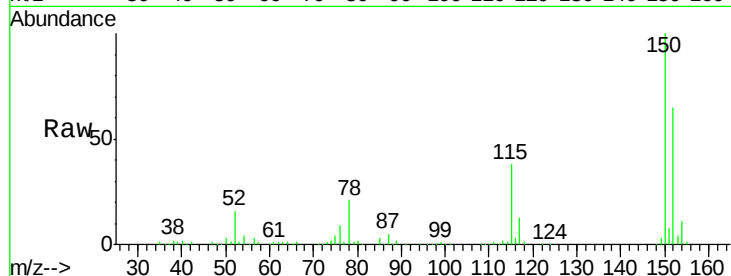


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

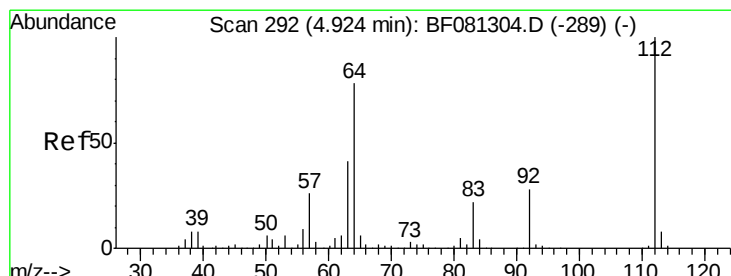
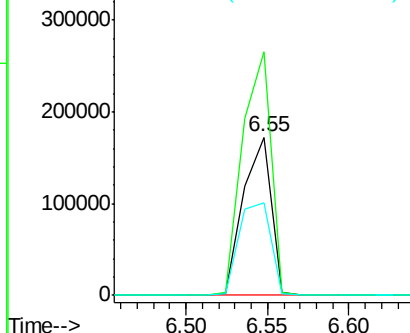


#5
 2-Fluorophenol
 Concen: 31.71 ng
 RT: 4.94 min Scan# 293
 Delta R.T. 0.01 min
 Lab File: BF081335.D
 Acq: 2 Sep 2015 7:25

Tgt Ion:112 Resp: 414502
 Ion Ratio Lower Upper
 112 100
 64 78.6 39.7 59.5#
 63 41.6 17.4 26.0#

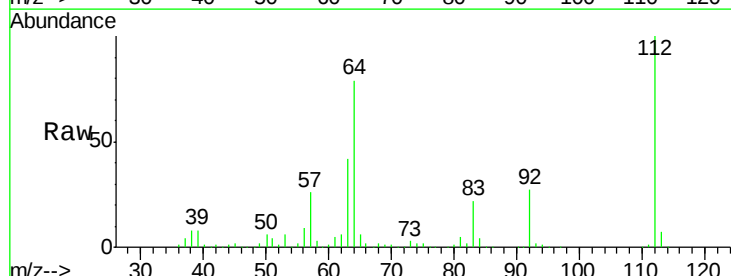

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF0
 Ion 63.00 (62.70 to 63.70): BF0

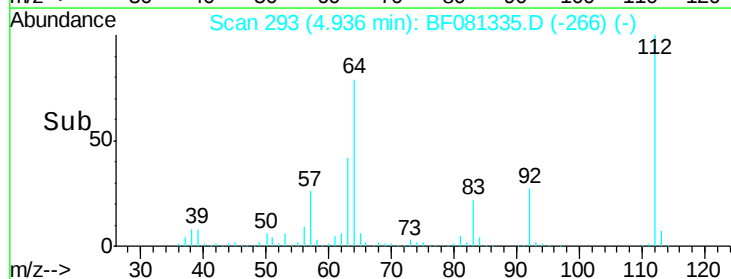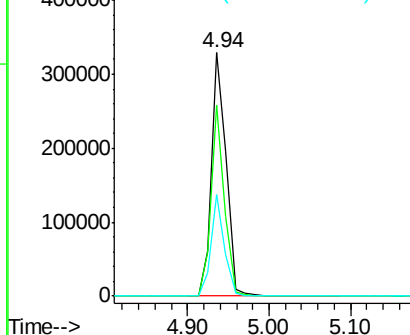



#7

Phenol-d6

Concen: 38.55 ng

RT: 6.06 min Scan# 391

Delta R.T. 0.00 min

Lab File: BF081335.D

Acq: 2 Sep 2015 7:25

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 99 Resp: 667124

Ion Ratio Lower Upper

99 100

42 16.8 13.7 20.5




71 32.6 14.2 21.2#

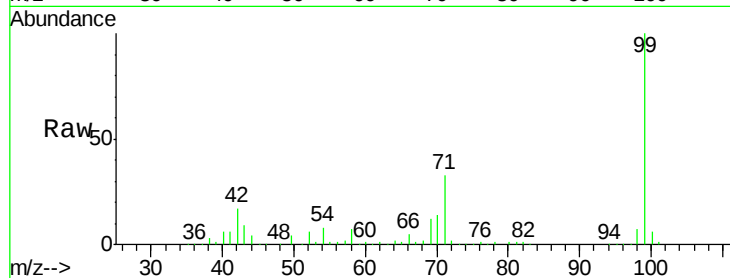

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

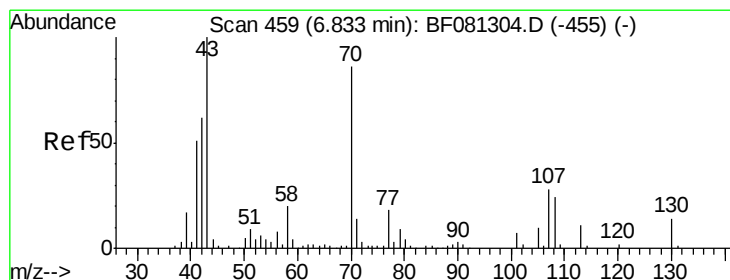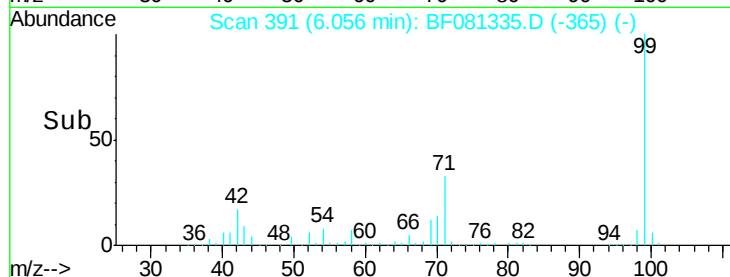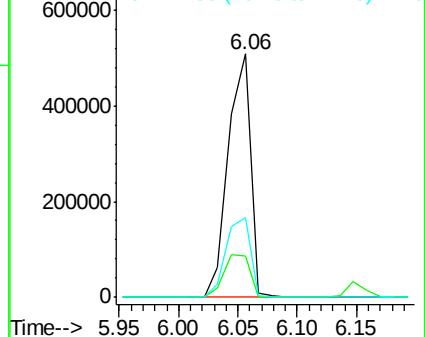

#19

n-Nitroso-di-n-propylamine

Concen: 4.03 ng

RT: 6.96 min Scan# 470

Delta R.T. 0.13 min

Lab File: BF081335.D

Acq: 2 Sep 2015 7:25

Tgt Ion: 70 Resp: 47415


Ion Ratio Lower Upper

70 100

42 53.5 63.8 95.6#

101 0.0 9.2 13.8#

130 1.7 27.3 40.9#


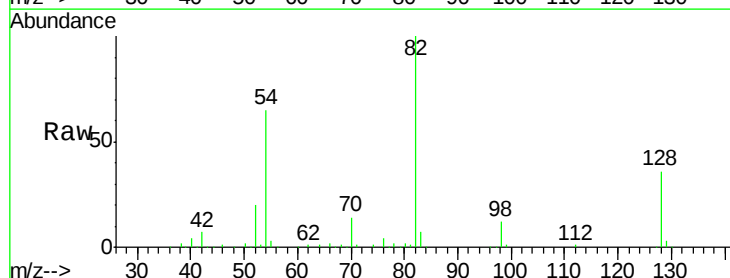


Abundance Ion 70.00 (69.70 to 70.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 101.00 (100.70 to 101.70): BF0

Ion 130.00 (129.70 to 130.70): BF0

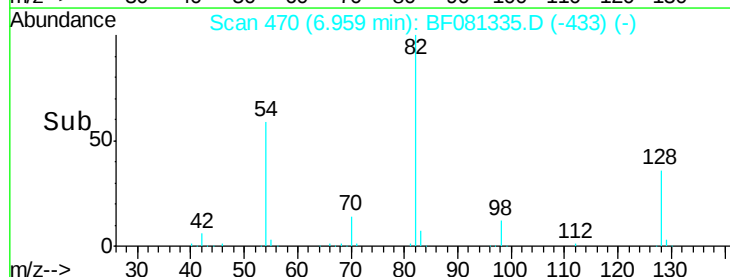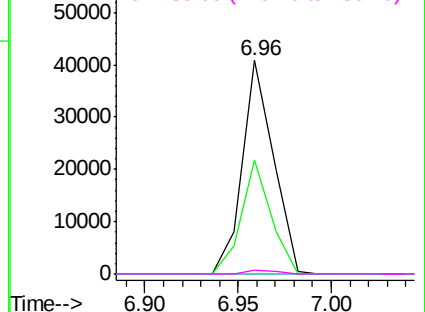



#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.68 min Scan# 533

Delta R.T. 0.00 min

Lab File: BF081335.D

Acq: 2 Sep 2015 7:25

Instrument :

BNA_F

ClientSampleId :

Tot Ion:136 Resp: 242146


Ion Ratio Lower Upper

136 100

137 10.6 9.0 13.6

54 8.8 8.2 12.2

68 4.1 5.8 8.6#



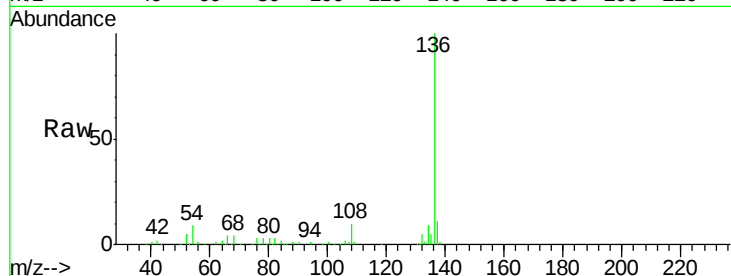


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

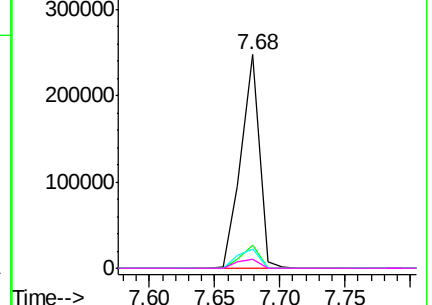

#23

Nitrobenzene-d5

Concen: 70.08 ng

RT: 6.96 min Scan# 470

Delta R.T. -0.01 min

Lab File: BF081335.D

Acq: 2 Sep 2015 7:25


Tgt Ion: 82 Resp: 351722

Ion Ratio Lower Upper

82 100

128 36.0 51.0 76.6#



54 65.0 47.5 71.3




Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF0

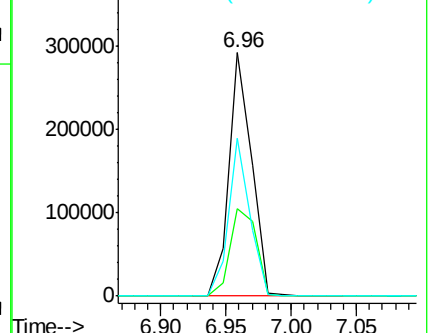



#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.42 min Scan# 685

Delta R.T. 0.00 min

Lab File: BF081335.D

Acq: 2 Sep 2015 7:25

Instrument :

BNA_F

ClientSampleId :


Tot Ion:164 Resp: 118007

Ion Ratio Lower Upper

164 100

162 102.1 75.2 112.8




160 47.2 31.5 47.3



Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

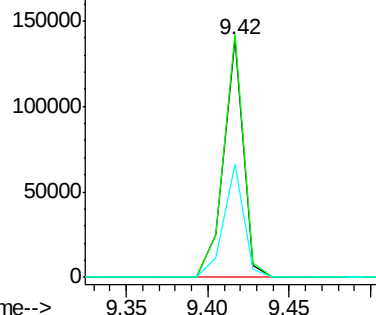

#41

2,4,6-Tribromophenol

Concen: 107.80 ng

RT: 10.20 min Scan# 754

Delta R.T. 0.00 min

Lab File: BF081335.D

Acq: 2 Sep 2015 7:25


Tgt Ion:330 Resp: 113266

Ion Ratio Lower Upper

330 100

332 98.5 76.6 114.8



141 39.4 29.7 44.5




Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

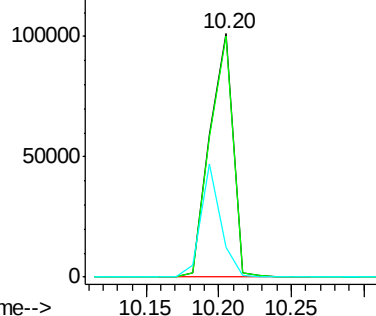


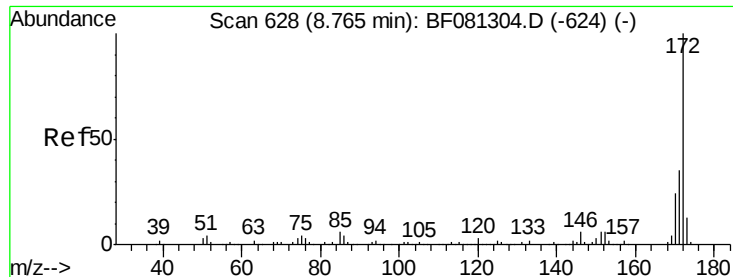




#44
2-Fluorobiphenyl
Concen: 65.43 ng
RT: 8.76 min Scan# 628
Delta R.T. 0.00 min
Lab File: BF081335.D
Acq: 2 Sep 2015 7:25

Instrument :
BNA_F
ClientSampleId :

Tot Ion:172 Resp: 602519
Ion Ratio Lower Upper
172 100
171 35.2 26.1 39.1
170 23.8 17.4 26.2

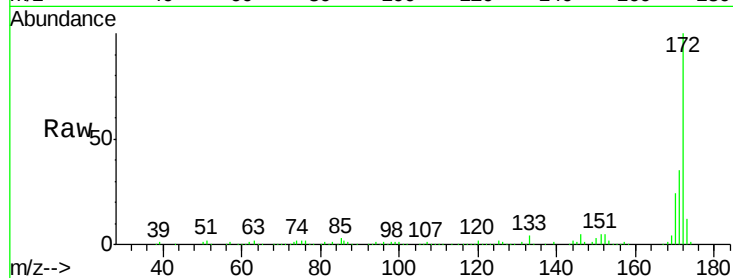


Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

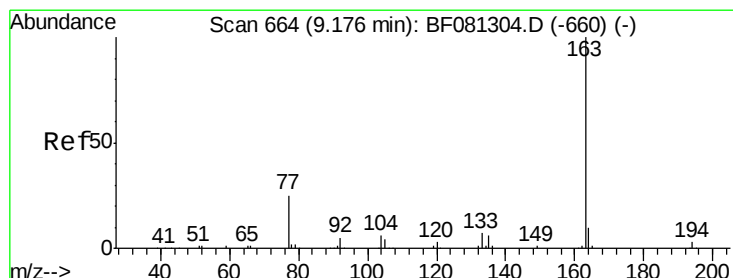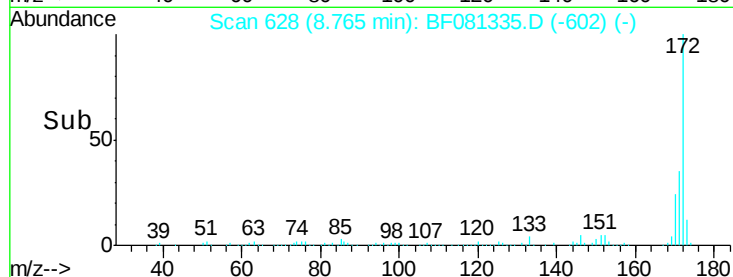
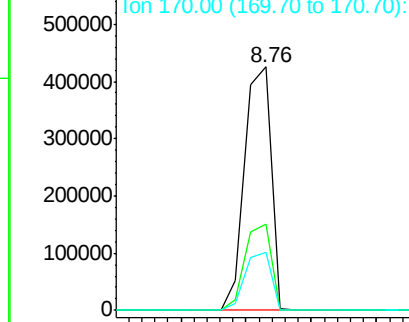


#49
Dimethylphthalate
Concen: 15.58 ng
RT: 9.16 min Scan# 663
Delta R.T. -0.01 min
Lab File: BF081335.D
Acq: 2 Sep 2015 7:25

Tgt Ion:163 Resp: 142853
Ion Ratio Lower Upper
163 100
194 3.4 4.4 6.6#
164 9.7 8.3 12.5

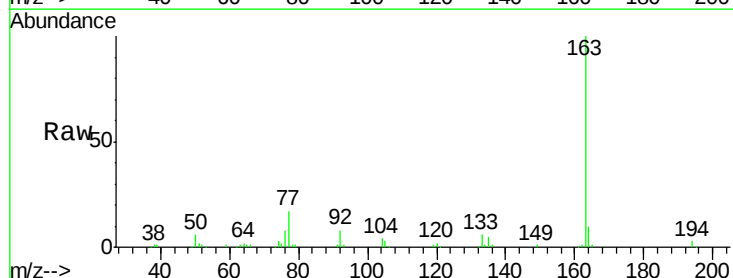

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E



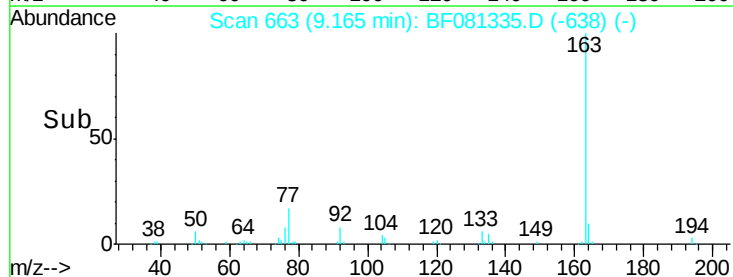
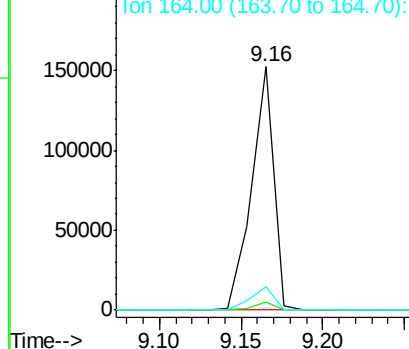




#56
 2,4-Dinitrotoluene
 Concen: 5.65 ng
 RT: 9.42 min Scan# 685
 Delta R.T. -0.22 min
 Lab File: BF081335.D
 Acq: 2 Sep 2015 7:25




Instrument :
 BNA_F
 ClientSampleId :


Tot Ion:165 Resp: 14970
 Ion Ratio Lower Upper
 165 100
 63 0.0 29.8 44.6#
 89 0.0 44.5 66.7#
 182 0.0 3.0 4.4#

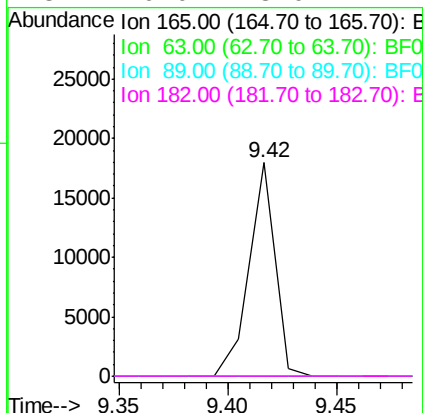

#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 10.88 min Scan# 813
 Delta R.T. 0.00 min
 Lab File: BF081335.D
 Acq: 2 Sep 2015 7:25

Tgt Ion:188 Resp: 219779
 Ion Ratio Lower Upper
 188 100
 94 9.1 11.1 16.7#
 80 9.3 11.0 16.4#

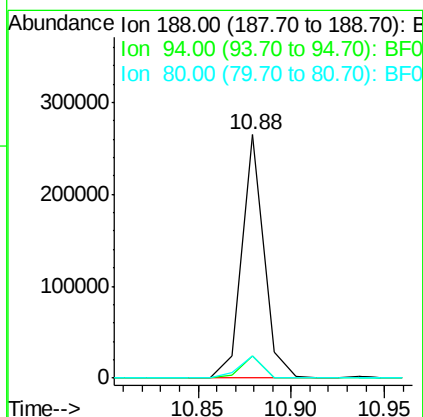


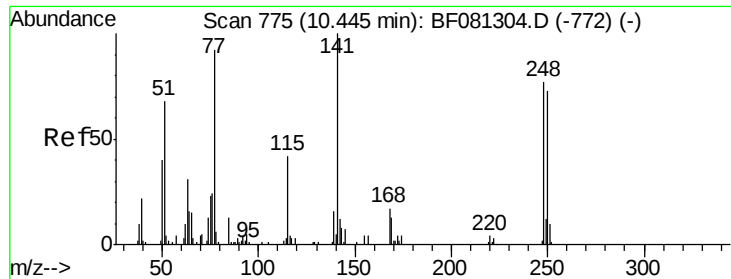




#66
 4-Bromophenyl-phenylether
 Concen: 3.55 ng
 RT: 10.19 min Scan# 753
 Delta R.T. -0.25 min
 Lab File: BF081335.D
 Acq: 2 Sep 2015 7:25

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:248 Resp: 7892
 Ion Ratio Lower Upper
 248 100
 250 203.5 78.5 117.7#
 141 805.8 59.0 88.6#

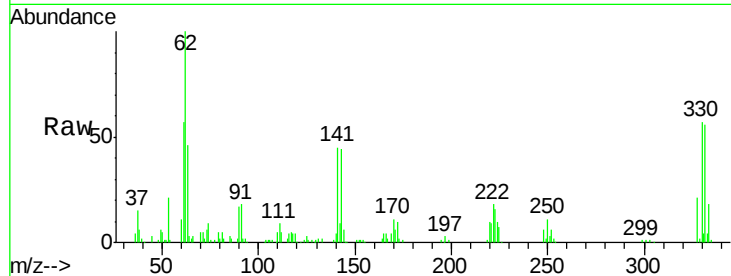


Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E


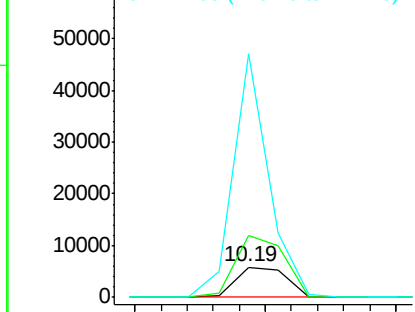


#75
 Chrysene-d12
 Concen: 20.00 ng
 RT: 13.49 min Scan# 1041
 Delta R.T. -0.01 min
 Lab File: BF081335.D
 Acq: 2 Sep 2015 7:25

Tgt Ion:240 Resp: 159220
 Ion Ratio Lower Upper
 240 100
 120 11.5 16.2 24.2#
 236 26.0 18.4 27.6



Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E




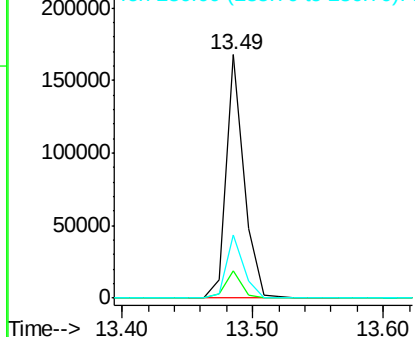




#78
 Terphenyl-d14
 Concen: 71.35 ng
 RT: 12.47 min Scan# 952
 Delta R.T. 0.00 min
 Lab File: BF081335.D
 Acq: 2 Sep 2015 7:25

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:244 Resp: 488048
 Ion Ratio Lower Upper
 244 100
 212 7.7 4.3 6.5#
 122 10.3 17.4 26.2#

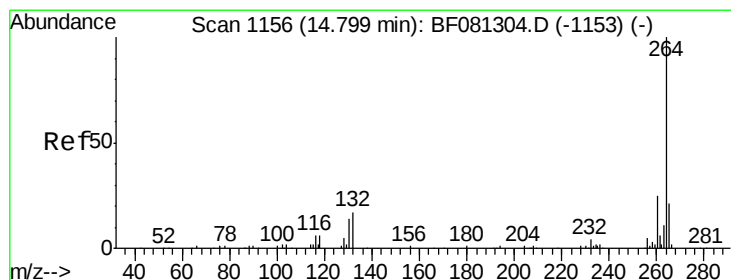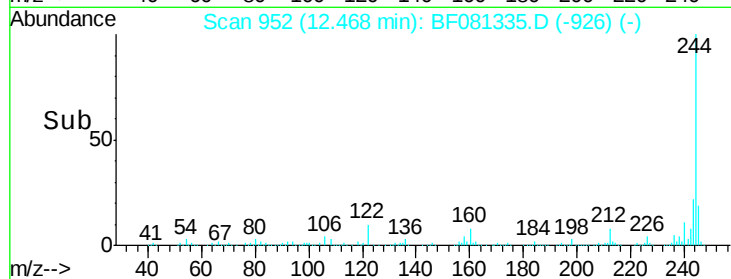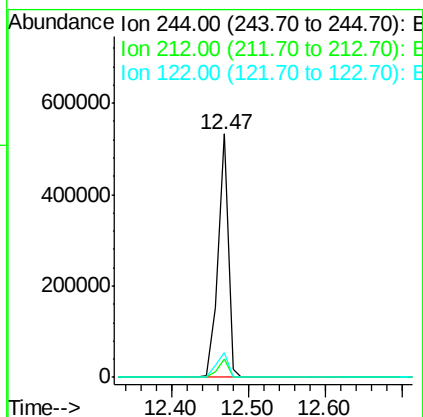

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 14.80 min Scan# 1156
 Delta R.T. 0.00 min
 Lab File: BF081335.D
 Acq: 2 Sep 2015 7:25

Tgt Ion:264 Resp: 123560
 Ion Ratio Lower Upper
 264 100
 260 24.1 16.7 25.1
 265 21.4 17.2 25.8

