
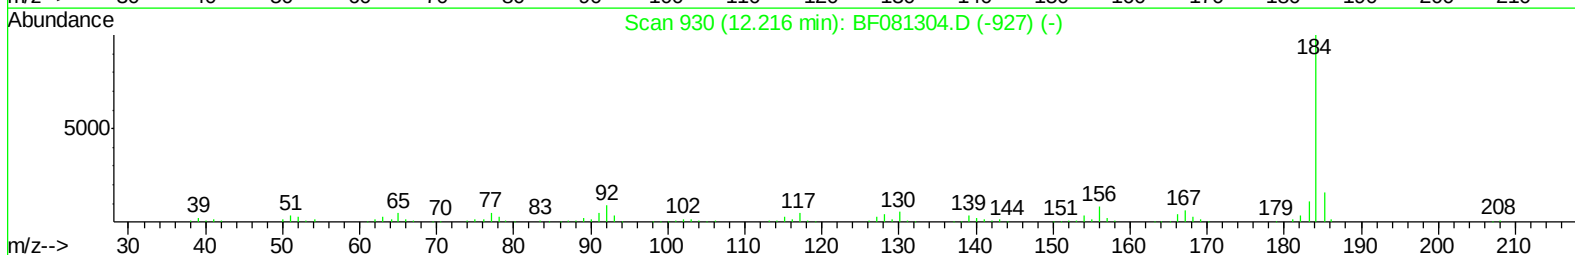
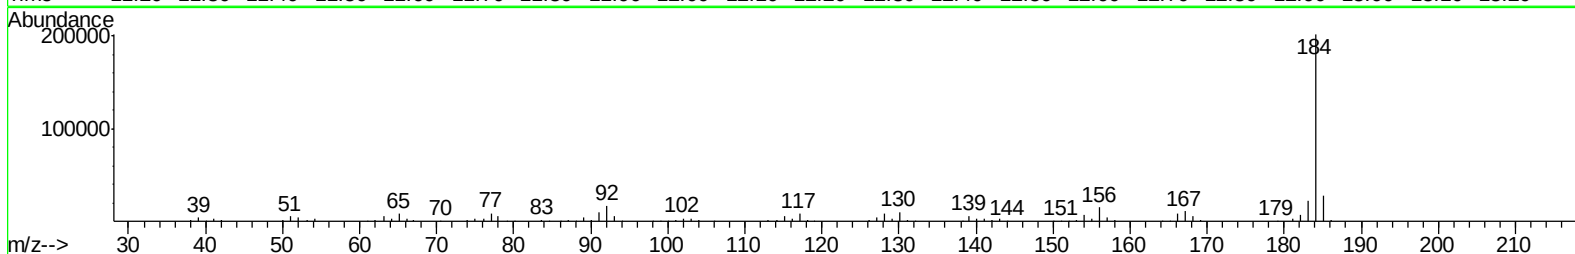


Data Path : Z:\HPCHEM1\BNA F\DATA\BF090115\
Data File : BF081299.D
Acq On : 1 Sep 2015 11:17
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 01 18:22:39 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF090115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 01 17:38:57 2015
Response via : Initial Calibration

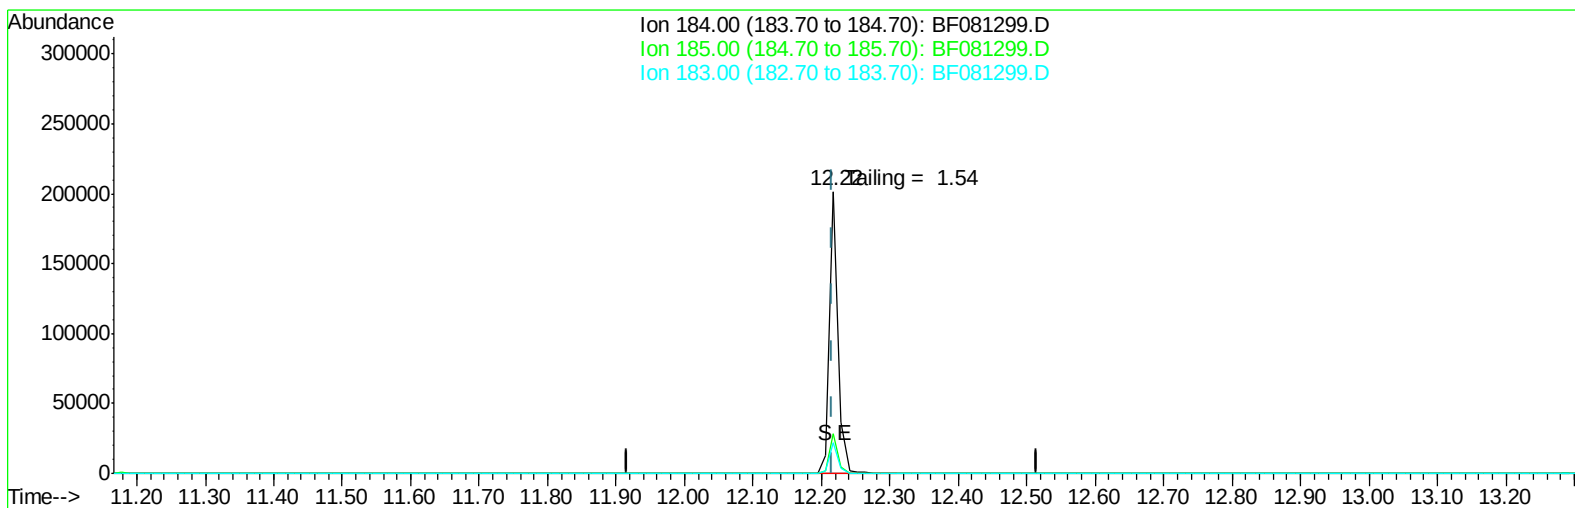

TIC: BF081299.D

(76) Benzidine




12.218min (+0.002) 0.00ng

response 175379

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	14.03
183.00	9.50	10.80
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF090115\
Data File : BF081299.D
Acq On : 1 Sep 2015 11:17
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 01 18:22:39 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF090115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 01 17:38:57 2015
Response via : Initial Calibration

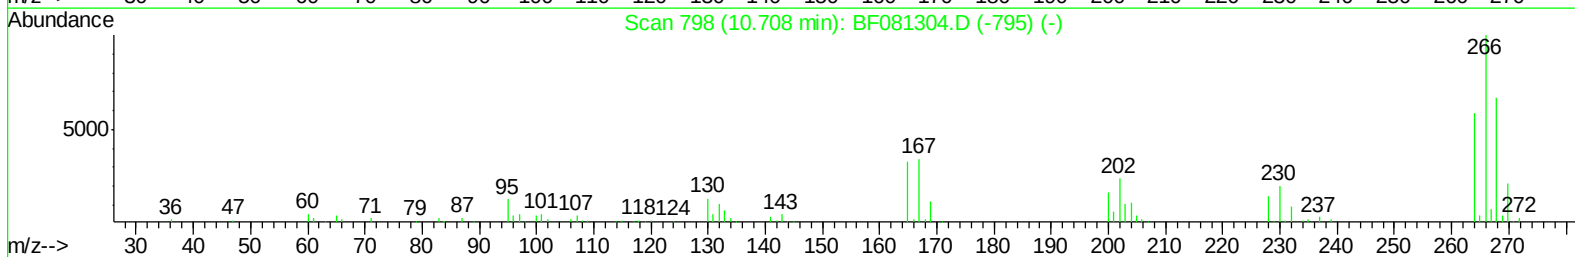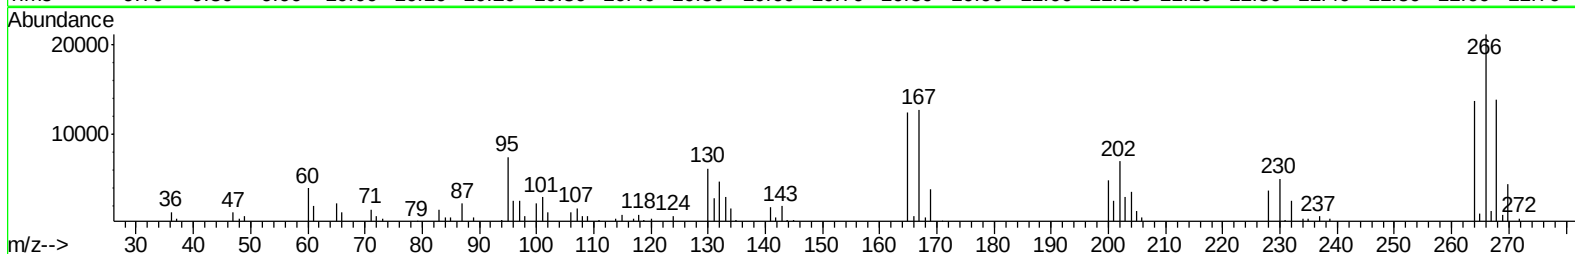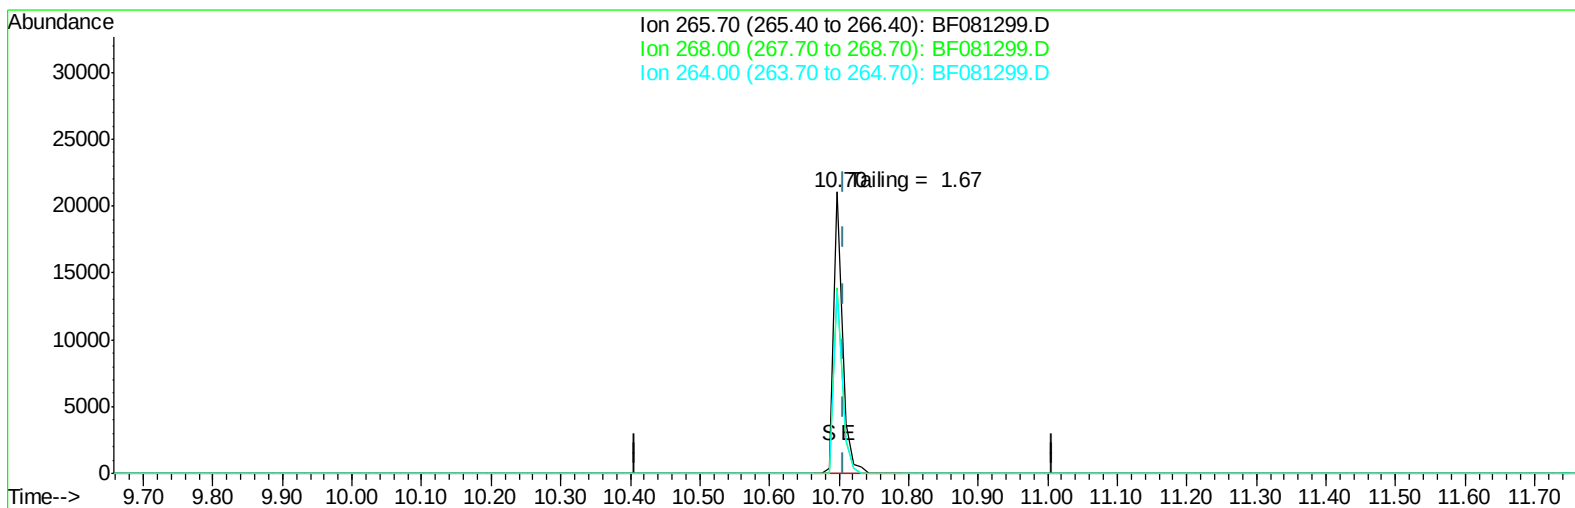

TIC: BF081299.D

(69) Pentachlorophenol (C)

10.698min (-0.009) 0.00ng

response 18056

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	65.75
264.00	62.70	65.18
0.00	0.00	0.00