


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF090115\
 Data File : BF081299.D
 Acq On : 1 Sep 2015 11:17
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF090115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 01 17:35:35 2015

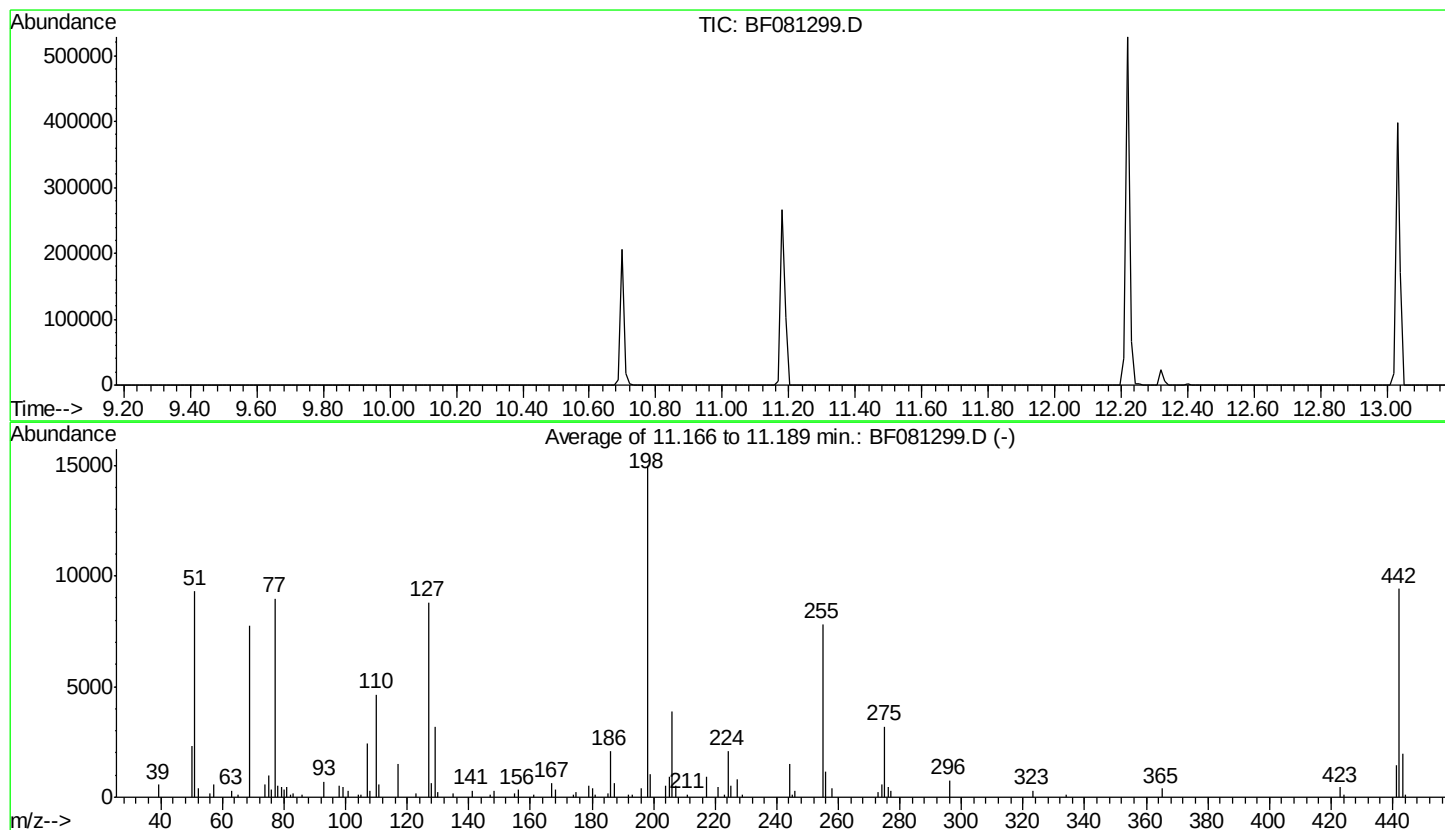

AutoFind: Scans 825, 826, 827; Background Corrected with Scan 822

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	62.3	9331	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	51.9	7777	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	58.7	8795	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	14984	PASS
199	198	5	9	6.8	1021	PASS
275	198	10	60	21.4	3203	PASS
365	198	1	100	2.5	379	PASS
441	442	0.01	24	15.5	1455	PASS
442	198	50	100	62.8	9415	PASS
443	442	15	24	20.8	1956	PASS