
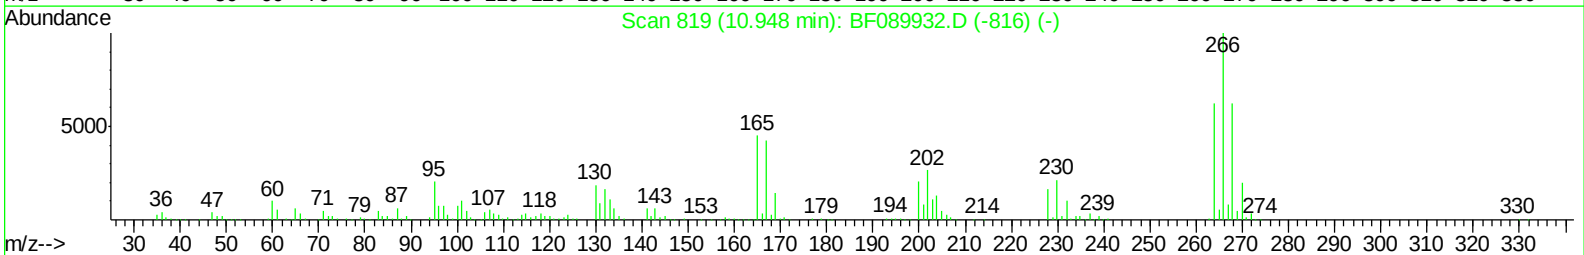
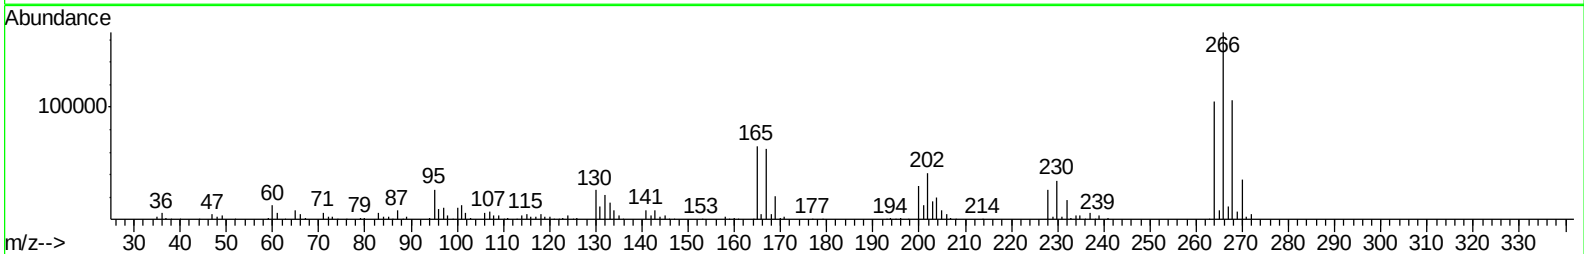


```
Data Path : Z:\HPCHEM1\BNA_F\Data\BF090116\  
Data File : BF089962.D  
Acq On    : 1 Sep 2016 10:24  
Operator  : UM/SJ  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1 Sample Multiplier: 1
```

Quant Time: Sep 02 05:54:28 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF083116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 31 11:55:18 2016
Response via : Initial Calibration

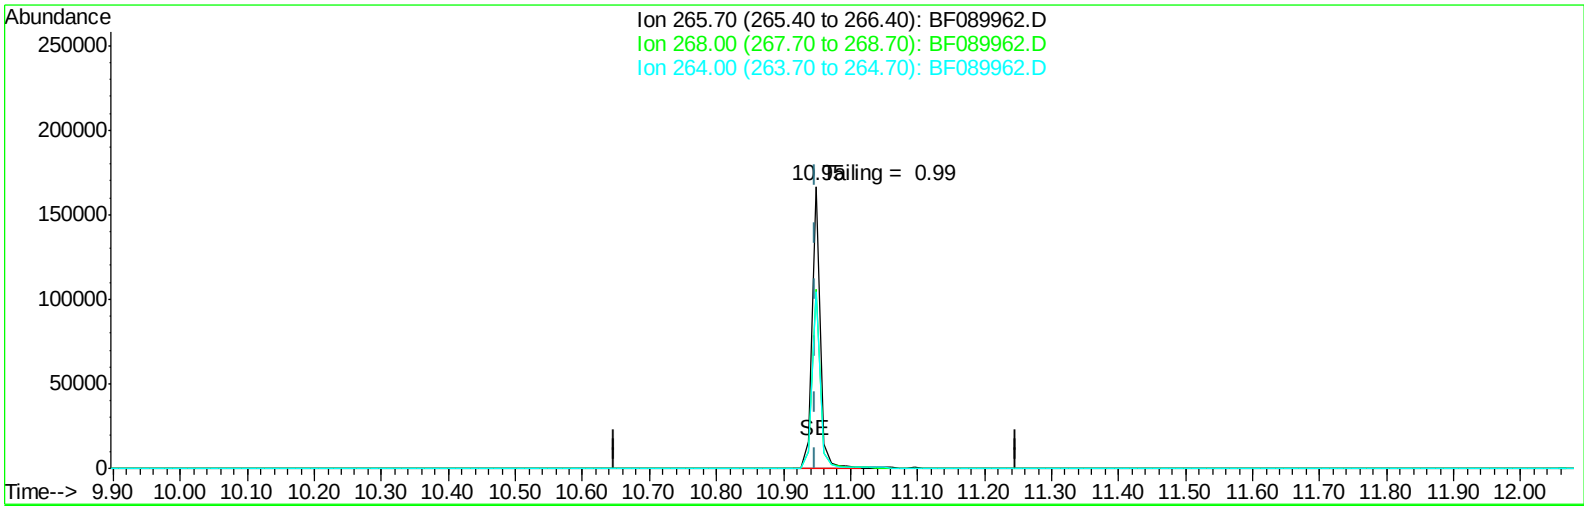

TIC: BF089962.D

(69) Pentachlorophenol (C)




10.948min (+0.001) 0.00ng

response 142589

Ion	Exp%	Act%
265.70	100	100
268.00	63.80	63.67
264.00	63.20	62.77
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF090116\
Data File : BF089962.D
Acq On : 1 Sep 2016 10:24
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 02 05:54:28 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF083116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 31 11:55:18 2016
Response via : Initial Calibration

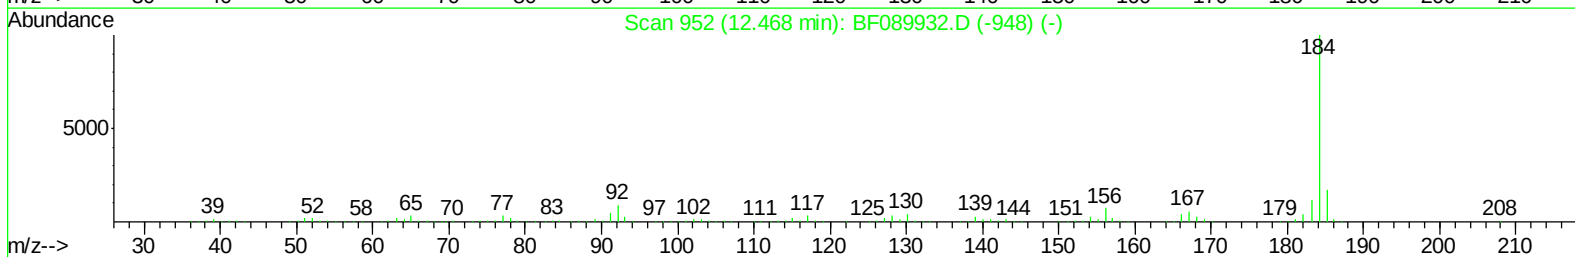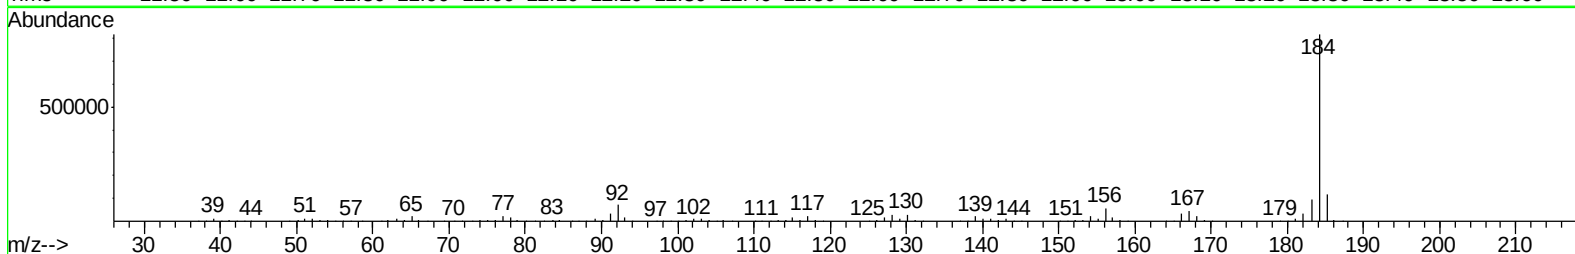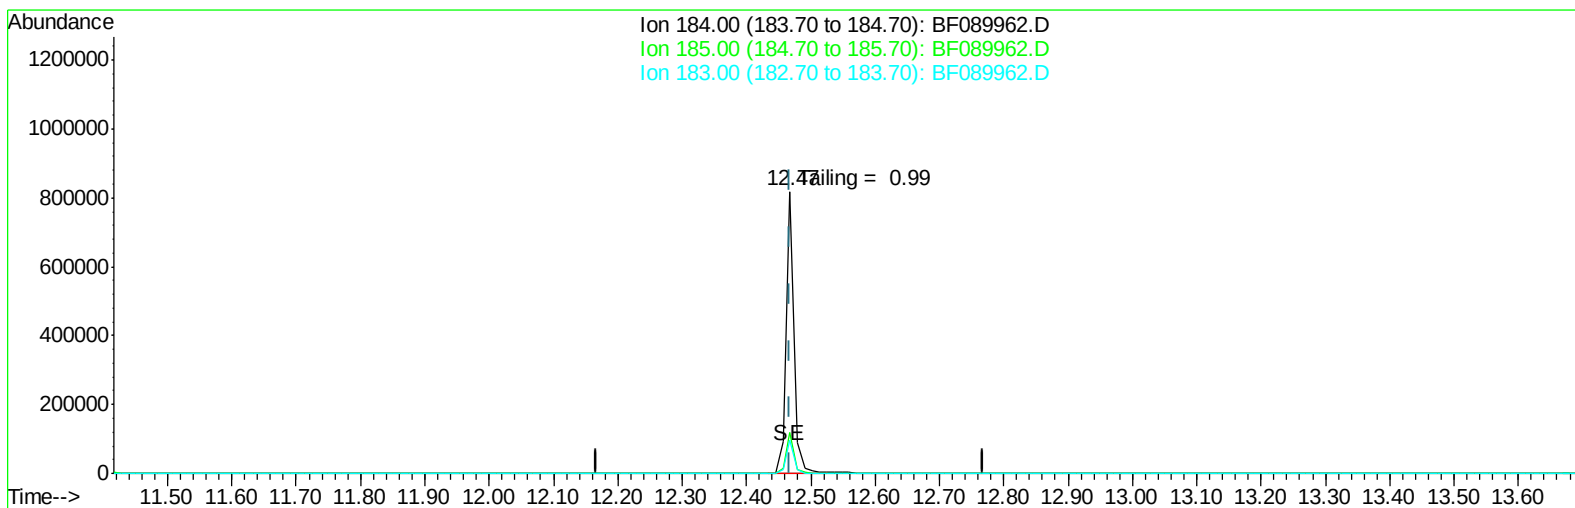

TIC: BF089962.D

(76) Benzidine

12.468min (+0.000) 11930.48ng

response 722690

Ion	Exp%	Act%
184.00	100	100
185.00	17.30	14.38
183.00	12.00	11.81
0.00	0.00	0.00