
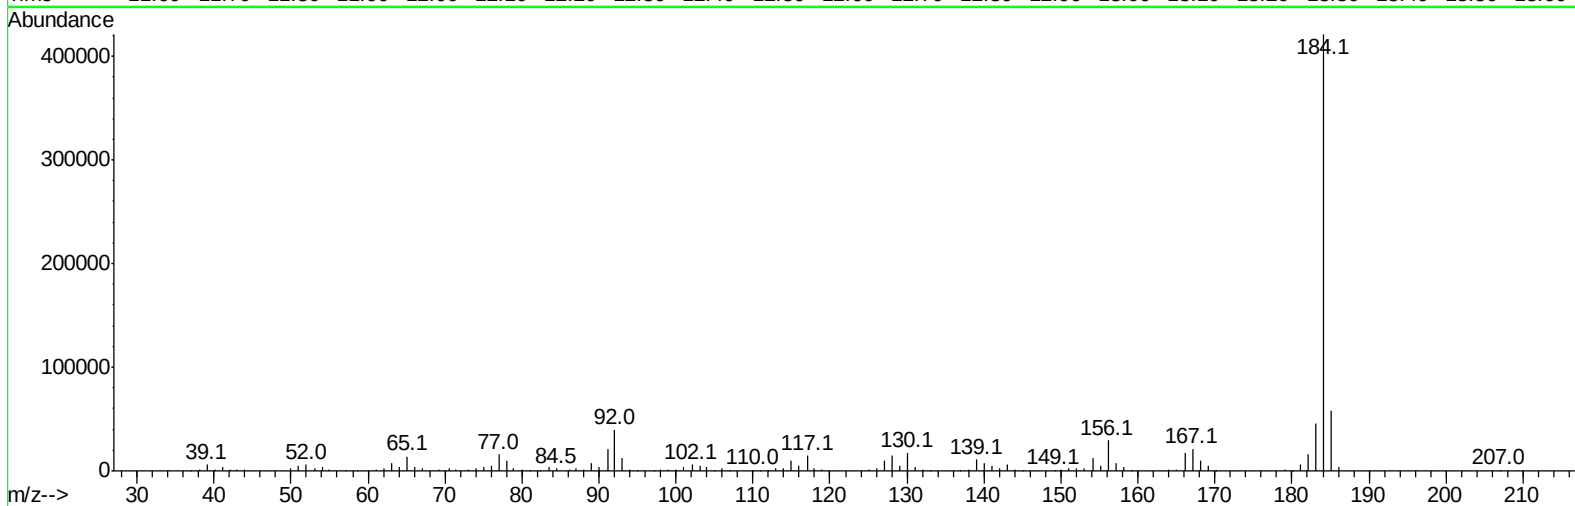


Data Path : Z:\HPCHEM1\BNA F\DATA\BF090117\  
Data File : BF098213.D  
Acq On : 1 Sep 2017 8:30  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 02 00:58:12 2017  
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Aug 21 15:59:04 2017  
Response via : Initial Calibration

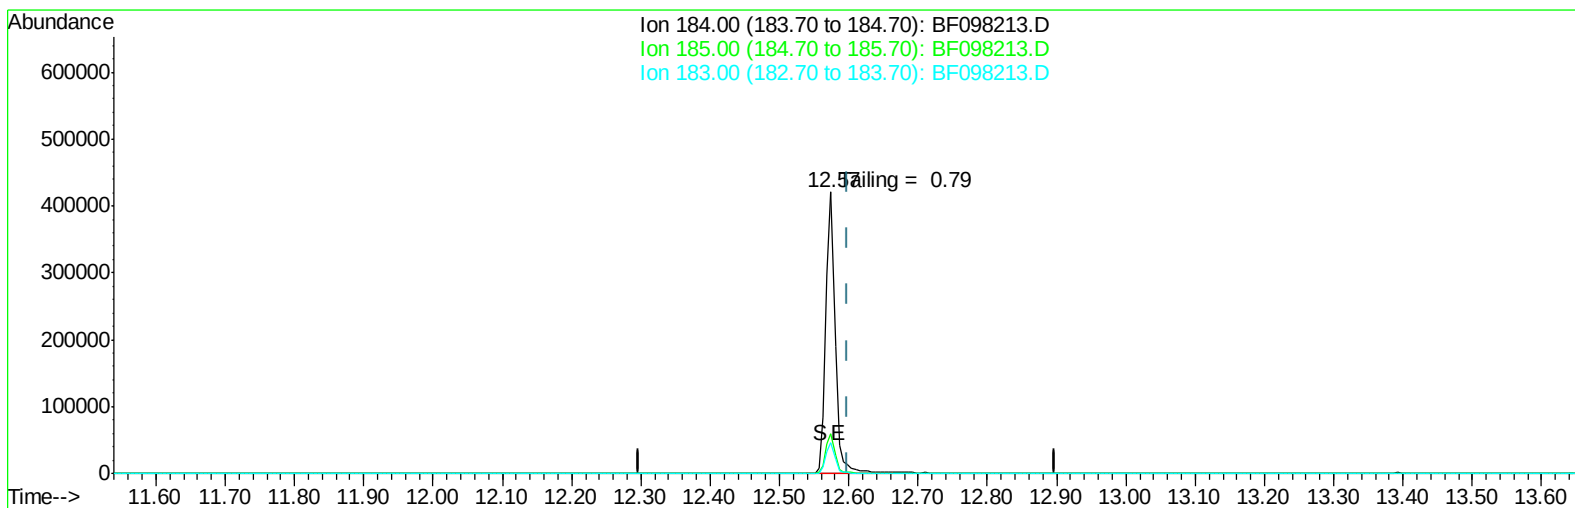

TIC: BF098213.D

(76) Benzidine



12.575min (-0.023) 3899.34ng

response 391990

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 184.00 | 100   | 100    |
| 185.00 | 19.40 | 13.89# |
| 183.00 | 12.20 | 10.79  |
| 0.00   | 0.00  | 0.00   |

Data Path : Z:\HPCHEM1\BNA F\DATA\BF090117\  
Data File : BF098213.D  
Acq On : 1 Sep 2017 8:30  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 02 00:58:12 2017  
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Aug 21 15:59:04 2017  
Response via : Initial Calibration

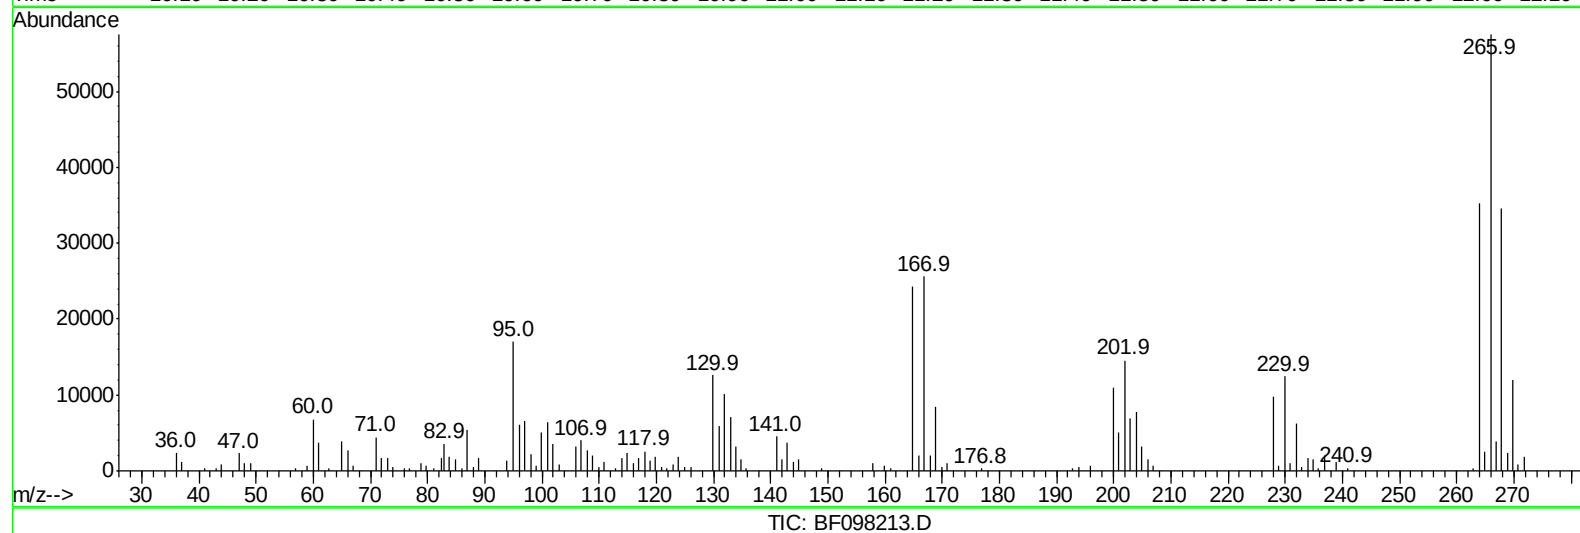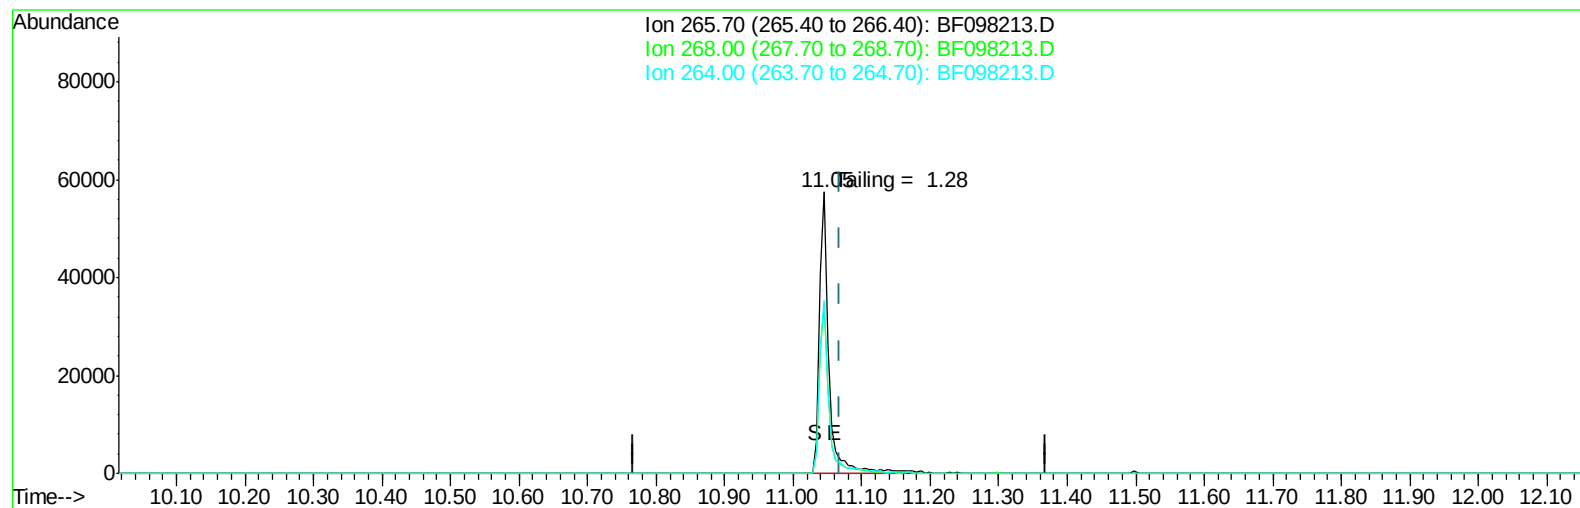

TIC: BF098213.D

(69) Pentachlorophenol (C)

11.045min (-0.023) 59529.42ng

response 56943

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 63.90 | 60.14 |
| 264.00 | 64.60 | 61.29 |
| 0.00   | 0.00  | 0.00  |