

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF090117\
 Data File : BF098240.D
 Acq On : 1 Sep 2017 21:27
 Operator : SJ/JU
 Sample : I5048-02
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OILY-RAGS-DEBRIS

Quant Time: Sep 02 00:10:51 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 21 15:59:04 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.72	152	110292	20.00	ng	-0.04
21) Naphthalene-d8	8.00	136	423446	20.00	ng	-0.03
38) Acenaphthene-d10	9.75	164	155180	20.00	ng	-0.04
63) Phenanthrene-d10	11.23	188	237368	20.00	ng	-0.03
75) Chrysene-d12	13.87	240	239483	20.00	ng	-0.03
86) Perylene-d12	15.28	264	173058	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.34	112	708407	97.70	ng	-0.01
7) Phenol-d6	6.37	99	1054804	107.07	ng	-0.02
23) Nitrobenzene-d5	7.29	82	709724	91.05	ng	-0.04
41) 2,4,6-Tribromophenol	10.54	330	109671	81.45	ng	-0.04
44) 2-Fluorobiphenyl	9.08	172	1006033	95.25	ng	-0.03
78) Terphenyl-d14	12.82	244	672265	58.54	ng	-0.03
Target Compounds						Qvalue
49) Dimethylphthalate	9.47	163	118693	10.464	ng	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA F\DATA\BF090117\
Data File : BF098240.D
Acq On : 1 Sep 2017 21:27
Operator : SJ/JU
Sample : I5048-02
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OILY-RAGS-DEBRIS

Quant Time: Sep 02 00:10:51 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 21 15:59:04 2017
Response via : Initial Calibration

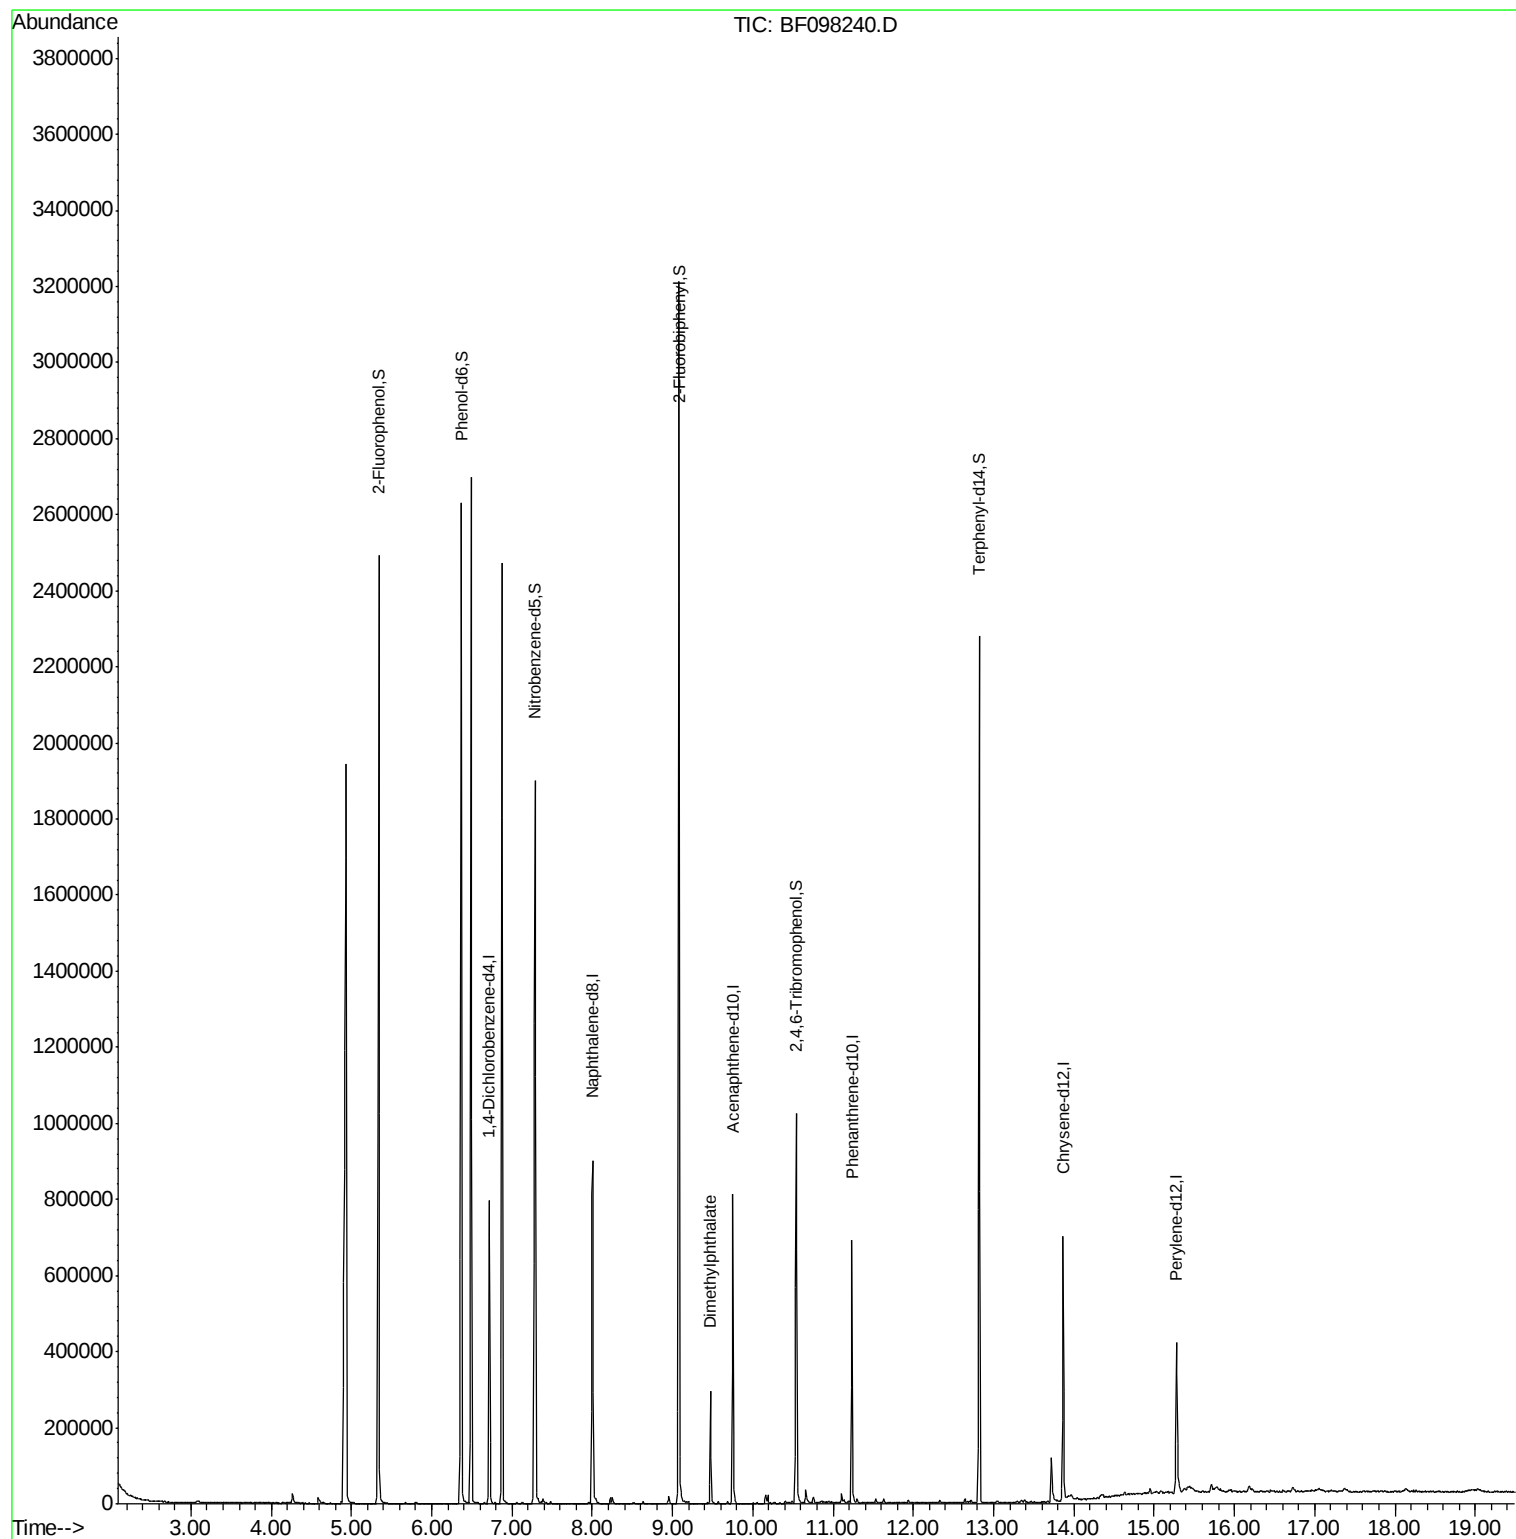




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.72 min Scan# 787
Delta R.T. -0.04 min
Lab File: BF098240.D
Acq: 1 Sep 2017 21:27

Instrument :
BNA_F
ClientSampleId :
OILY-RAGS-DEBRIS

Tot Ion:152 Resp: 110292
Ion Ratio Lower Upper
152 100
150 158.3 126.2 189.2
115 67.2 52.2 78.2

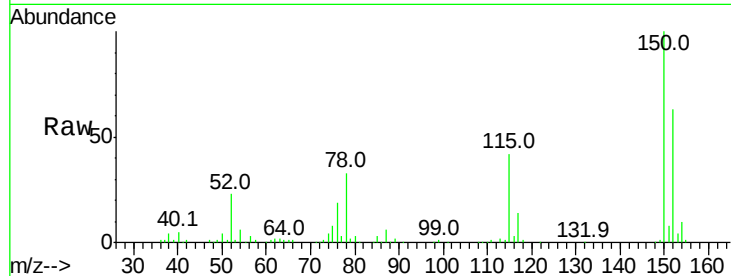


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

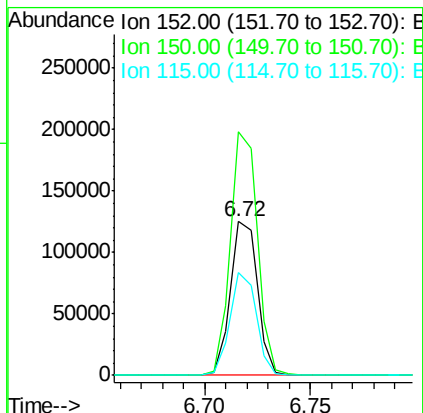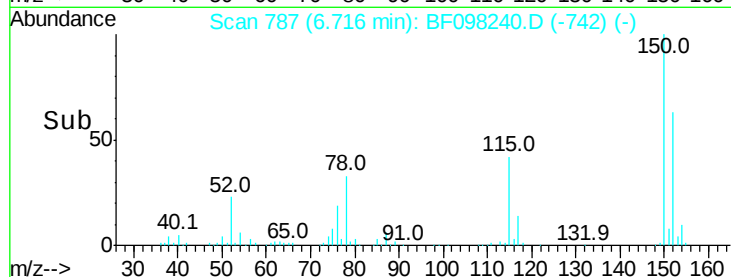



#5


2-Fluorophenol
Concen: 97.699 ng
RT: 5.34 min Scan# 553
Delta R.T. -0.01 min
Lab File: BF098240.D
Acq: 1 Sep 2017 21:27

Tgt Ion:112 Resp: 708407
Ion Ratio Lower Upper
112 100
64 58.4 46.0 69.0
63 29.3 23.4 35.0



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

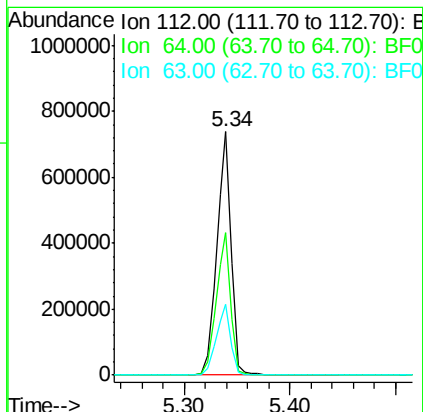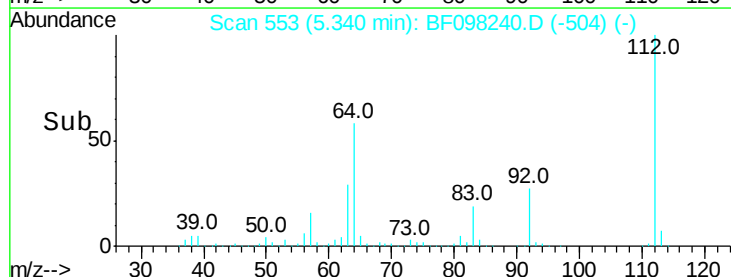

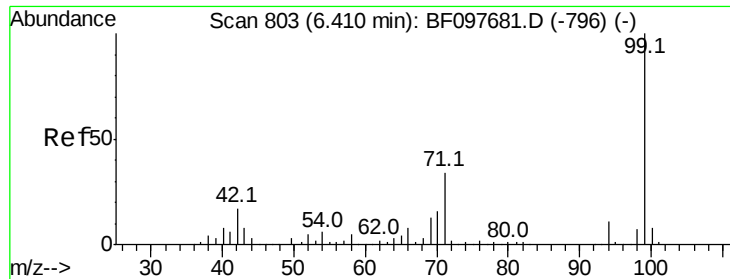

#7

Phenol-d6

Concen: 107.066 ng

RT: 6.37 min Scan# 728

Delta R.T. -0.02 min

Lab File: BF098240.D

Acq: 1 Sep 2017 21:27

Instrument :

BNA_F

ClientSampleId :

OILY-RAGS-DEBRIS


Tot Ion: 99 Resp: 1054804

Ion Ratio Lower Upper

99 100

42 14.5 13.5 20.3




71 31.6 24.5 36.7

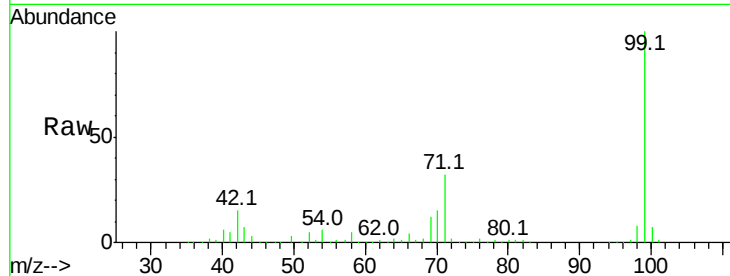

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

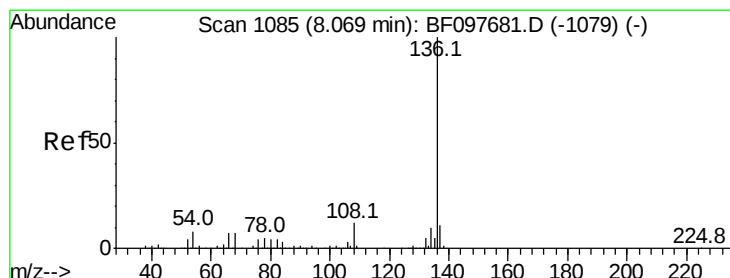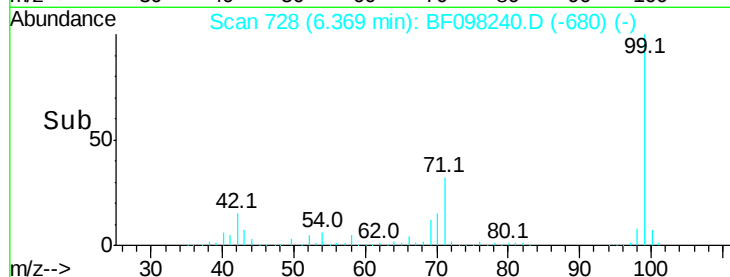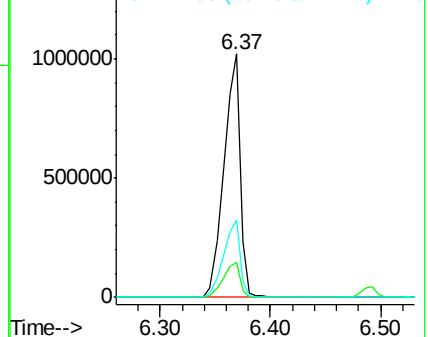

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.00 min Scan# 1006

Delta R.T. -0.03 min

Lab File: BF098240.D

Acq: 1 Sep 2017 21:27

Tgt Ion: 136 Resp: 423446


Ion Ratio Lower Upper

136 100

137 10.7 8.5 12.7

54 7.3 4.9 7.3

68 6.6 4.1 6.1#


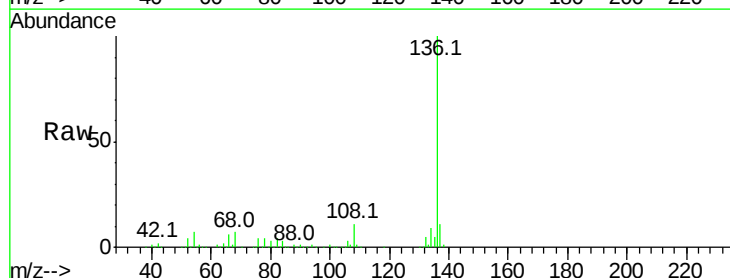


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0



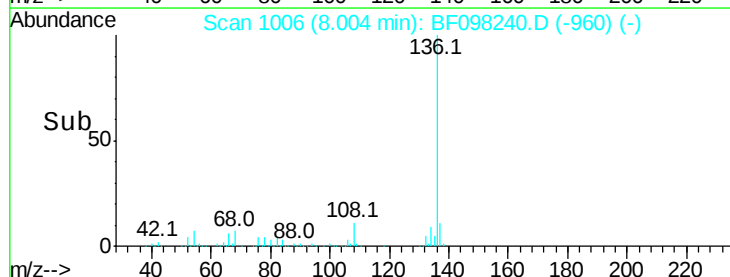
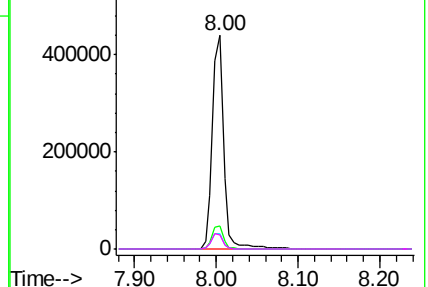




#23
 Nitrobenzene-d5
 Concen: 91.052 ng
 RT: 7.29 min Scan# 884
 Delta R.T. -0.04 min
 Lab File: BF098240.D
 Acq: 1 Sep 2017 21:27




Instrument :
 BNA_F
 ClientSampleId :
 OILY-RAGS-DEBRIS

Tot Ion: 82 Resp: 709724
 Ion Ratio Lower Upper
 82 100
 128 39.3 34.0 51.0
 54 40.6 42.2 63.2#

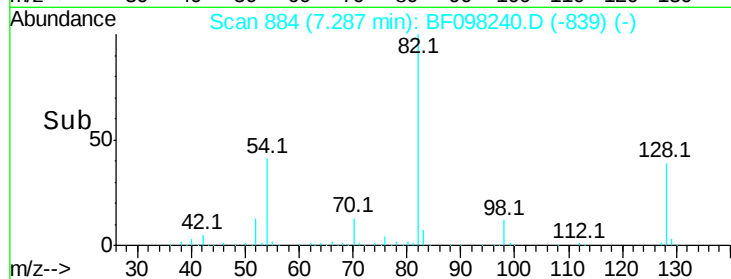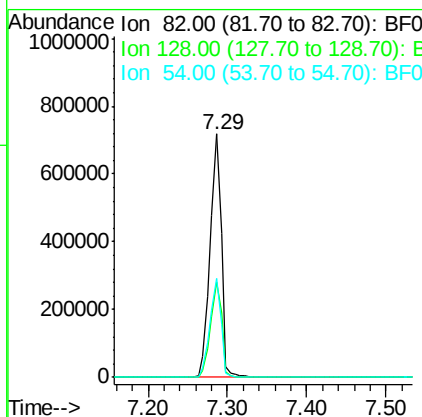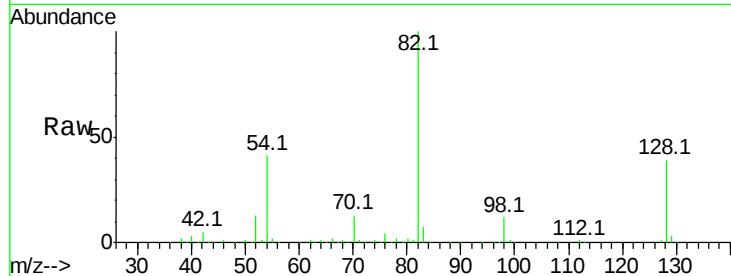

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.75 min Scan# 1303
 Delta R.T. -0.04 min
 Lab File: BF098240.D
 Acq: 1 Sep 2017 21:27

Tgt Ion:164 Resp: 155180
 Ion Ratio Lower Upper
 164 100
 162 101.5 82.6 123.8
 160 46.8 36.2 54.2

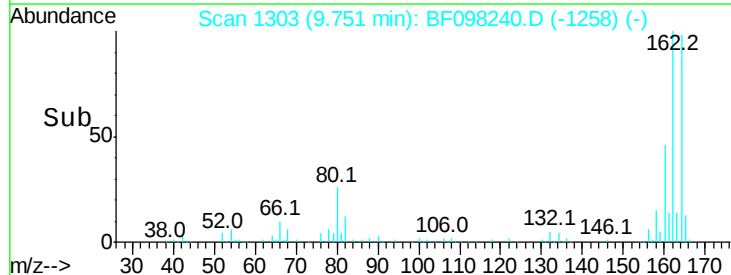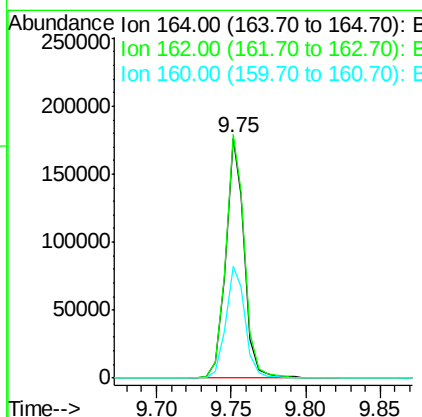







#41
 2,4,6-Tribromophenol
 Concen: 81.453 ng
 RT: 10.54 min Scan# 1437
 Delta R.T. -0.04 min
 Lab File: BF098240.D
 Acq: 1 Sep 2017 21:27

Instrument :
 BNA_F
 ClientSampleId :
 OILY-RAGS-DEBRIS

Tot Ion:330 Resp: 109671
 Ion Ratio Lower Upper
 330 100
 332 95.6 76.6 115.0
 141 38.0 31.4 47.2




Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

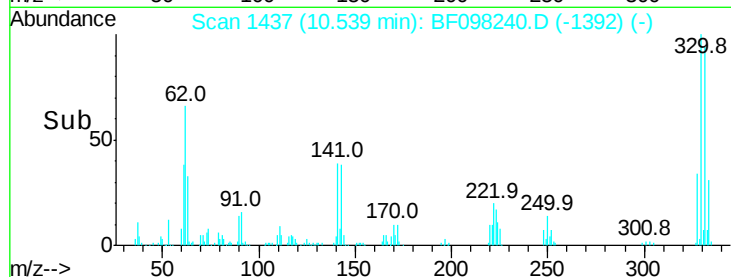
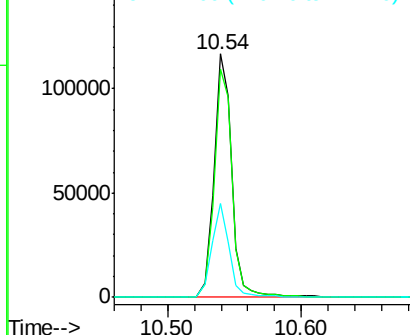



#44
 2-Fluorobiphenyl
 Concen: 95.249 ng
 RT: 9.08 min Scan# 1189
 Delta R.T. -0.03 min
 Lab File: BF098240.D
 Acq: 1 Sep 2017 21:27

Tgt Ion:172 Resp: 1006033
 Ion Ratio Lower Upper
 172 100
 171 36.0 29.6 44.4
 170 24.4 19.8 29.8



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

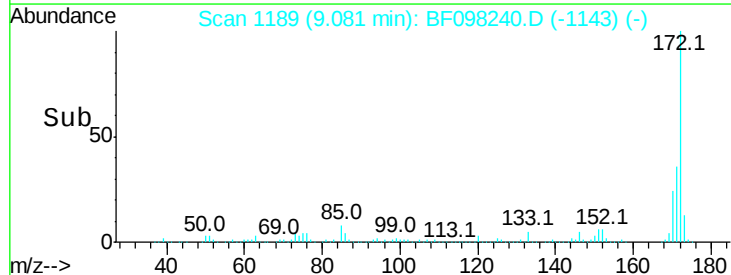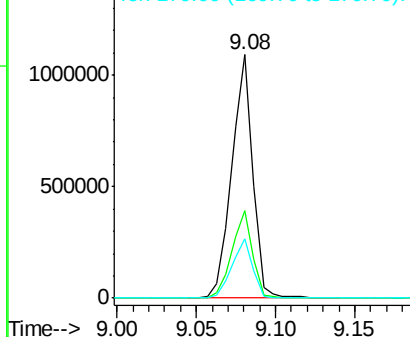


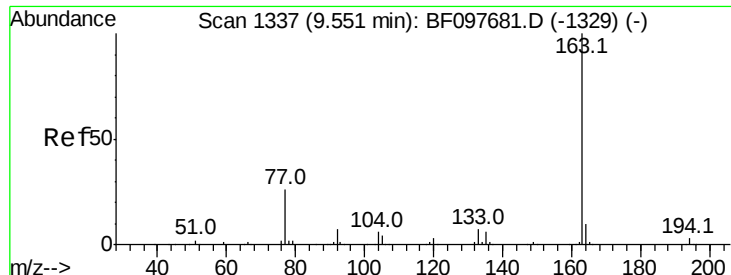




#49
Dimethylphthalate
Concen: 10.464 ng
RT: 9.47 min Scan# 1256
Delta R.T. -0.04 min
Lab File: BF098240.D
Acq: 1 Sep 2017 21:27

Instrument :
BNA_F
ClientSampleId :
OILY-RAGS-DEBRIS

Tot Ion:163 Resp: 118693
Ion Ratio Lower Upper
163 100
194 3.5 2.6 4.0
164 9.6 8.4 12.6

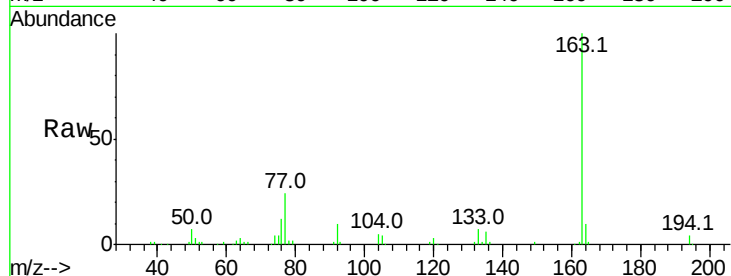


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

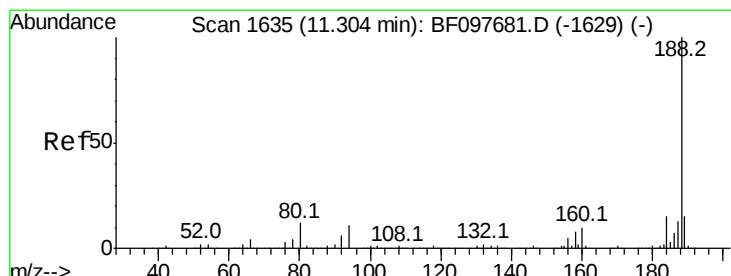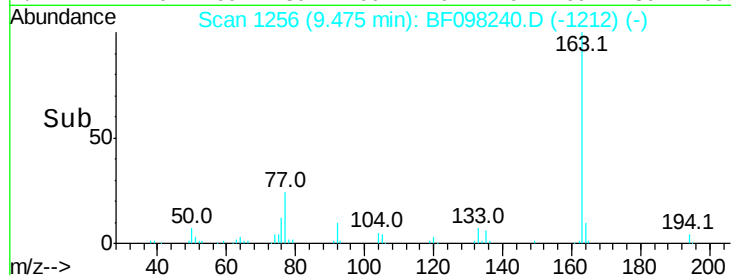
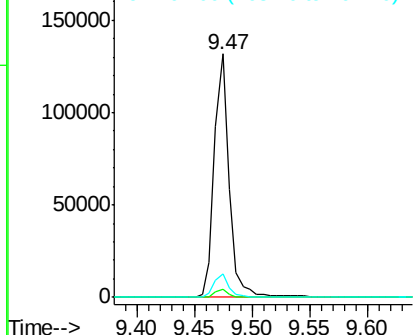



#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.23 min Scan# 1555
Delta R.T. -0.03 min
Lab File: BF098240.D
Acq: 1 Sep 2017 21:27

Tgt Ion:188 Resp: 237368
Ion Ratio Lower Upper
188 100
94 12.1 9.4 14.2
80 13.2 10.2 15.2

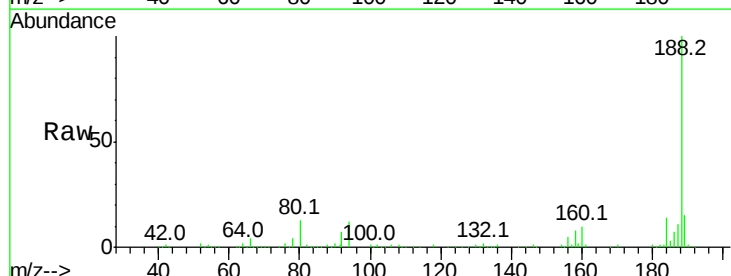

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

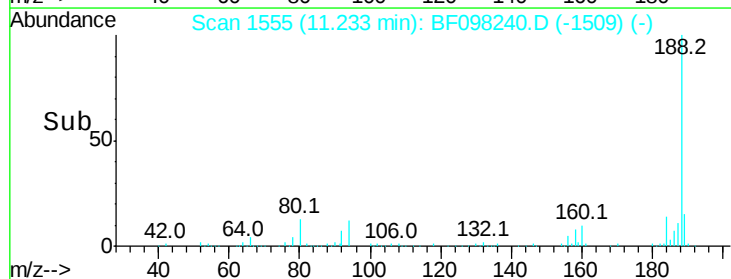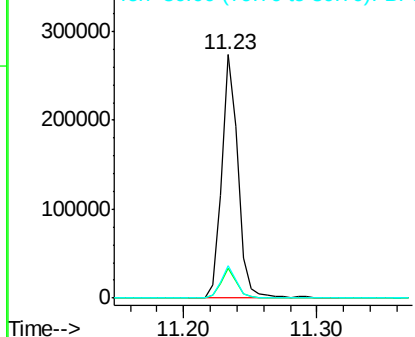

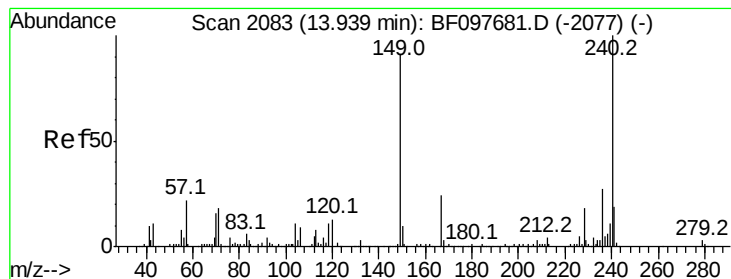

#75

Chrysene-d12

Concen: 20.000 ng

RT: 13.87 min Scan# 2003

Delta R.T. -0.03 min

Lab File: BF098240.D

Acq: 1 Sep 2017 21:27

Instrument :

BNA_F

ClientSampleId :

OILY-RAGS-DEBRIS


Tot Ion:240 Resp: 239483

Ion Ratio Lower Upper

240 100

120 12.2 5.8 8.8#



236 26.1 20.5 30.7



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

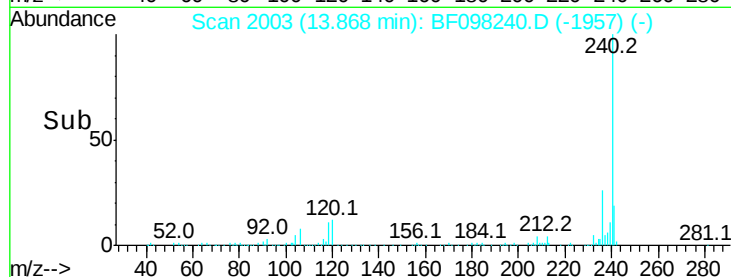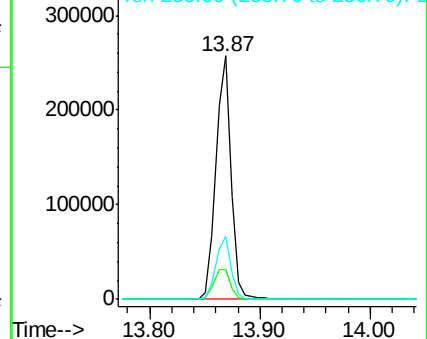

#78

Terphenyl-d14

Concen: 58.539 ng

RT: 12.82 min Scan# 1825

Delta R.T. -0.03 min

Lab File: BF098240.D

Acq: 1 Sep 2017 21:27


Tgt Ion:244 Resp: 672265

Ion Ratio Lower Upper

244 100

212 7.2 6.0 9.0



122 12.8 10.3 15.5




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

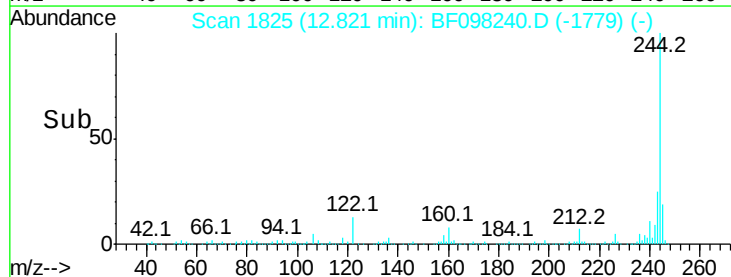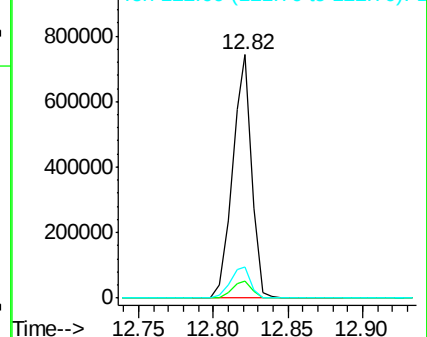


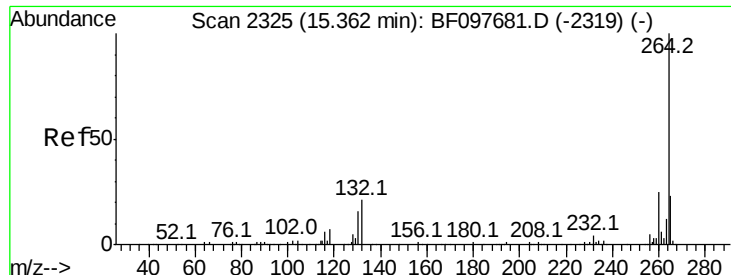

#86
Pervlene-d12
Concen: 20.000 ng
RT: 15.28 min Scan# 2243
Delta R.T. -0.03 min
Lab File: BF098240.D
Acq: 1 Sep 2017 21:27

Instrument :
BNA_F
ClientSampleId :
OILY-RAGS-DEBRIS

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.1	19.5	29.3
265	21.4	17.2	25.8



Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

