


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA F\Data\BF090117\
 Data File : BF098238.D
 Acq On : 1 Sep 2017 20:32
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 21 15:59:04 2017

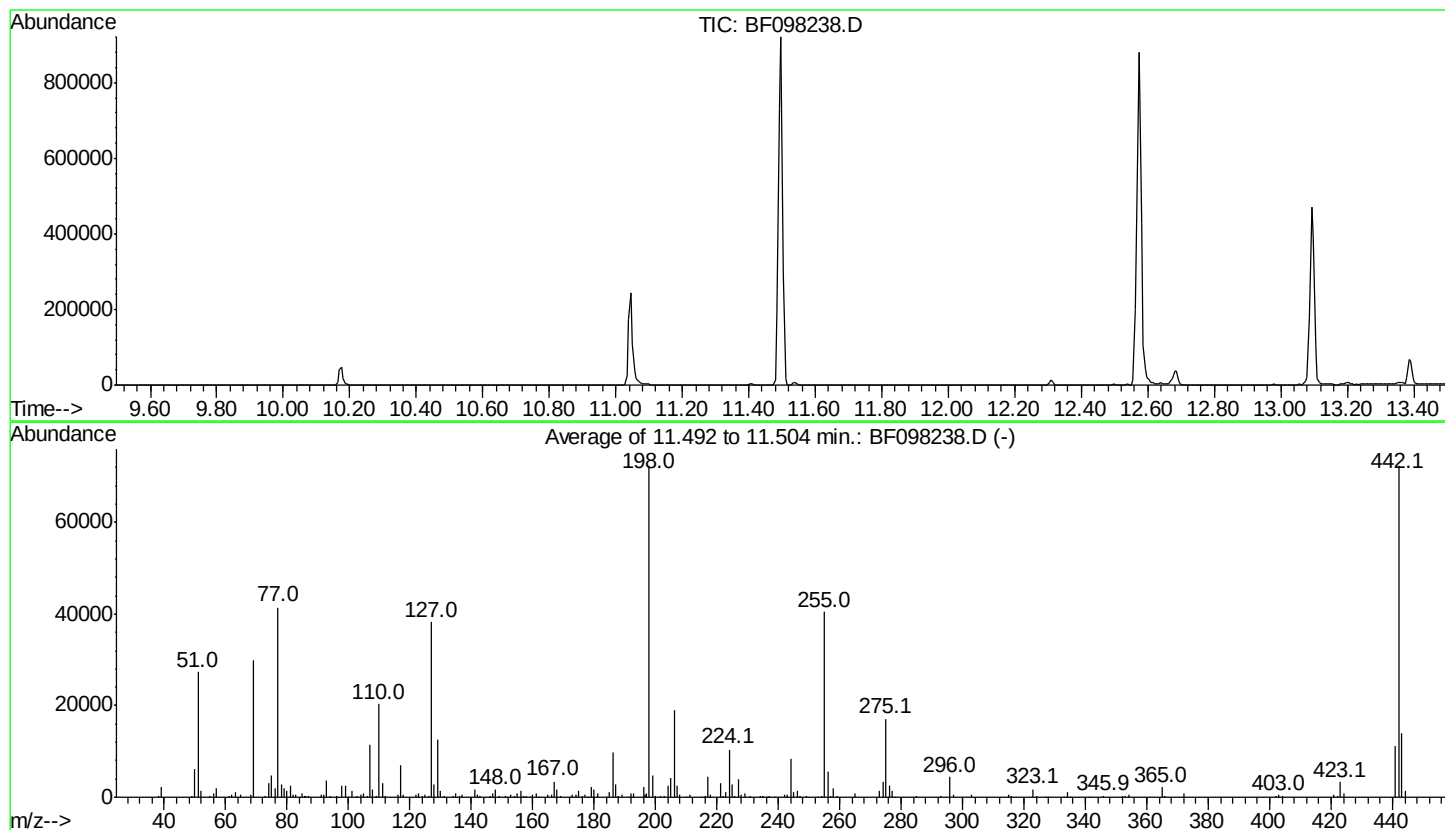

AutoFind: Scans 1599, 1600, 1601; Background Corrected with Scan 1594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.7	27256	PASS
68	69	0.00	2	1.6	466	PASS
69	198	0.00	100	41.3	29877	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.8	38188	PASS
197	198	0.00	2	1.0	716	PASS
198	198	100	100	100.0	72384	PASS
199	198	5	9	6.7	4870	PASS
275	198	10	60	23.7	17171	PASS
365	198	1	100	3.1	2219	PASS
441	442	0.01	24	15.3	11051	PASS
442	198	50	100	99.8	72269	PASS
443	442	15	24	19.4	13986	PASS