
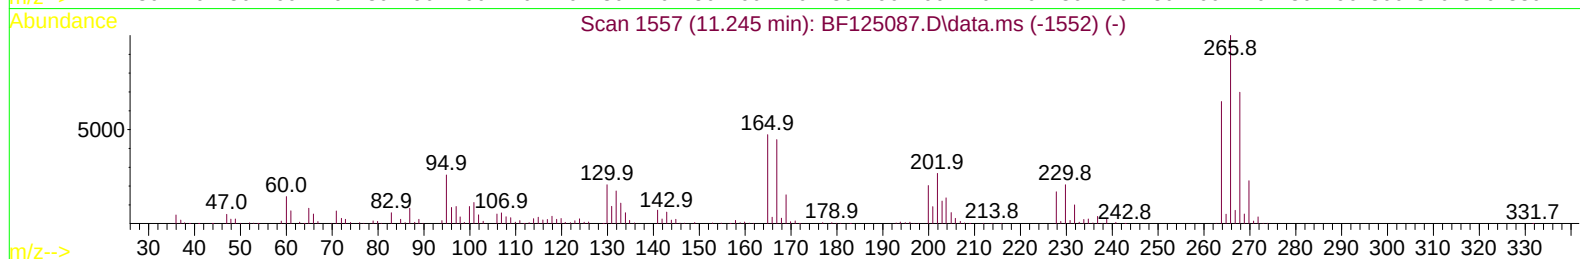
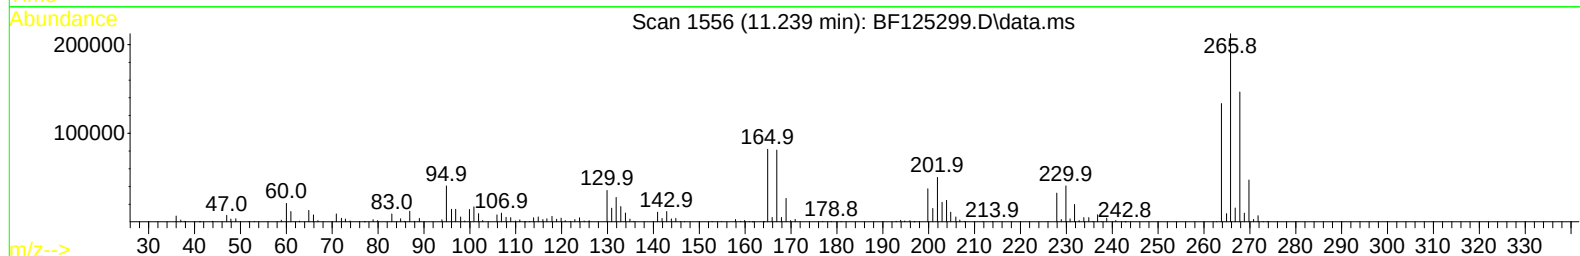


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090121\
 Data File : BF125299.D
 Acq On : 1 Sep 2021 11:04
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 01 13:23:31 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 24 12:39:21 2021
 Response via : Initial Calibration

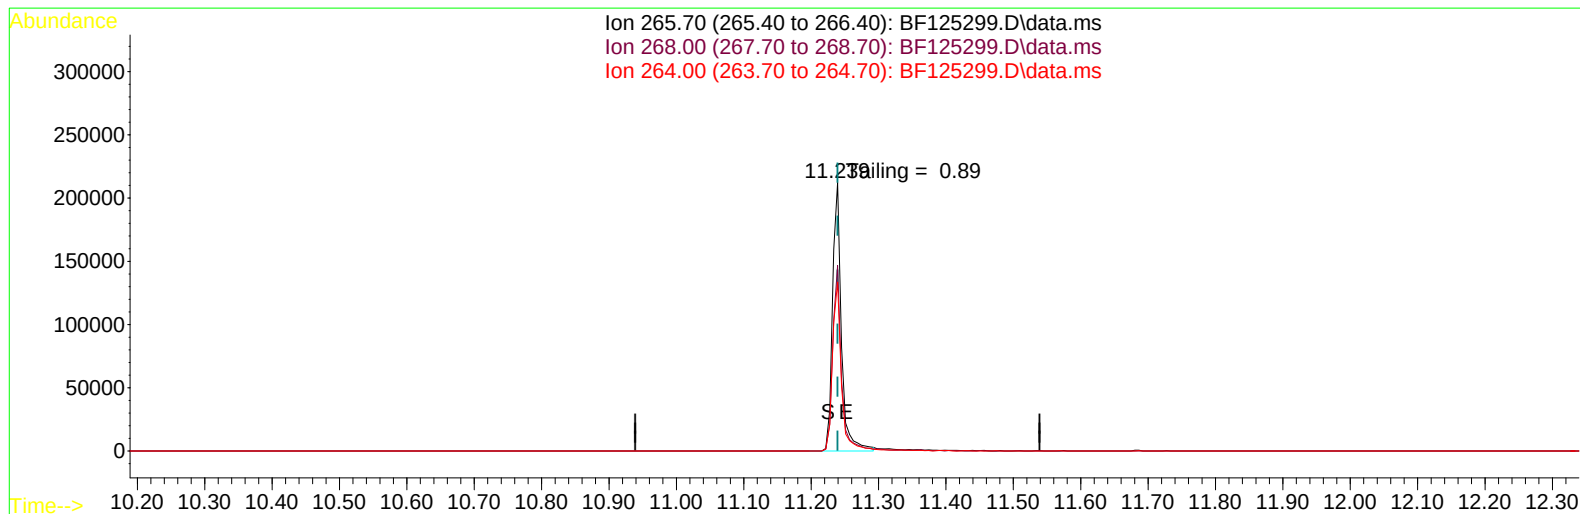

TIC: BF125299.D\data.ms

(70) Pentachlorophenol (C)




11.239min (+ 0.000) 30794.74 ng

response 199023

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	69.09
264.00	69.90	62.94
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090121\
Data File : BF125299.D
Acq On : 1 Sep 2021 11:04
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 01 13:23:31 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 24 12:39:21 2021
Response via : Initial Calibration

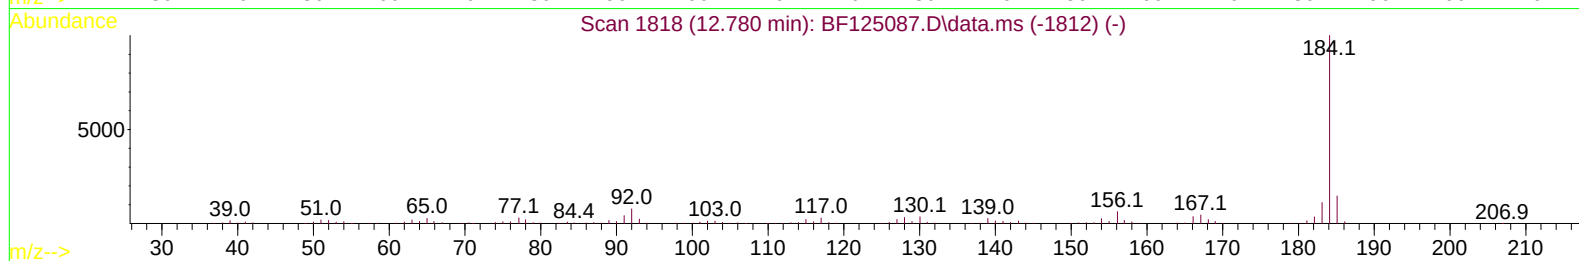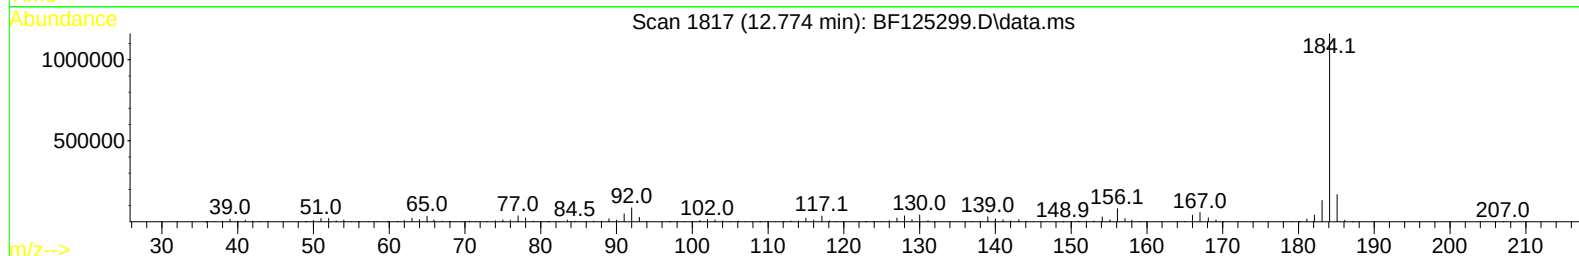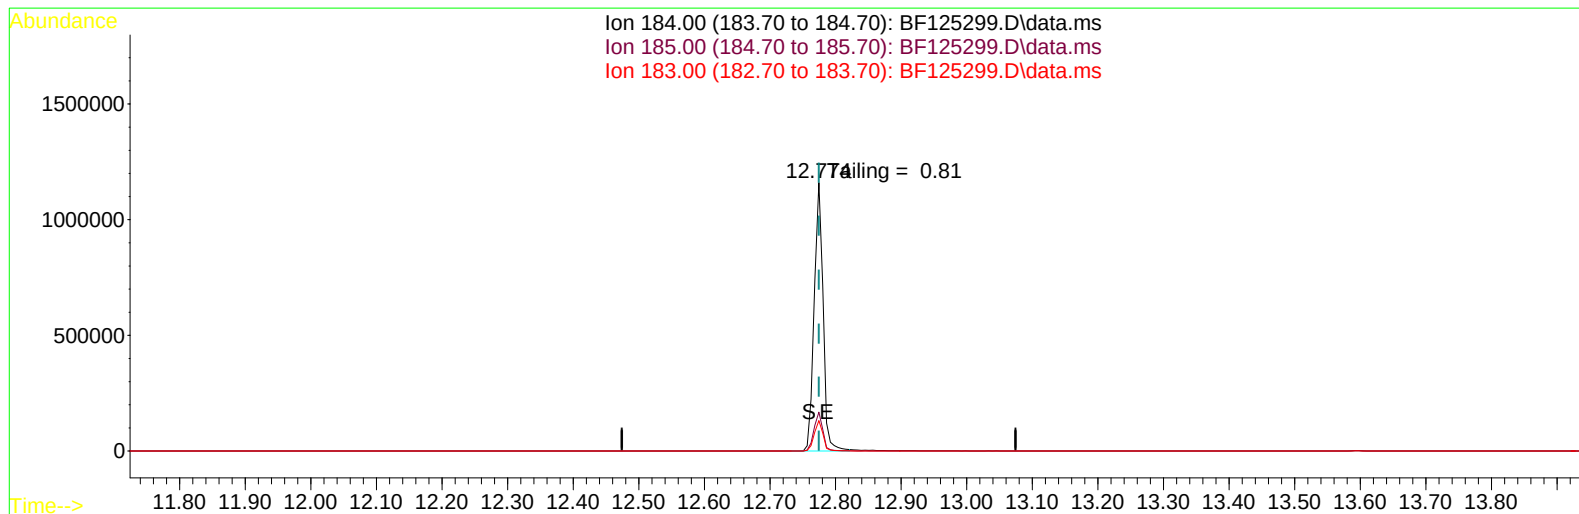

TIC: BF125299.D\data.ms

(77) Benzidine

12.774min (+ 0.000) 0.00 ng

response 1105864

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.53
183.00	10.10	11.36
0.00	0.00	0.00