

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090121\
 Data File : BF125301.D
 Acq On : 1 Sep 2021 12:08
 Operator : JU/CG
 Sample : PB138856BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB138856BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF125301.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.240	20	26	30	rBV	144072	180118	2.54%	0.434%
2	5.534	581	586	589	rBV	4926907	5457006	77.07%	13.153%
3	6.540	751	757	760	rBV	4674375	5322699	75.17%	12.829%
4	6.904	816	819	823	rBV	1471400	1218058	17.20%	2.936%
5	7.469	910	915	919	rBV	3066216	3530983	49.87%	8.511%
6	8.192	1033	1038	1041	rBV	1685746	1623667	22.93%	3.914%
7	9.269	1215	1221	1224	rBV	6244253	6058494	85.56%	14.603%
8	9.945	1331	1336	1346	rBV	2209684	1864262	26.33%	4.493%
9	10.739	1466	1471	1474	rBV	4483056	4146661	58.56%	9.995%
10	11.433	1585	1589	1596	rBV	2177361	1994865	28.17%	4.808%
11	13.027	1854	1860	1863	rBV	6837086	7080595	100.00%	17.066%
12	13.945	2012	2016	2021	rVB	98349	113877	1.61%	0.274%
13	14.074	2034	2038	2047	rVB	1659748	1610876	22.75%	3.883%
14	15.574	2287	2293	2302	rBV2	873482	1207350	17.05%	2.910%
15	17.268	2573	2581	2589	rBV7	22157	78968	1.12%	0.190%




Sum of corrected areas: 41488479

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090121\
Data File : BF125301.D
Acq On : 1 Sep 2021 12:08
Operator : JU/CG
Sample : PB138856BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB138856BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

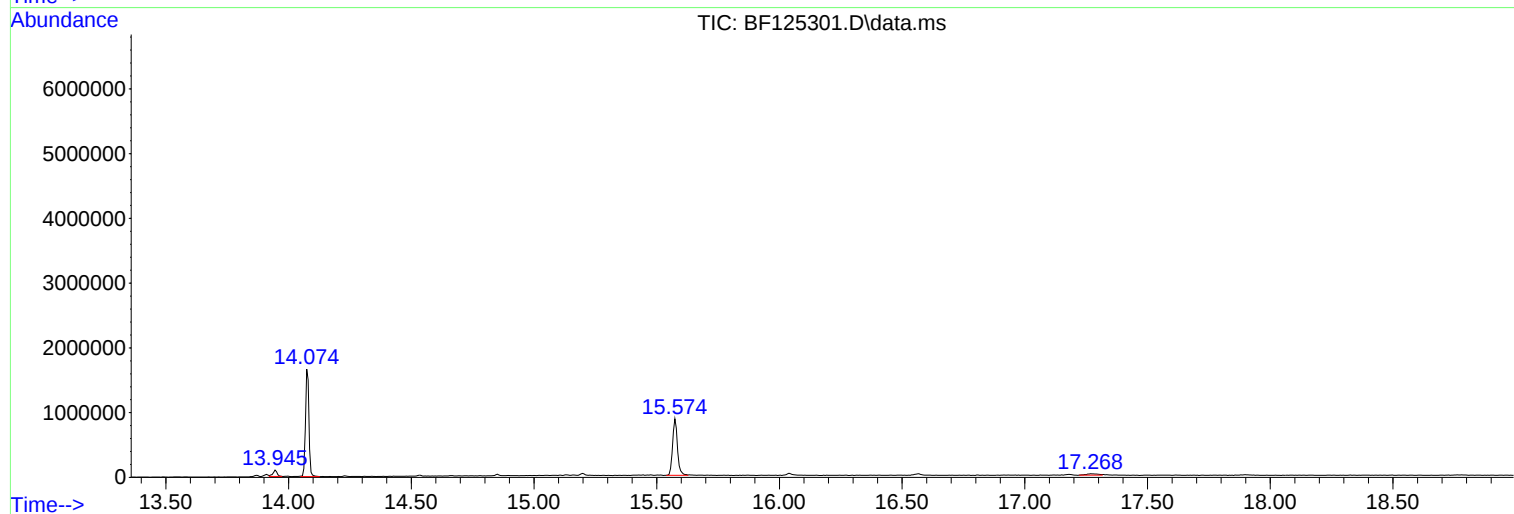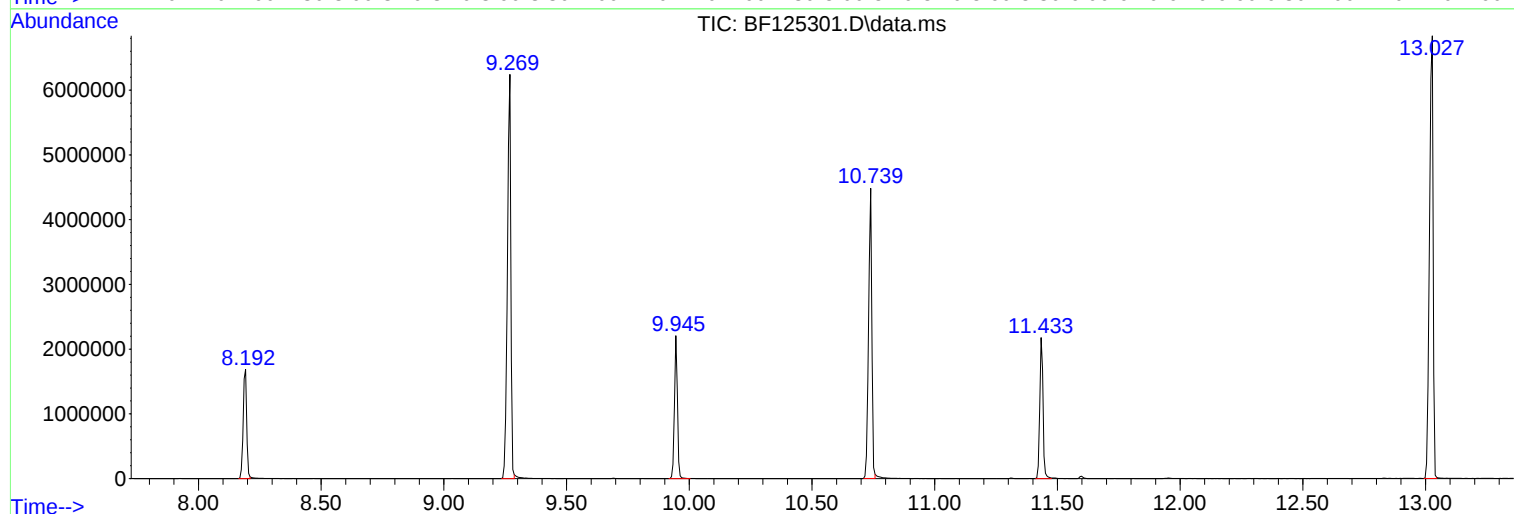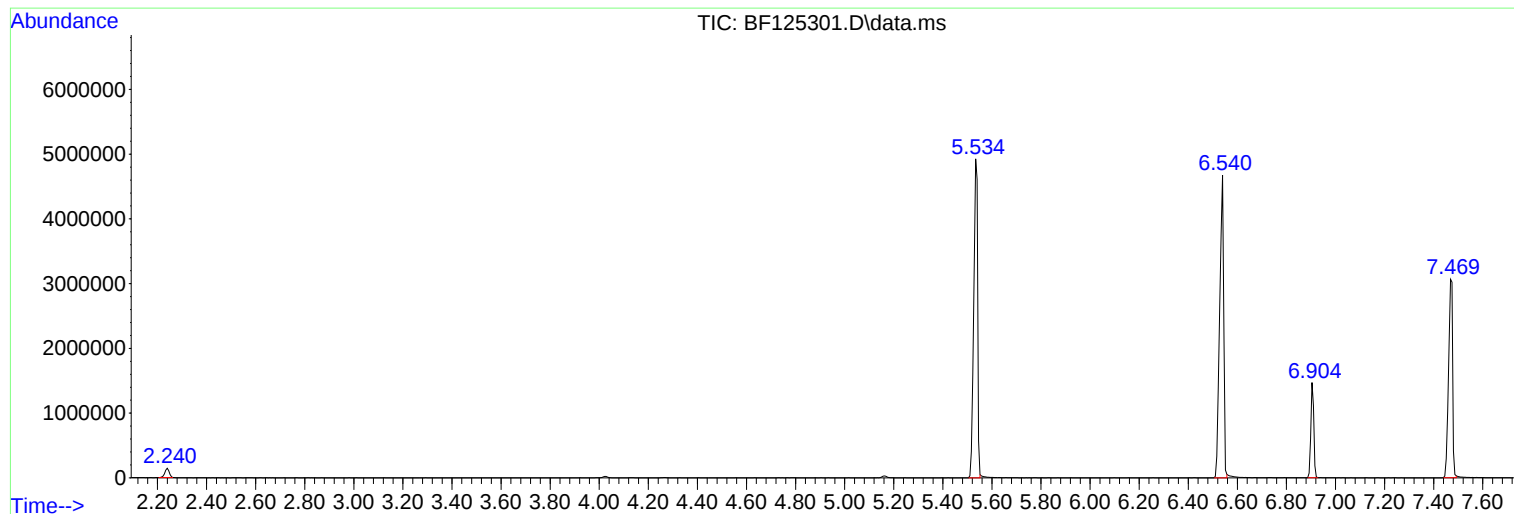

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090121\
Data File : BF125301.D
Acq On : 1 Sep 2021 12:08
Operator : JU/CG
Sample : PB138856BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB138856BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.240	2.96 ng	180118	1,4-Dichlorobenzene-d4	6.904

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	39
3			Silane, tetramethyl-	88	C4H12Si	000075-76-3	38
4			3-Pentanol, 2,4-dimethyl-	116	C7H16O	000600-36-2	37
5			1,3-Dioxolane, 2-methyl-	88	C4H8O2	000497-26-7	37

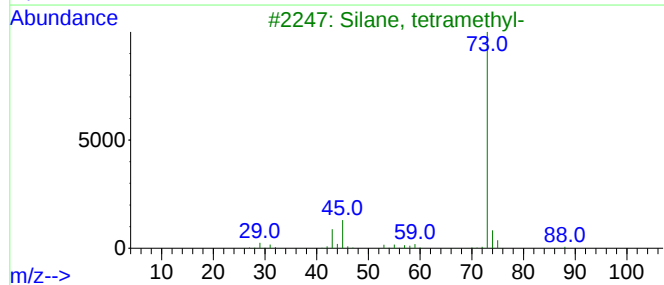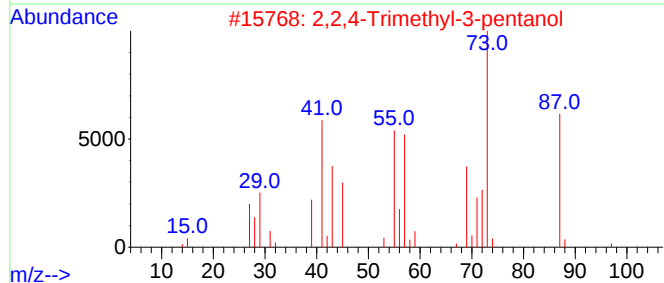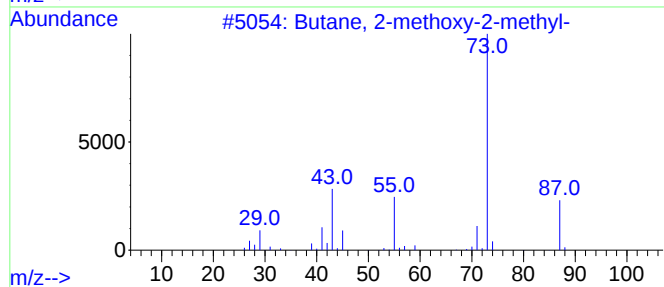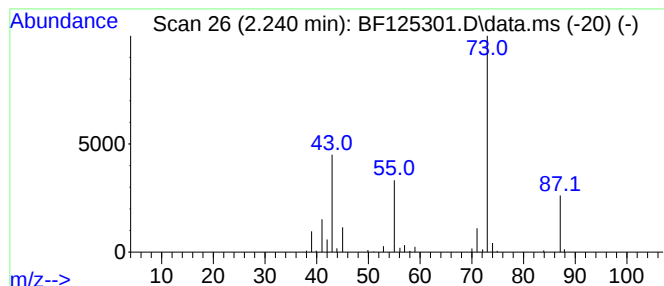

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090121\
Data File : BF125301.D
Acq On : 1 Sep 2021 12:08
Operator : JU/CG
Sample : PB138856BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB138856BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.240	3.0	ng	180118	1	6.904	1218060	20.0