
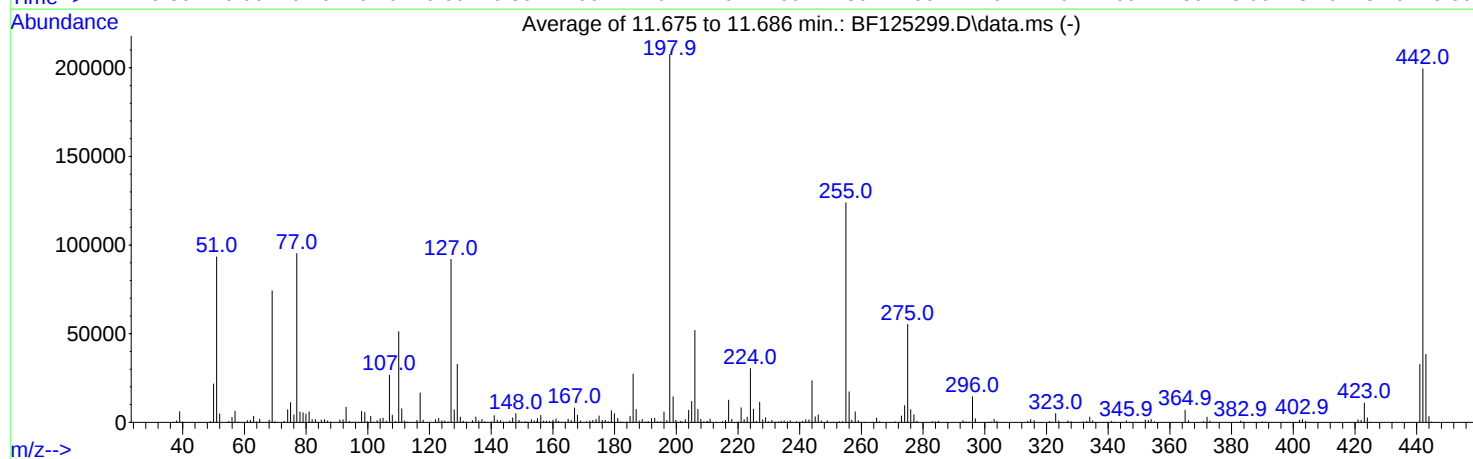


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090121\
 Data File : BF125299.D
 Acq On : 1 Sep 2021 11:04
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 24 12:39:21 2021

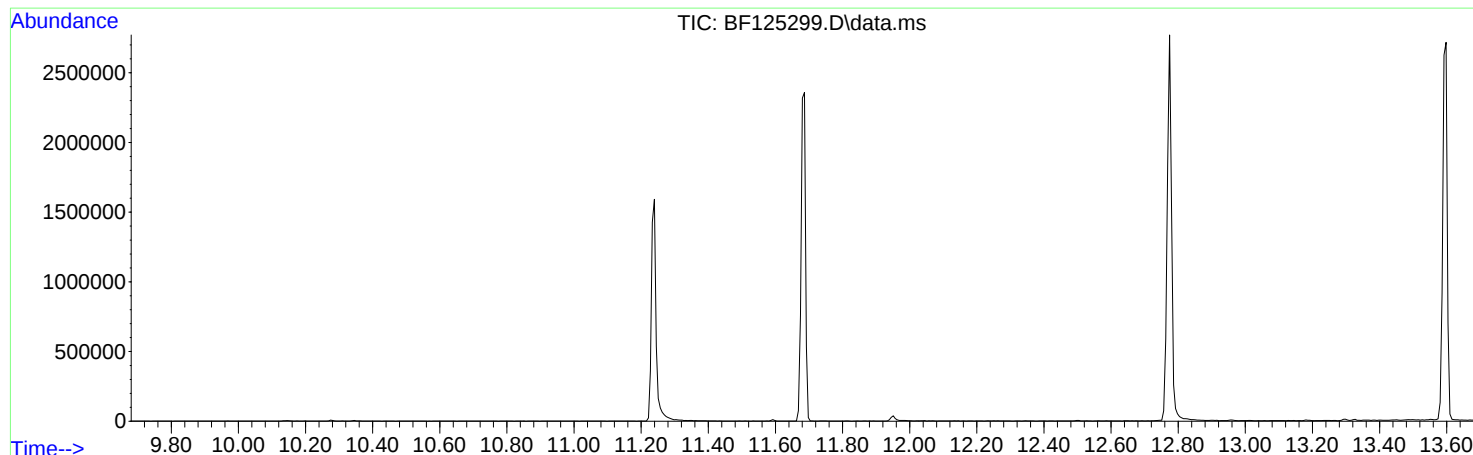




AutoFind: Scans 1630, 1631, 1632; Background Corrected with Scan 1626

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.0	93355	PASS
68	69	0.00	2	1.7	1249	PASS
69	198	0.00	100	35.7	74176	PASS
70	69	0.00	2	0.5	400	PASS
127	198	10	80	44.3	91944	PASS
197	198	0.00	2	0.5	1045	PASS
198	198	100	100	100.0	207493	PASS
199	198	5	9	7.0	14481	PASS
275	198	10	60	26.6	55229	PASS
365	198	1	100	3.4	6988	PASS
441	198	0.01	100	15.7	32638	PASS
442	442	50	100	100.0	199445	PASS
443	442	15	24	19.2	38324	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090121\
 Data File : BF125299.D
 Acq On : 1 Sep 2021 11:04
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Sep 01 13:23:31 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 24 12:39:21 2021
 Response via : Initial Calibration

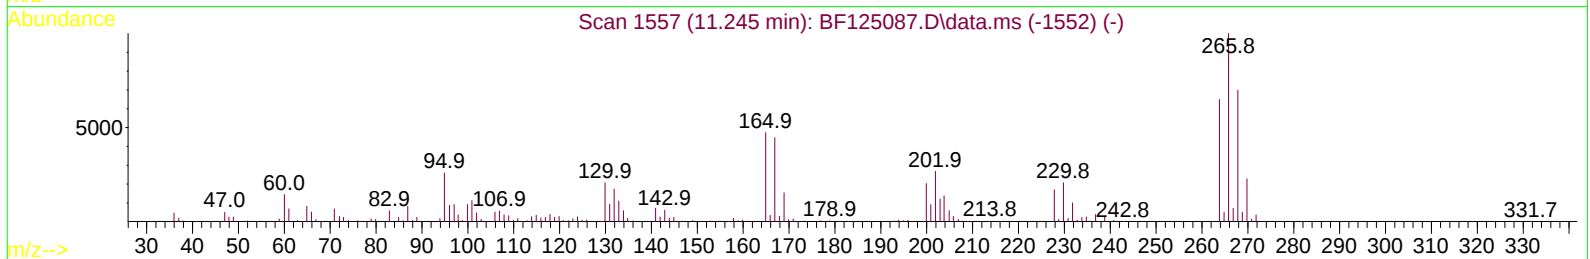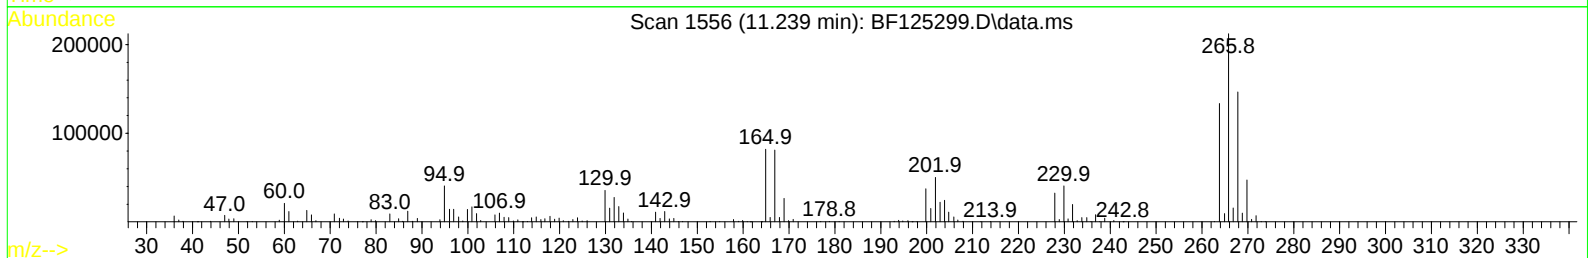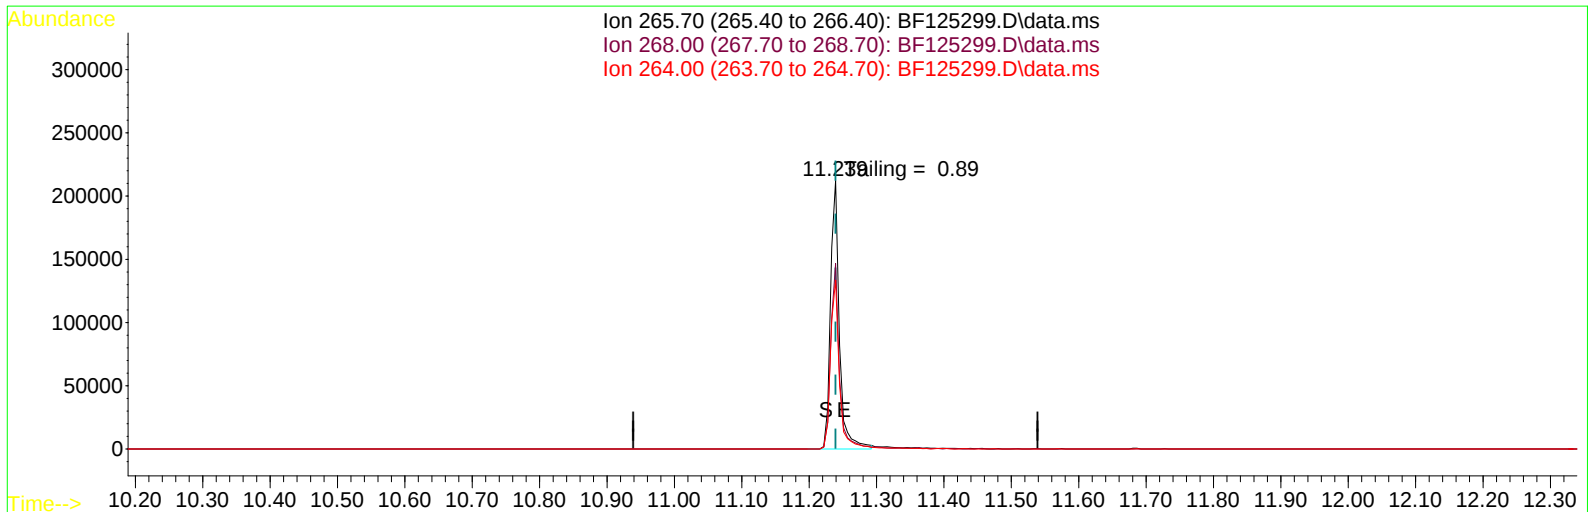

TIC: BF125299.D\data.ms

(70) Pentachlorophenol (C)

11.239min (+ 0.000) 30794.74 ng




response 199023

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	69.09
264.00	69.90	62.94
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090121\
 Data File : BF125299.D
 Acq On : 1 Sep 2021 11:04
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Sep 01 13:23:31 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 24 12:39:21 2021
 Response via : Initial Calibration

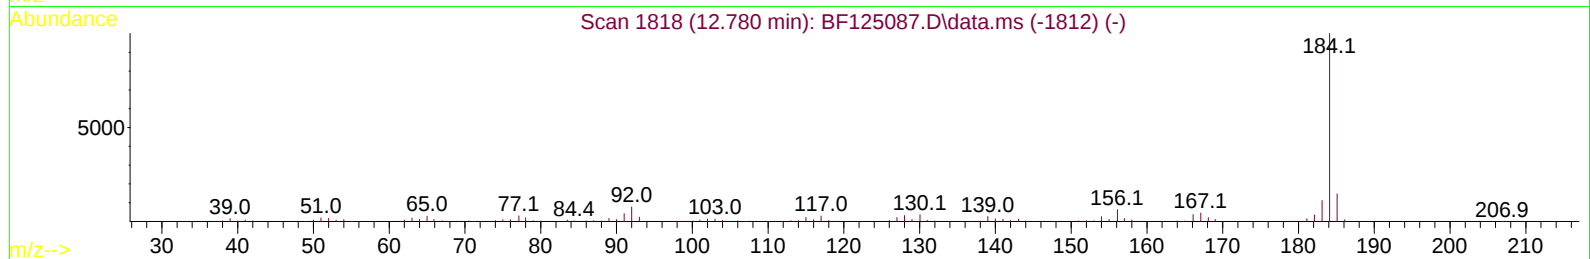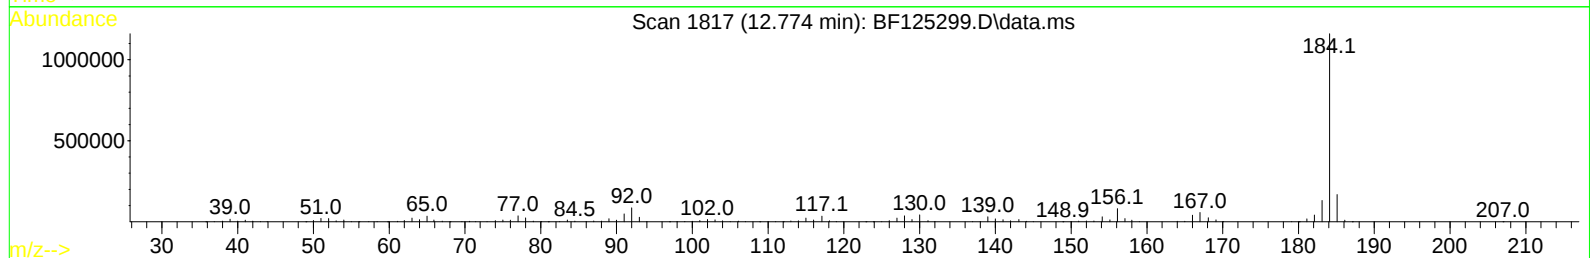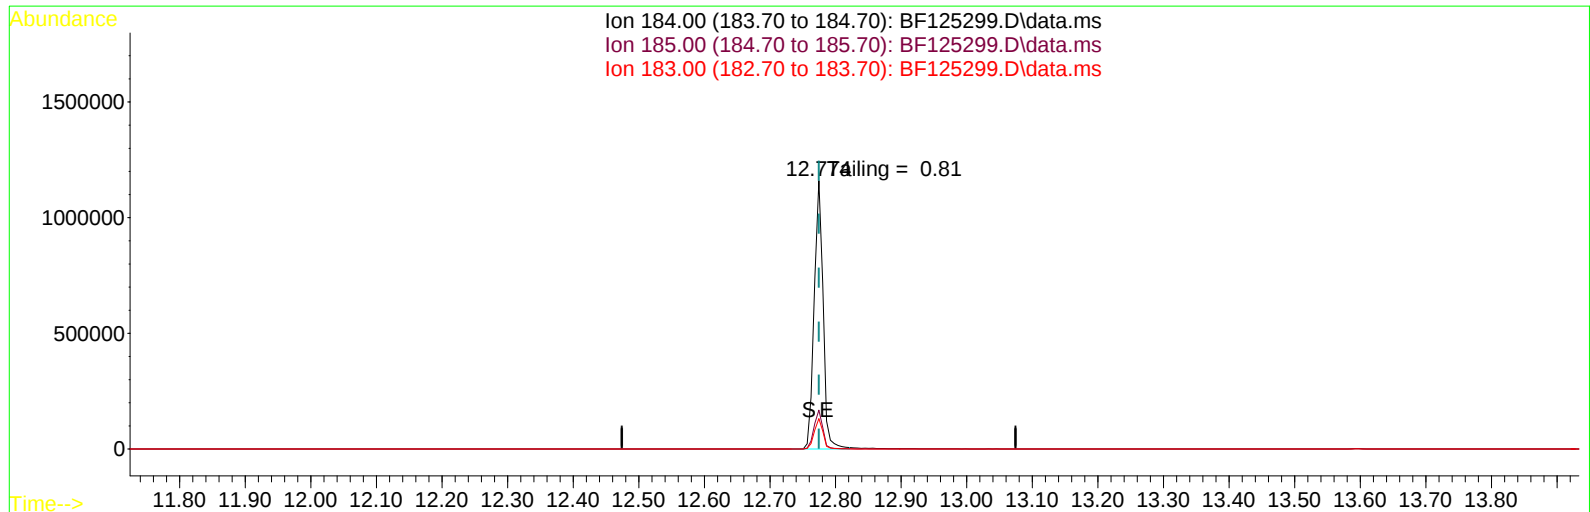

TIC: BF125299.D\data.ms

(77) Benzidine

12.774min (+ 0.000) 0.00 ng

response 1105864

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.53
183.00	10.10	11.36
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/1/2021	BNA_F	<u>BF125299.D</u>
Compound Name	Response	Retention Time
DDT	513896	13.59
DDD	3039	13.29
DDE	1223	12.95
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4262	518158	0.82

Instrument :
BNA_F
ClientSampleId :
DFTPP