
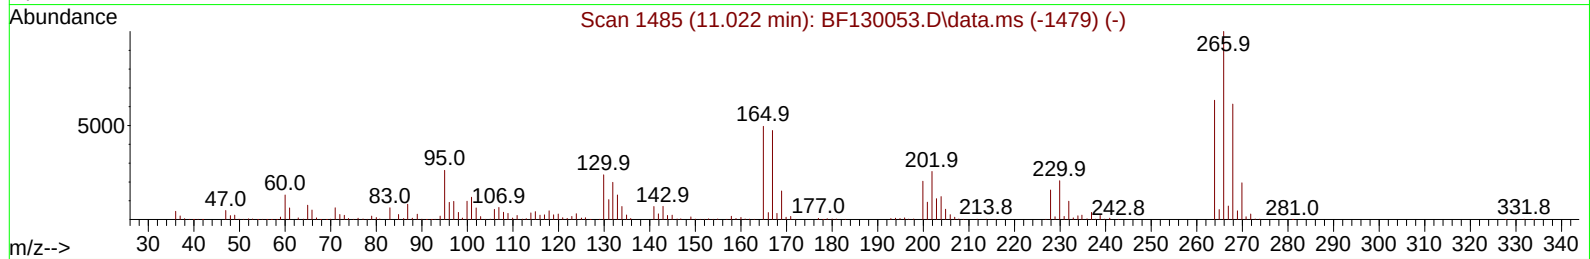
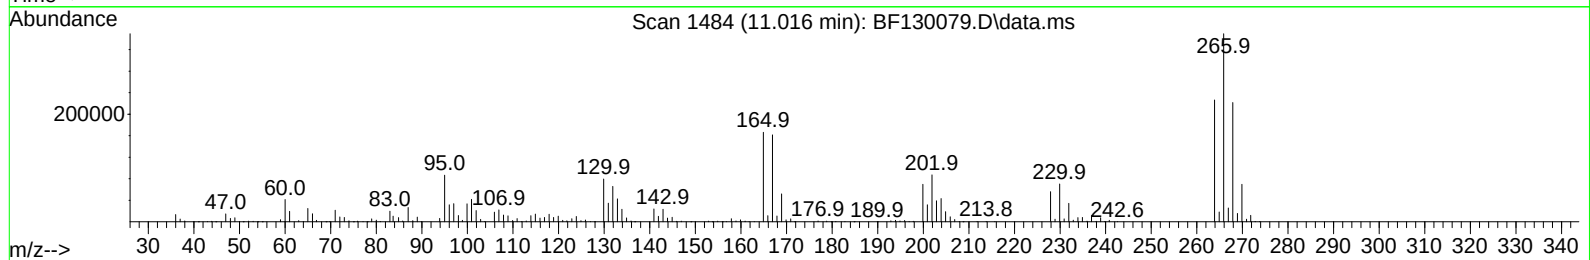


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090122\
 Data File : BF130079.D
 Acq On : 01 Sep 2022 15:53
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 02 05:06:15 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 31 18:15:32 2022
 Response via : Initial Calibration

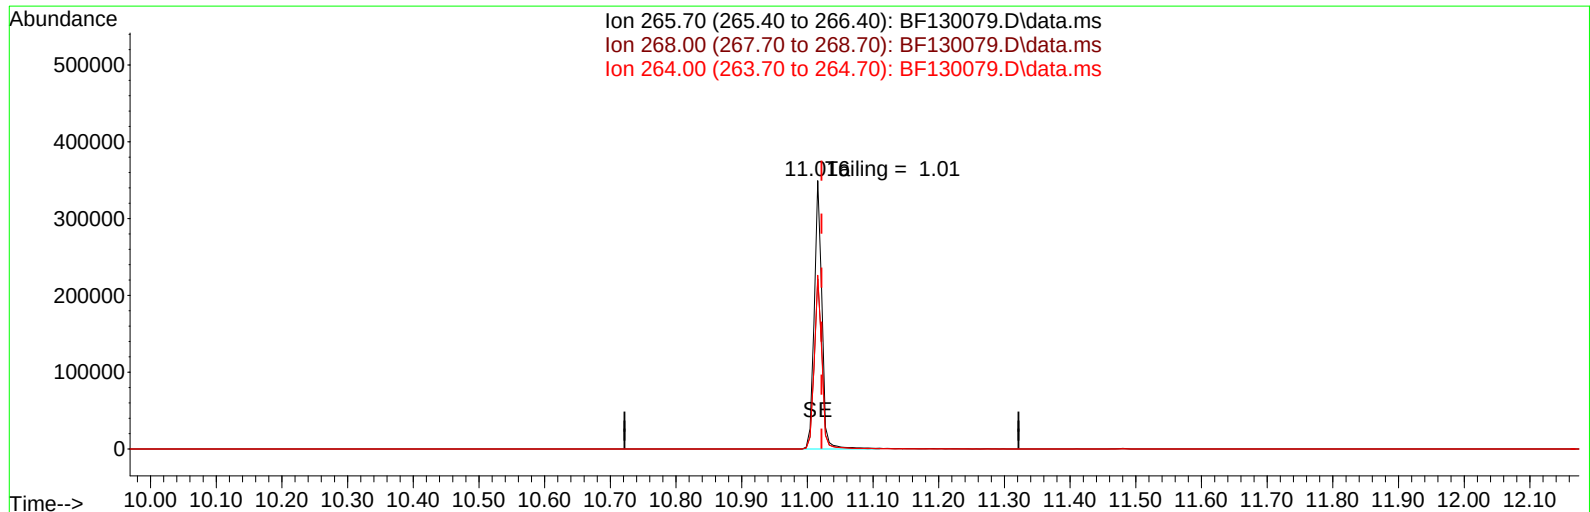

TIC: BF130079.D\data.ms

(70) Pentachlorophenol (C)




11.016min (-0.006) 526235.50 ng

response 288885

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	63.39
264.00	59.90	64.74
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090122\
Data File : BF130079.D
Acq On : 01 Sep 2022 15:53
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 02 05:06:15 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 31 18:15:32 2022
Response via : Initial Calibration

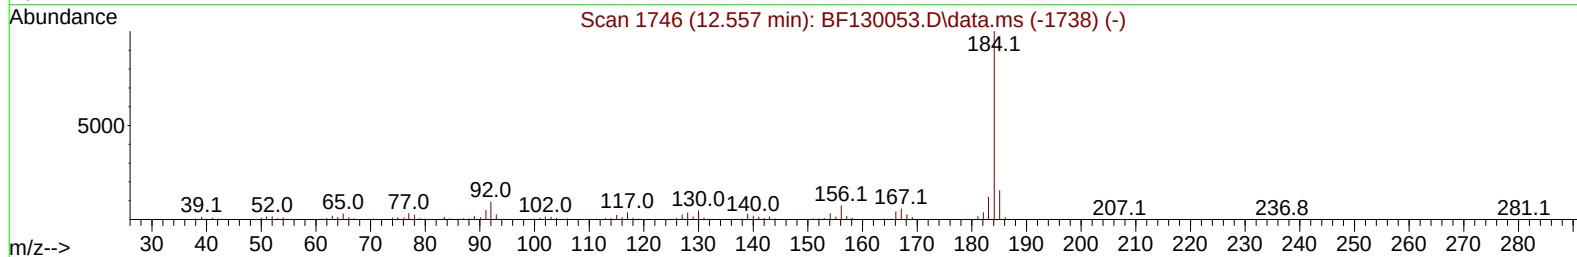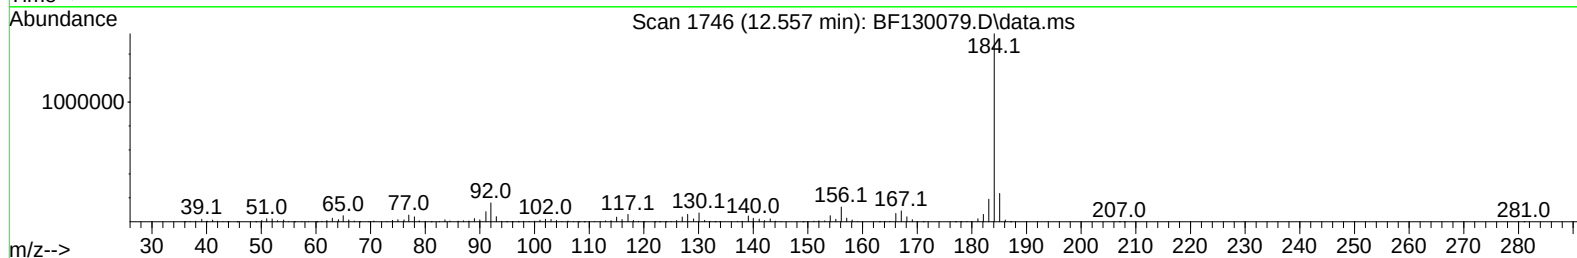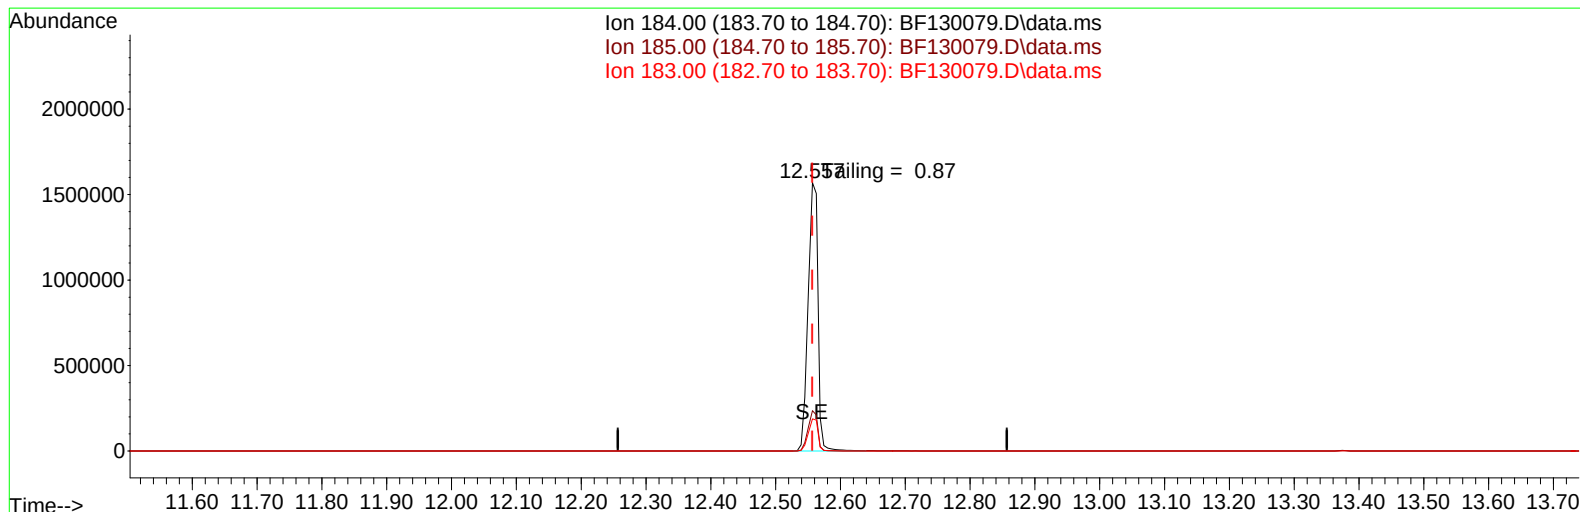

TIC: BF130079.D\data.ms

(77) Benzidine

12.557min (+ 0.000) 0.00 ng

response 1663952

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	15.07
183.00	11.80	11.98
0.00	0.00	0.00