

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090122\
 Data File : BF130085.D
 Acq On : 01 Sep 2022 19:15
 Operator : CG\JU
 Sample : N4385-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 265751-2

Quant Time: Sep 02 04:03:00 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 31 18:15:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.704	152	226193	20.000	ng	0.00
21) Naphthalene-d8	7.981	136	888840	20.000	ng	#-0.01
39) Acenaphthene-d10	9.734	164	470615	20.000	ng	-0.01
64) Phenanthrene-d10	11.216	188	772878	20.000	ng	0.00
76) Chrysene-d12	13.845	240	511857	20.000	ng	-0.01
86) Perylene-d12	15.245	264	427162	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.304	112	774375	58.119	ng	0.00
7) Phenol-d6	6.322	99	568212	34.207	ng	-0.02
23) Nitrobenzene-d5	7.269	82	1271009	91.898	ng	-0.01
42) 2,4,6-Tribromophenol	10.522	330	551354	128.703	ng	-0.01
45) 2-Fluorobiphenyl	9.063	172	2274823	80.141	ng	0.00
79) Terphenyl-d14	12.804	244	2214139	75.013	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090122\
Data File : BF130085.D
Acq On : 01 Sep 2022 19:15
Operator : CG\JU
Sample : N4385-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
265751-2

Quant Time: Sep 02 04:03:00 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 31 18:15:32 2022
Response via : Initial Calibration




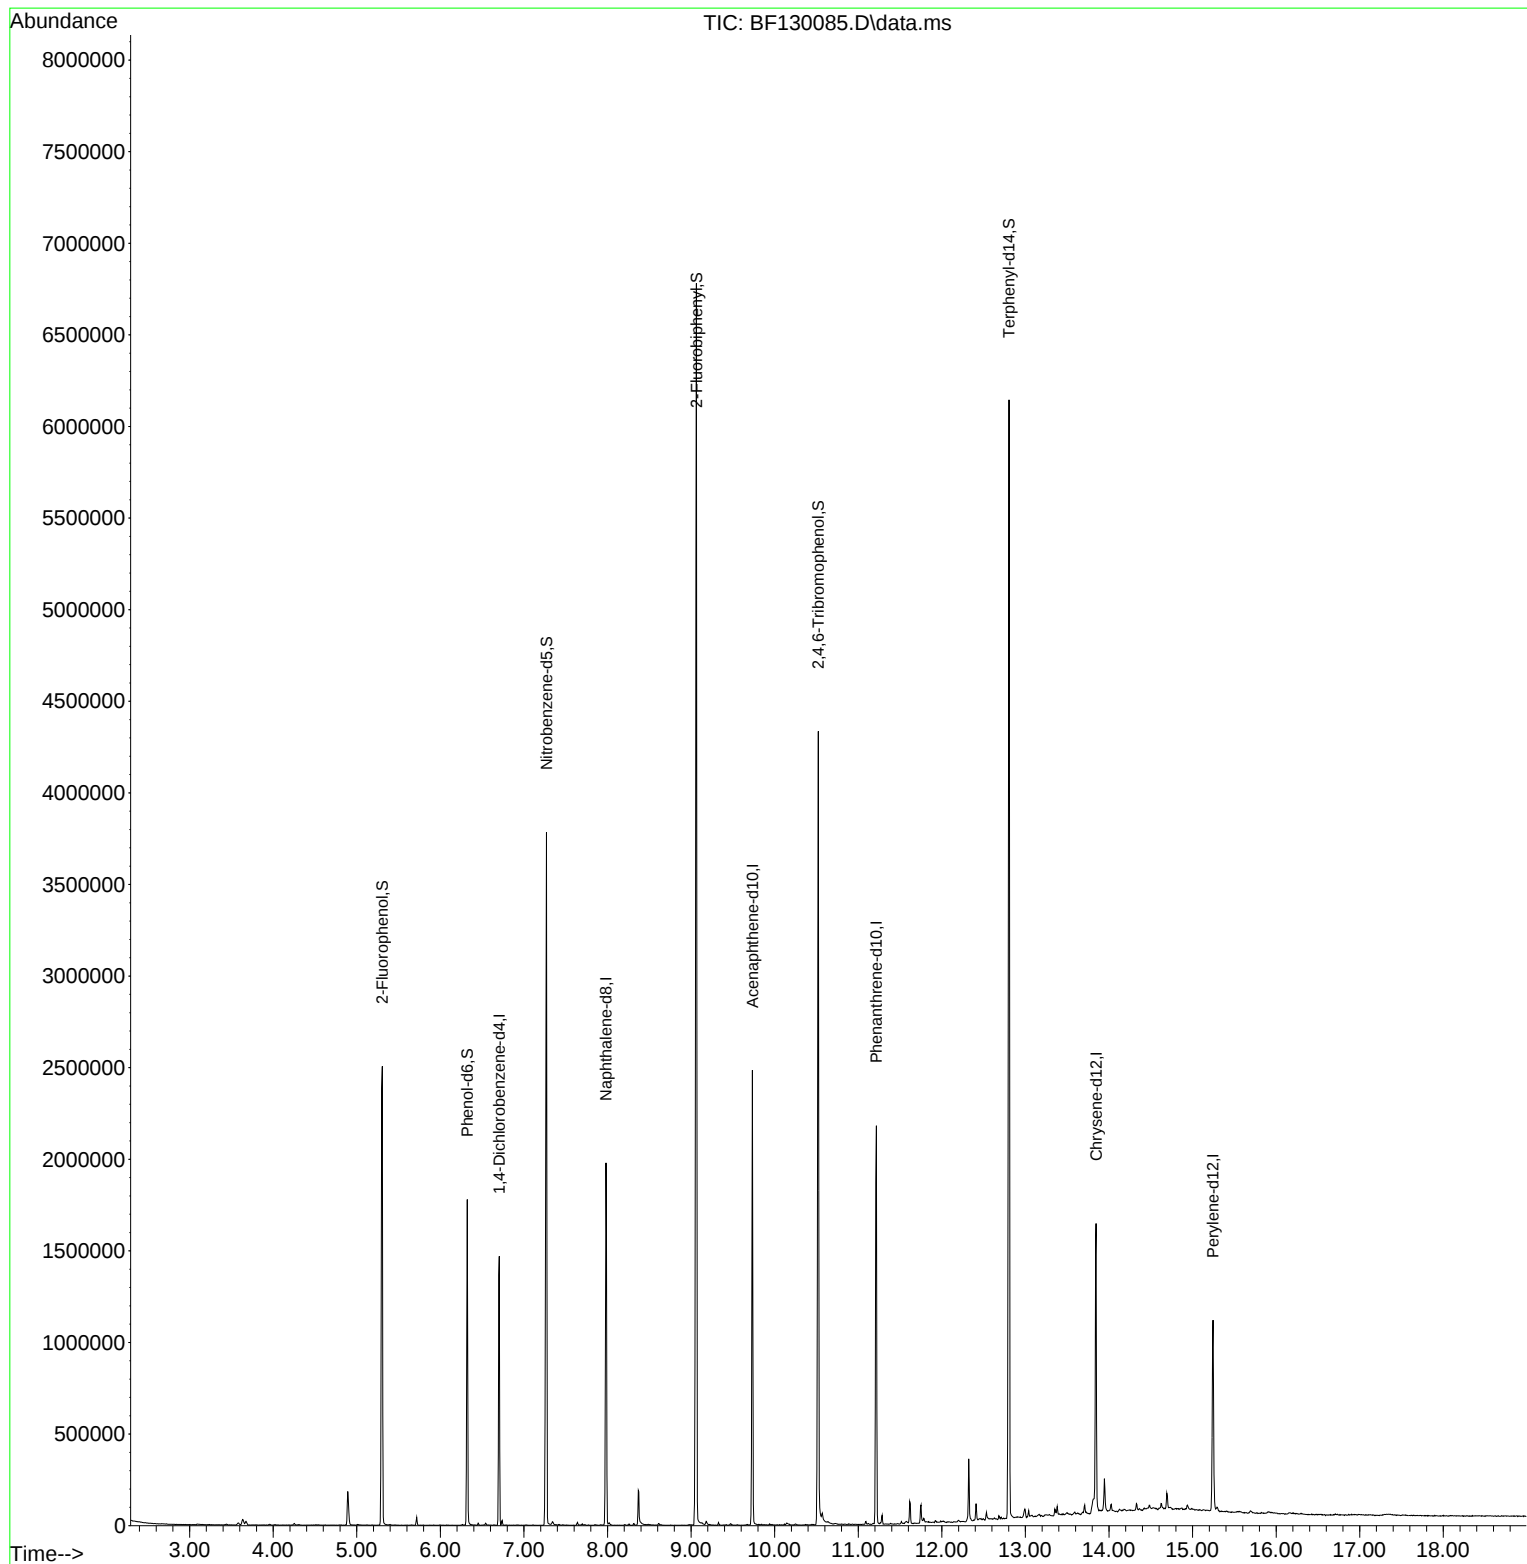


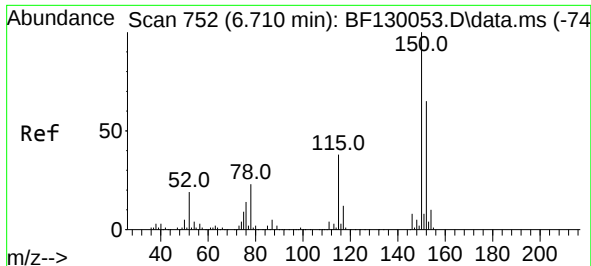

#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.704 min Scan# 751
 Delta R.T. -0.006 min
 Lab File: BF130085.D
 Acq: 01 Sep 2022 19:15




Instrument :
 BNA_F
 ClientSampleId :
 265751-2

Tgt Ion:152 Resp: 226193
 Ion Ratio Lower Upper
 152 100
 150 157.0 126.9 190.3
 115 59.7 53.4 80.0

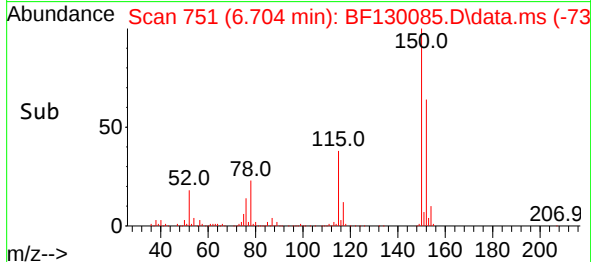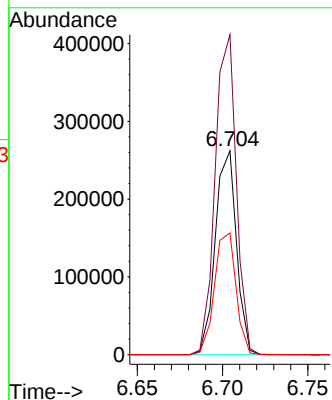

#5
 2-Fluorophenol
 Concen: 58.119 ng
 RT: 5.304 min Scan# 513
 Delta R.T. -0.006 min
 Lab File: BF130085.D
 Acq: 01 Sep 2022 19:15

Tgt Ion:112 Resp: 774375
 Ion Ratio Lower Upper
 112 100
 64 52.7 47.6 71.4
 63 26.2 24.6 37.0


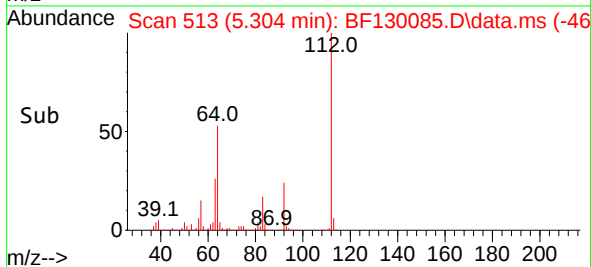
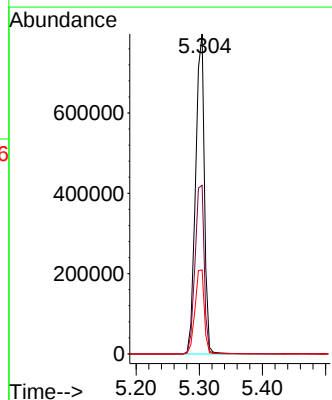
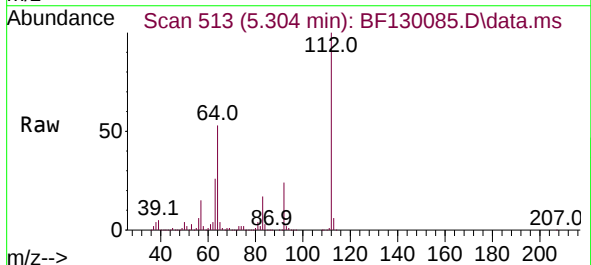




#7
Phenol-d6
Concen: 34.207 ng
RT: 6.322 min Scan# 68
Delta R.T. -0.023 min
Lab File: BF130085.D
Acq: 01 Sep 2022 19:15




Instrument :
BNA_F
ClientSampleId :
265751-2


Tgt Ion: 99 Resp: 568212
Ion Ratio Lower Upper
99 100
42 15.6 15.0 22.4
71 30.6 28.8 43.2

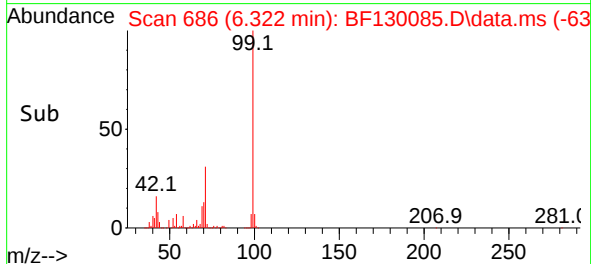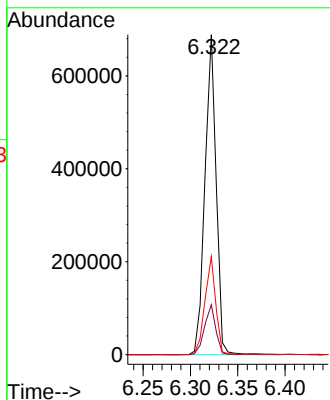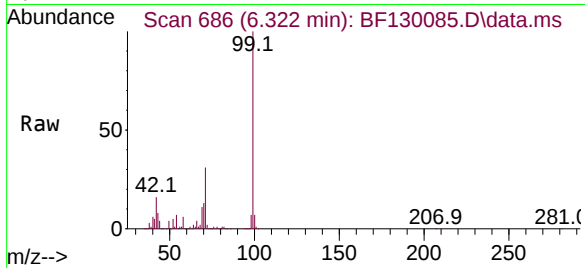

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 7.981 min Scan# 968
Delta R.T. -0.011 min
Lab File: BF130085.D
Acq: 01 Sep 2022 19:15

Tgt Ion: 136 Resp: 888840
Ion Ratio Lower Upper
136 100
137 11.3 8.4 12.6
54 8.1 6.2 9.2
68 6.8 4.2 6.4

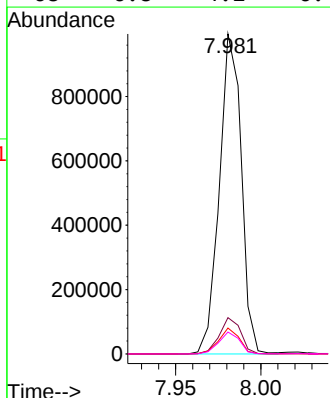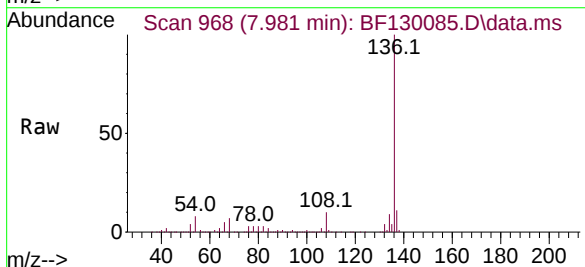



#23

Nitrobenzene-d5

Concen: 91.898 ng

RT: 7.269 min Scan# 84

Delta R.T. -0.012 min

Lab File: BF130085.D

Acq: 01 Sep 2022 19:15

Instrument :





BNA_F

ClientSampleId :

265751-2

Tgt Ion: 82 Resp: 1271009

Ion	Ratio	Lower	Upper
82	100		
128	47.1	36.1	54.1
54	47.3	40.0	60.0

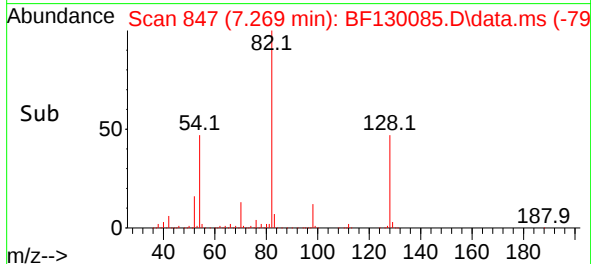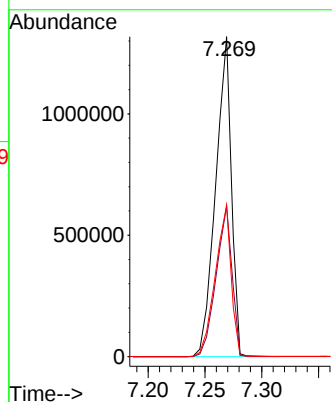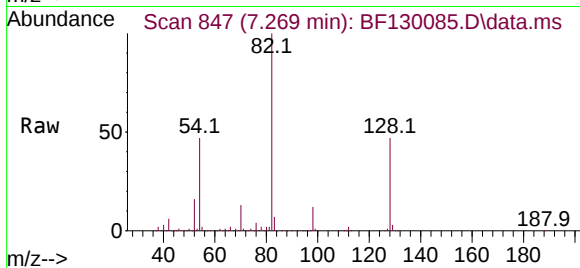

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.734 min Scan# 1266




Delta R.T. -0.011 min


Lab File: BF130085.D

Acq: 01 Sep 2022 19:15

Tgt Ion: 164 Resp: 470615

Ion	Ratio	Lower	Upper
164	100		
162	100.6	82.0	123.0
160	43.4	35.4	53.0

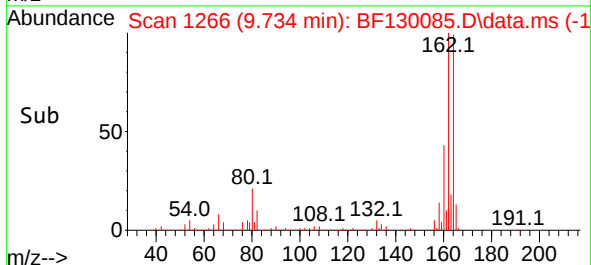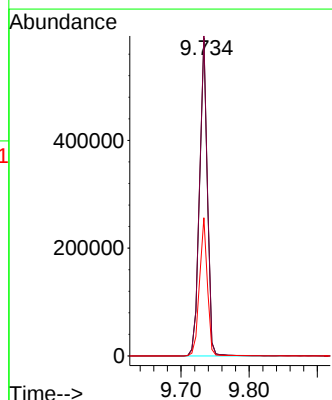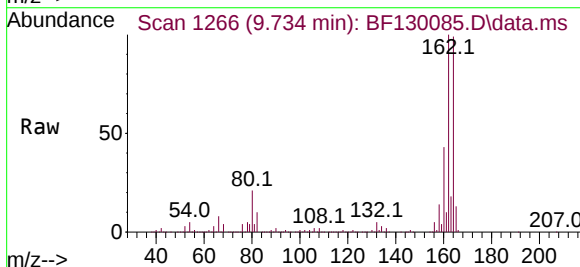

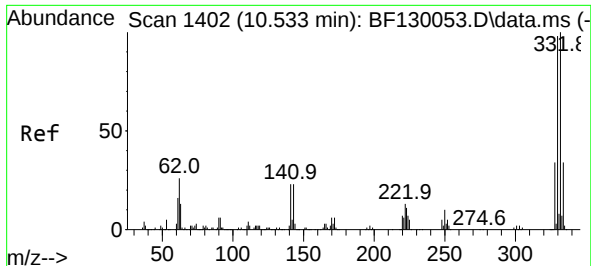

#42

2,4,6-Tribromophenol

Concen: 128.703 ng

RT: 10.522 min Scan# 1400

Delta R.T. -0.012 min

Lab File: BF130085.D

Acq: 01 Sep 2022 19:15

Instrument :

BNA_F

ClientSampleId :

265751-2





Tgt Ion:330 Resp: 551354

Ion Ratio Lower Upper

330 100

332 103.1 82.6 124.0

141 32.9 27.6 41.4

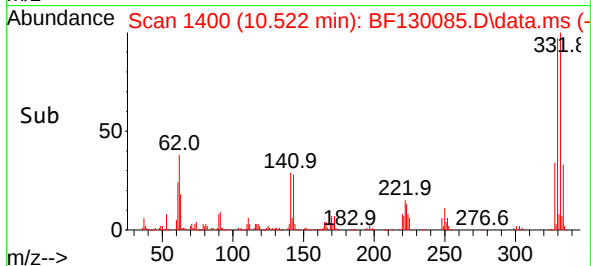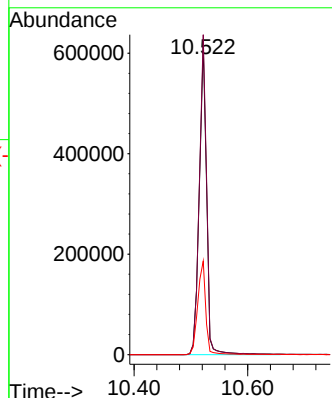

#45

2-Fluorobiphenyl

Concen: 80.141 ng

RT: 9.063 min Scan# 1152

Delta R.T. -0.006 min

Lab File: BF130085.D

Acq: 01 Sep 2022 19:15




Tgt Ion:172 Resp: 2274823


Ion Ratio Lower Upper

172 100

171 35.9 28.4 42.6

170 24.1 19.1 28.7


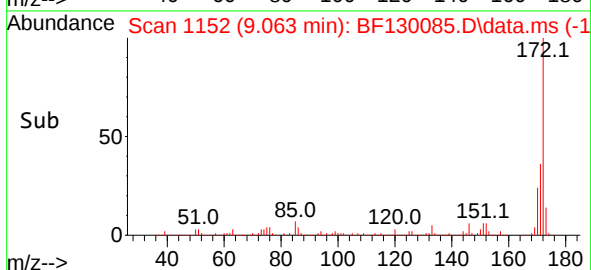
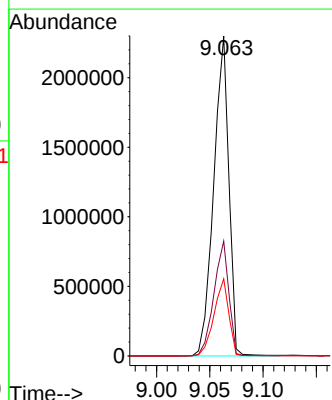
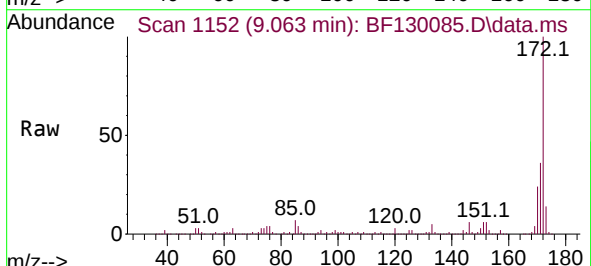


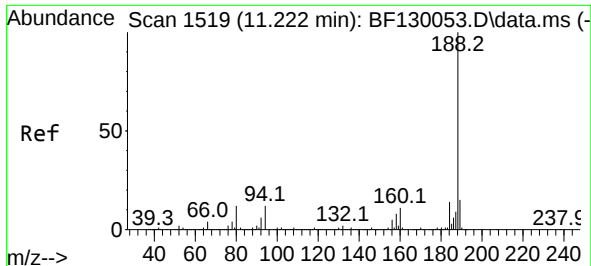

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.216 min Scan# 1518
Delta R.T. -0.006 min
Lab File: BF130085.D
Acq: 01 Sep 2022 19:15




Instrument :
BNA_F
ClientSampleId :
265751-2


Tgt Ion:188 Resp: 772878
Ion Ratio Lower Upper
188 100
94 10.3 7.4 11.2
80 10.8 7.9 11.9

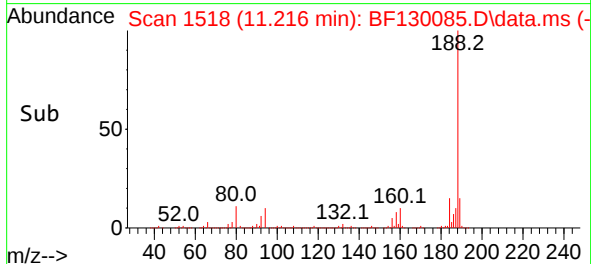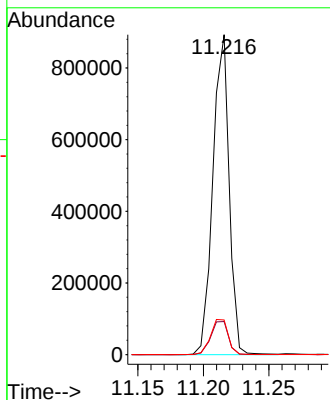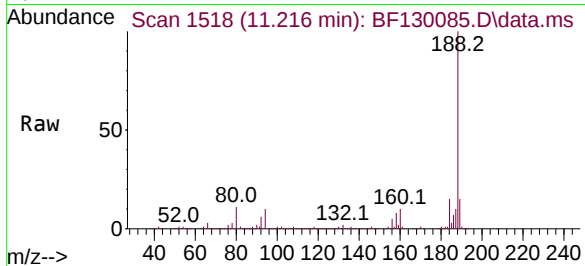

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.845 min Scan# 1965
Delta R.T. -0.012 min
Lab File: BF130085.D
Acq: 01 Sep 2022 19:15

Tgt Ion:240 Resp: 511857
Ion Ratio Lower Upper
240 100
120 12.9 9.2 13.8
236 24.7 20.7 31.1


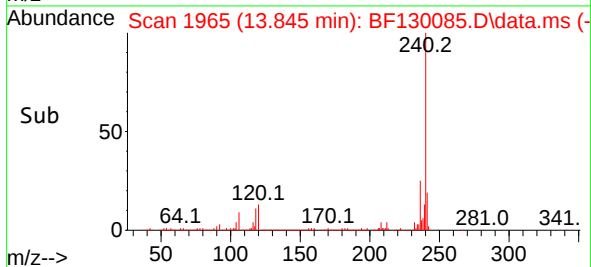
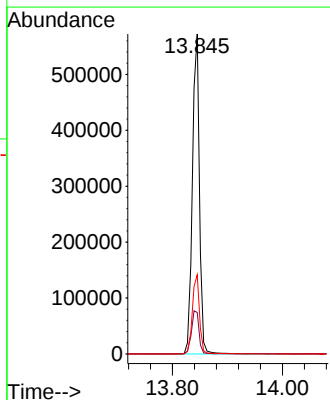
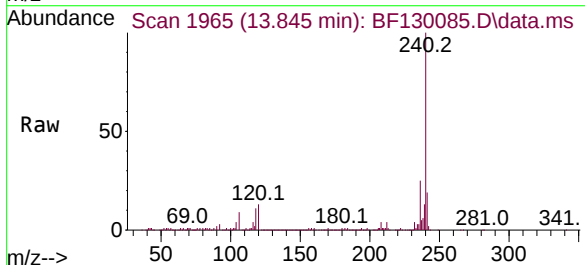


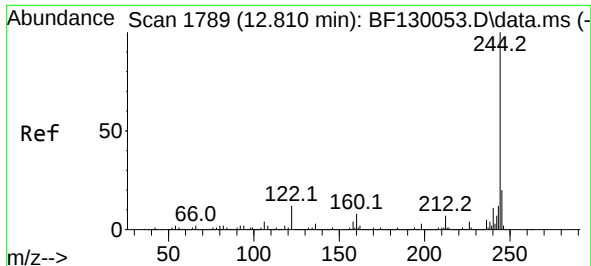

#79
 Terphenyl-d14
 Concen: 75.013 ng
 RT: 12.804 min Scan# 11
 Delta R.T. -0.006 min
 Lab File: BF130085.D
 Acq: 01 Sep 2022 19:15

Instrument :
 BNA_F
 ClientSampleId :
 265751-2

Tgt Ion:244 Resp: 2214139
 Ion Ratio Lower Upper
 244 100
 212 7.1 5.9 8.9
 122 12.5 9.9 14.9

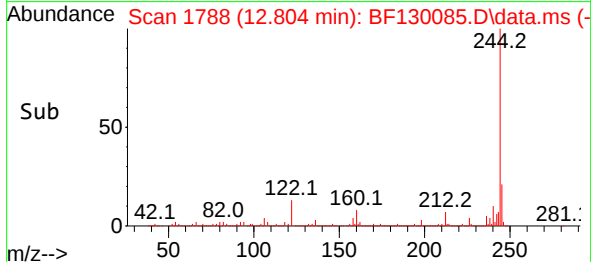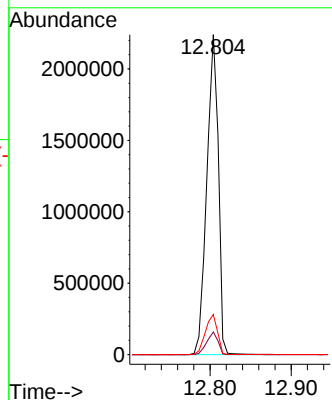

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.245 min Scan# 2203
 Delta R.T. -0.006 min
 Lab File: BF130085.D
 Acq: 01 Sep 2022 19:15

Tgt Ion:264 Resp: 427162
 Ion Ratio Lower Upper
 264 100
 260 23.4 19.1 28.7
 265 21.6 16.7 25.1

