

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090122\
 Data File : BF130070.D
 Acq On : 01 Sep 2022 10:20
 Operator : CG\JU
 Sample : PB147382BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB147382BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF130070.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.934	443	450	462	rVB	229316	387590	4.61%	0.737%
2	5.322	509	516	519	rBV	5490040	6620389	78.73%	12.589%
3	6.340	682	689	692	rBV	4999535	6683265	79.48%	12.708%
4	6.704	747	751	754	rBV	1799380	1504588	17.89%	2.861%
5	7.269	841	847	850	rBV	3857777	4547958	54.09%	8.648%
6	7.987	963	969	972	rBV	2117370	2162977	25.72%	4.113%
7	9.063	1146	1152	1155	rBV	7335135	8393126	99.81%	15.960%
8	9.734	1260	1266	1269	rBV	3047813	2596328	30.88%	4.937%
9	10.528	1393	1401	1404	rBV	5093086	5630381	66.96%	10.706%
10	11.216	1514	1518	1521	rBV	3129015	2567795	30.54%	4.883%
11	12.810	1783	1789	1792	rBV	7688723	8408812	100.00%	15.990%
12	13.845	1961	1965	1968	rBV	2011876	1793980	21.33%	3.411%
13	15.245	2198	2203	2210	rBV	1150981	1291850	15.36%	2.457%




Sum of corrected areas: 52589039

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090122\
Data File : BF130070.D
Acq On : 01 Sep 2022 10:20
Operator : CG\JU
Sample : PB147382BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB147382BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

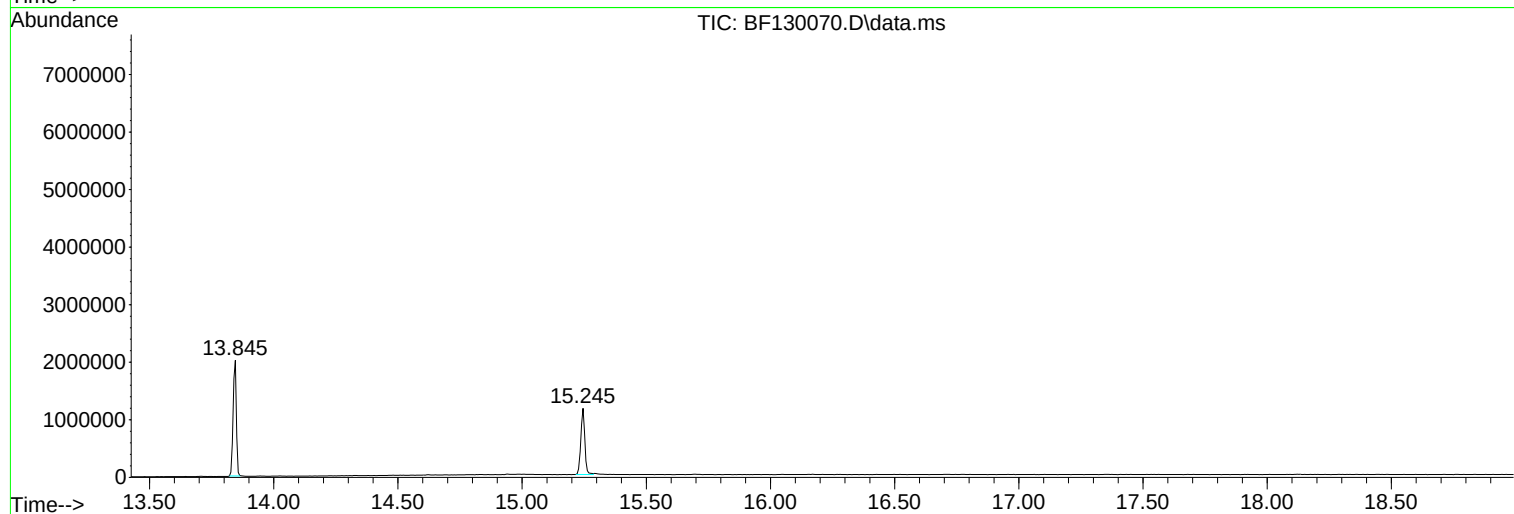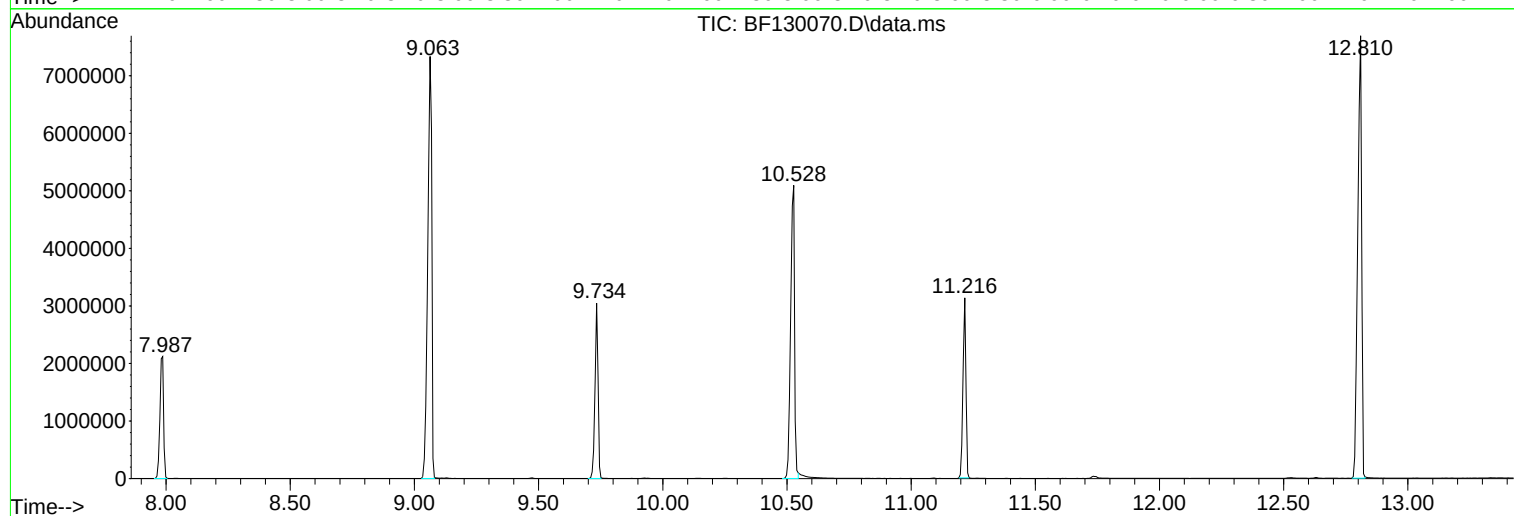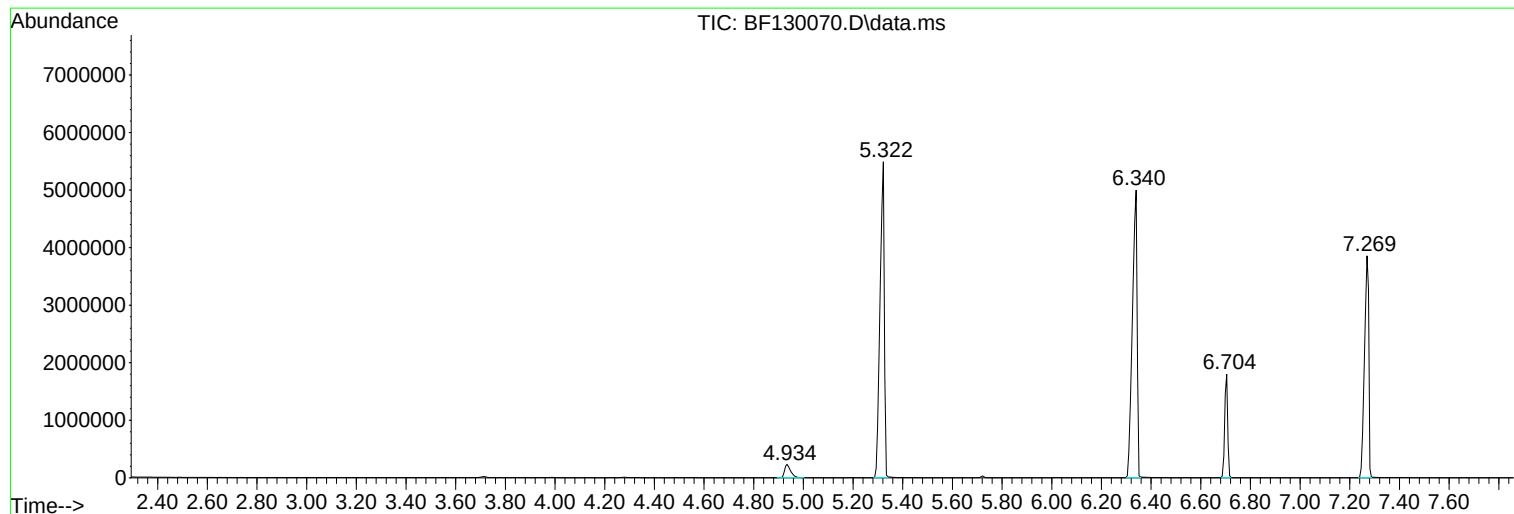

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090122\
Data File : BF130070.D
Acq On : 01 Sep 2022 10:20
Operator : CG\JU
Sample : PB147382BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB147382BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090122\
Data File : BF130070.D
Acq On : 01 Sep 2022 10:20
Operator : CG\JU
Sample : PB147382BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB147382BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------