

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090122\
 Data File : BF130090.D
 Acq On : 01 Sep 2022 21:57
 Operator : CG\JU
 Sample : N4391-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 256317-3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF130090.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.898	440	444	455	rVB	223938	261818	3.63%	0.676%
2	5.304	508	513	516	rBV	2978850	2785682	38.63%	7.194%
3	6.322	682	686	689	rBV	2008768	1665738	23.10%	4.302%
4	6.704	747	751	754	rBV	1562802	1402418	19.45%	3.622%
5	7.269	841	847	850	rBV	3878332	3978334	55.18%	10.273%
6	7.981	964	968	972	rBV	2114057	1908630	26.47%	4.929%
7	9.063	1146	1152	1155	rBV	7100471	7210295	100.00%	18.620%
8	9.451	1214	1218	1224	rBV2	191737	170025	2.36%	0.439%
9	9.733	1260	1266	1269	rBV	2578925	2173977	30.15%	5.614%
10	10.522	1393	1400	1403	rBV	4625430	4462470	61.89%	11.524%
11	10.622	1413	1417	1429	rVB3	94787	167843	2.33%	0.433%
12	11.216	1514	1518	1521	rBV	2260358	2068711	28.69%	5.342%
13	11.616	1583	1586	1590	rVB	114780	96260	1.34%	0.249%
14	11.751	1605	1609	1612	rBV	159362	169677	2.35%	0.438%
15	12.533	1739	1742	1754	rVB	70905	81612	1.13%	0.211%
16	12.804	1783	1788	1791	rBV	6663057	6764276	93.81%	17.468%
17	13.798	1951	1957	1961	rBV5	58712	135406	1.88%	0.350%
18	13.845	1961	1965	1968	rVB	1669516	1593340	22.10%	4.115%
19	13.945	1976	1982	1993	rBV	306949	335677	4.66%	0.867%
20	15.245	2198	2203	2209	rBV	1148746	1292179	17.92%	3.337%




Sum of corrected areas: 38724368

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090122\
Data File : BF130090.D
Acq On : 01 Sep 2022 21:57
Operator : CG\JU
Sample : N4391-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
256317-3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

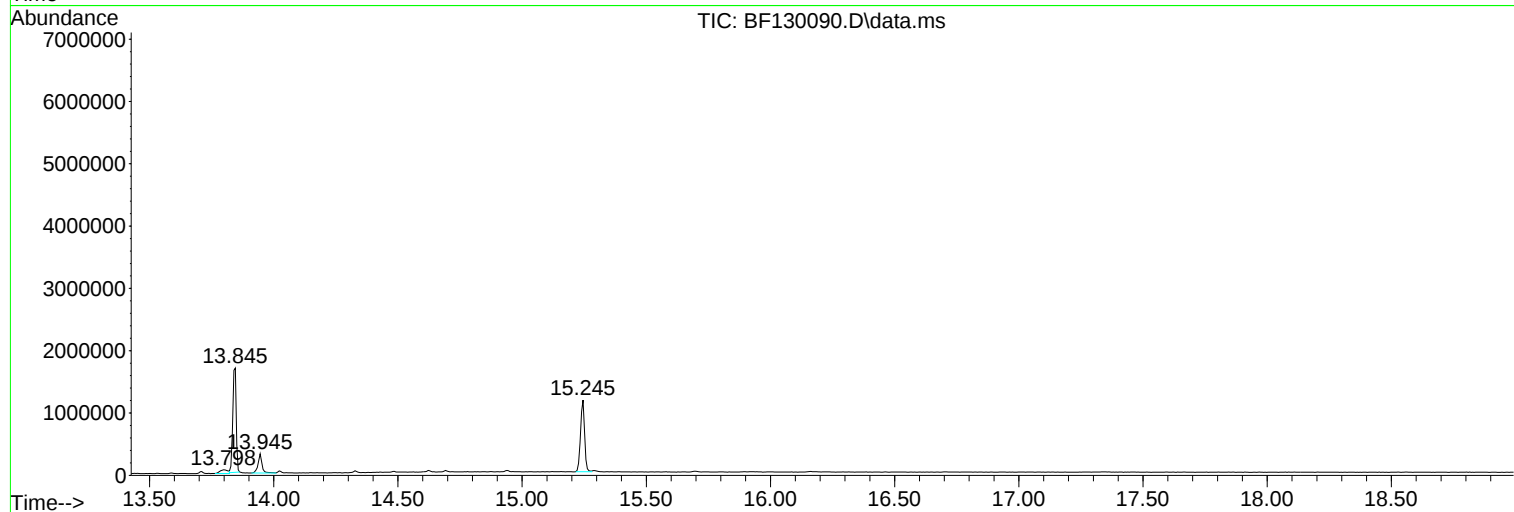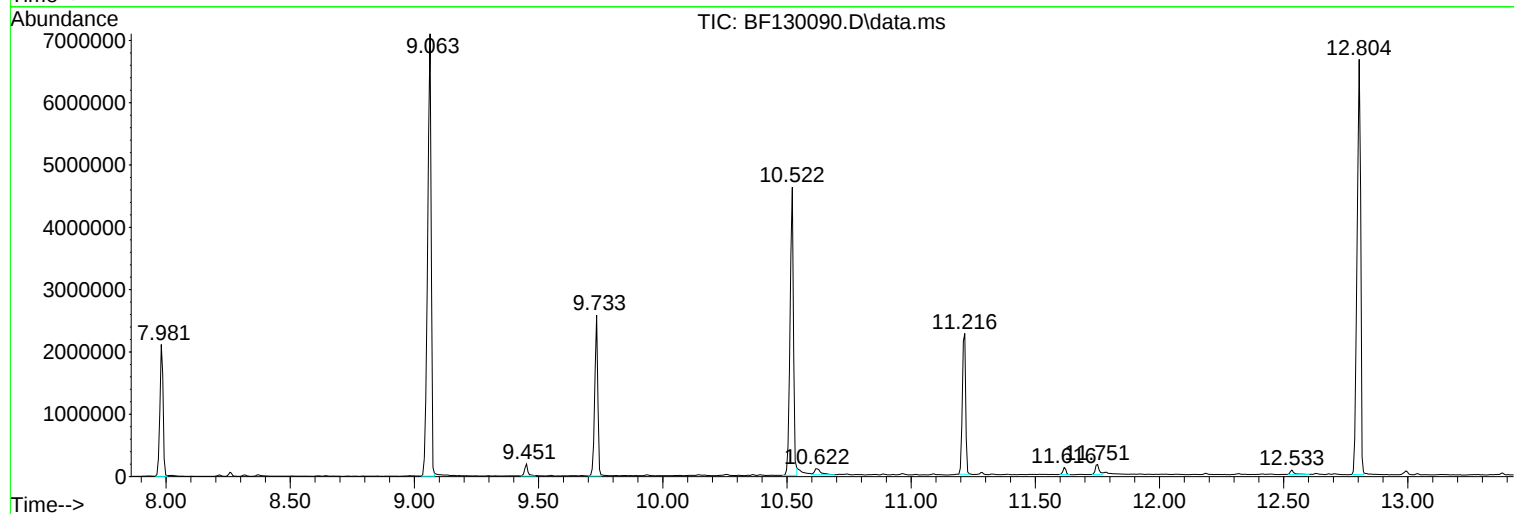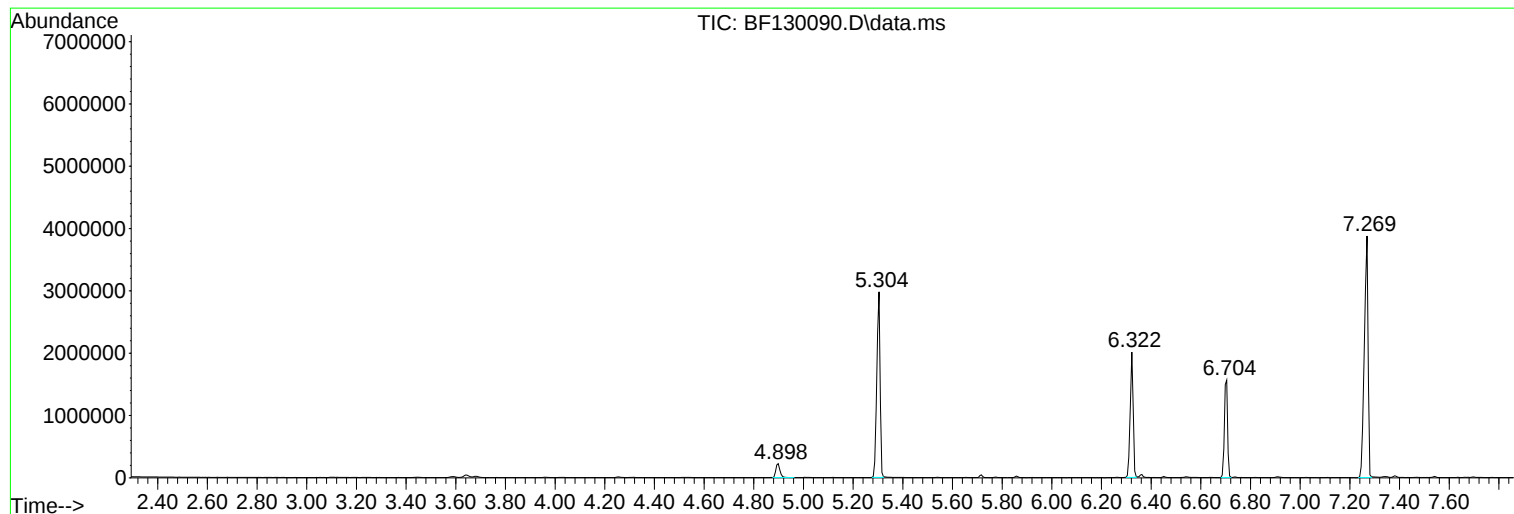

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090122\
Data File : BF130090.D
Acq On : 01 Sep 2022 21:57
Operator : CG\JU
Sample : N4391-01
Misc :
ALS Vial : 12 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
256317-3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.	
4.898	3.73 ng	261818	1,4-Dichlorobenzene-d4	6.704	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	50
2	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	32
3	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	25
4	Acetone	58	C3H6O	000067-64-1	10
5	Guanidine	59	CH5N3	000113-00-8	9

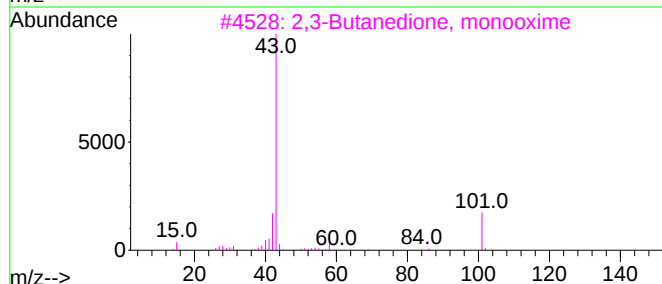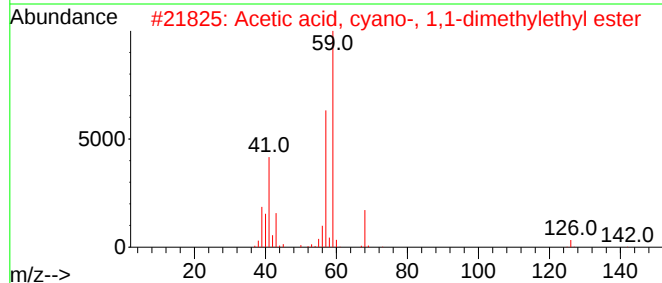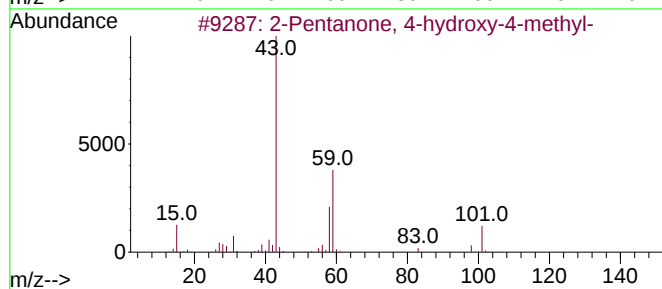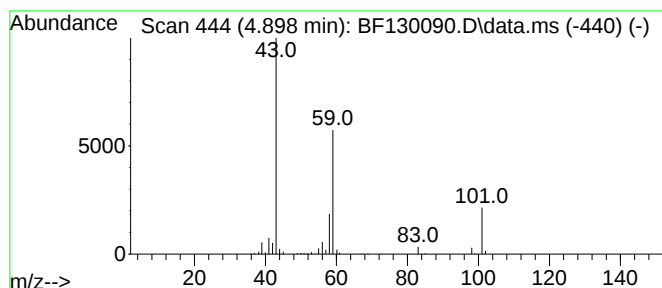

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090122\
Data File : BF130090.D
Acq On : 01 Sep 2022 21:57
Operator : CG\JU
Sample : N4391-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
256317-3










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.945	4.21 ng	335677	Chrysene-d12	13.845

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	98
2			(E)-7-Benzylidene-1-azabicyclo[3...]	293	C15H19N03S	1000483-83-4	70
3			Formaldehyde, (triphenylphosphor...]	304	C19H17N2P	015990-54-2	50
4			Carbazol-1-one, 1,2,3,4-tetrahyd...	277	C18H15N02	299962-12-2	37
5			2-Phenyl-6-(trifluoromethyl)-1H-...	277	C15H10F3NO	1000387-59-3	25

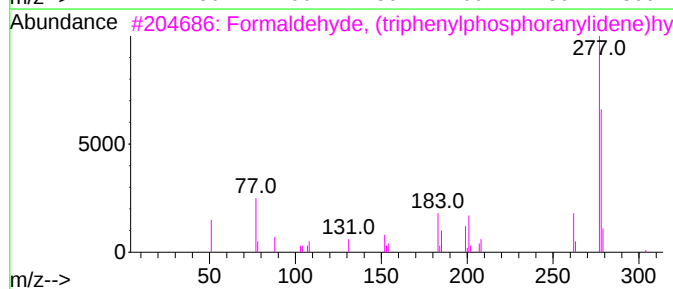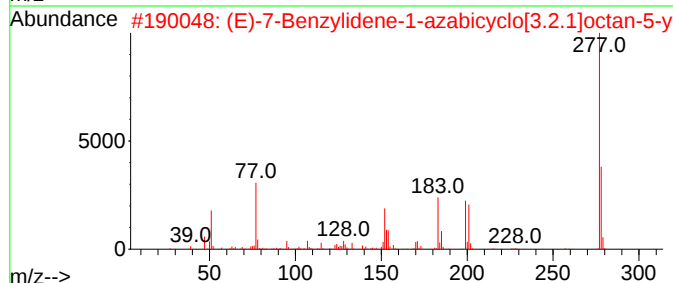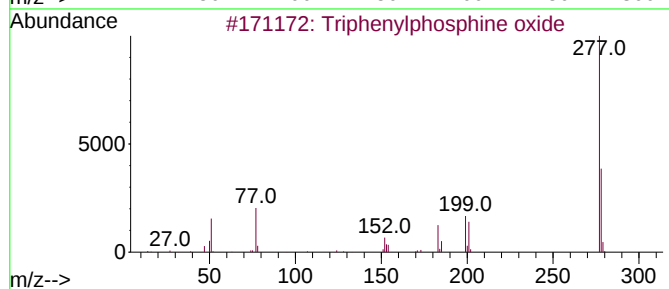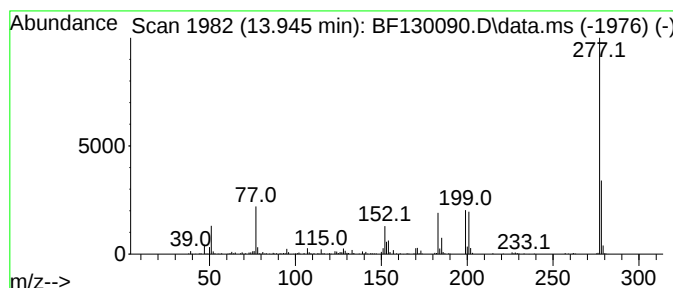

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090122\
Data File : BF130090.D
Acq On : 01 Sep 2022 21:57
Operator : CG\JU
Sample : N4391-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
256317-3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	4.898	3.7	ng	261818	1	6.704	1402420	20.0
Triphenylphosph...	13.945	4.2	ng	335677	5	13.845	1593340	20.0