


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090122\
 Data File : BF130068.D
 Acq On : 01 Sep 2022 09:13
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 31 18:15:32 2022

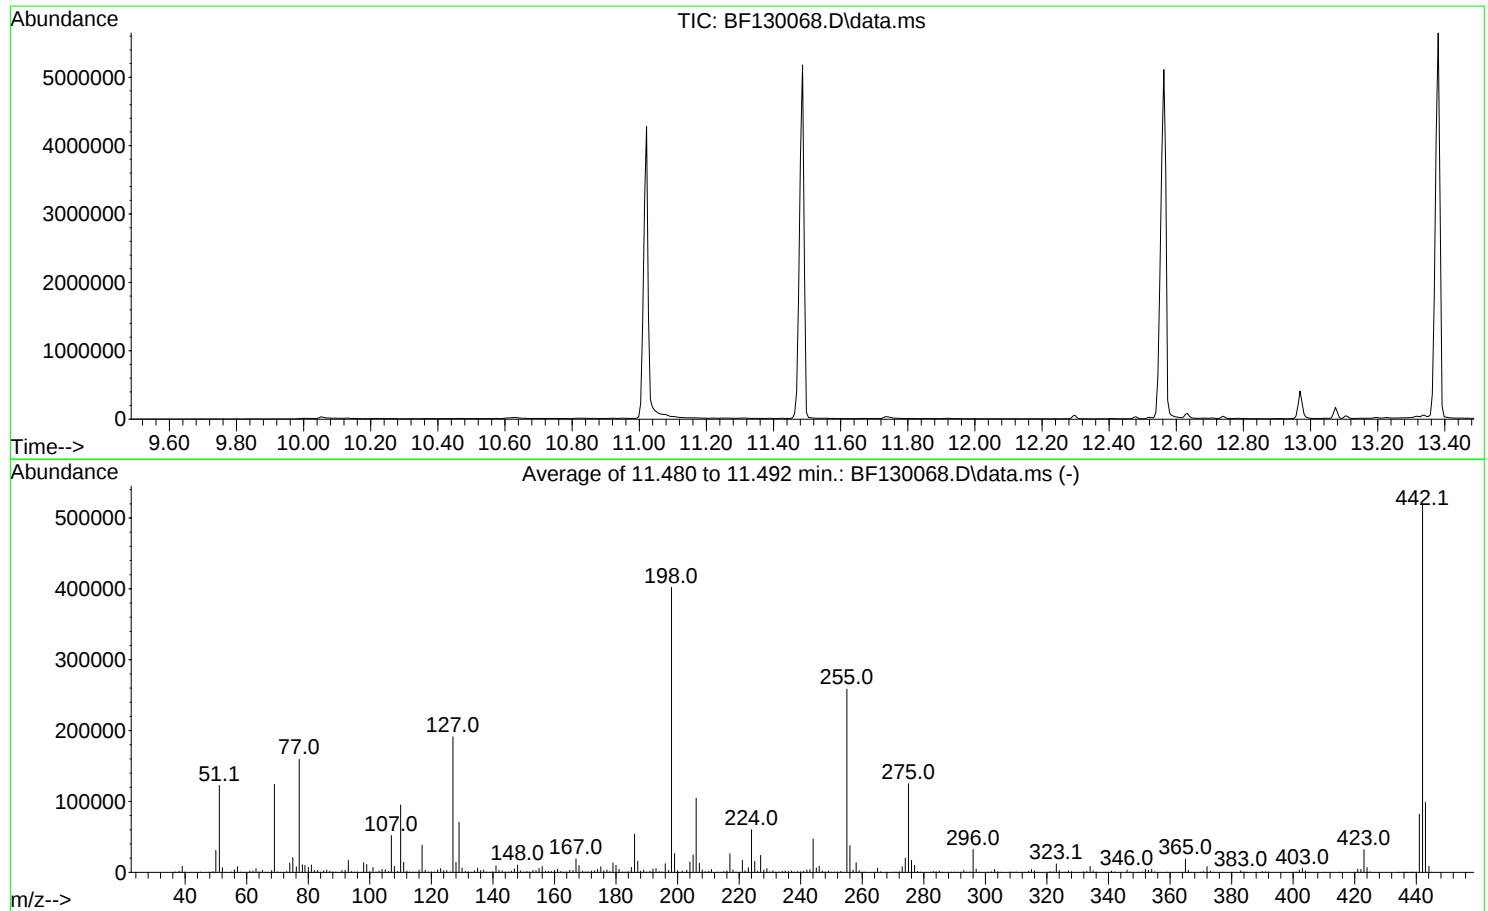


AutoFind: Scans 1563, 1564, 1565; Background Corrected with Scan 1556

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.5	122464	PASS
68	69	0.00	2	2.0	2449	PASS
69	198	0.00	100	30.9	124143	PASS
70	69	0.00	2	0.5	638	PASS
127	198	10	80	47.5	191168	PASS
197	198	0.00	2	0.7	2703	PASS
198	198	100	100	100.0	402048	PASS
199	198	5	9	6.6	26484	PASS
275	198	10	60	31.1	124968	PASS
365	198	1	100	4.6	18651	PASS
441	198	0.01	100	20.4	81936	PASS
442	442	50	100	100.0	519168	PASS
443	442	15	24	19.0	98667	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090122\
Data File : BF130068.D
Acq On : 01 Sep 2022 09:13
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 01 17:25:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 31 18:15:32 2022
Response via : Initial Calibration

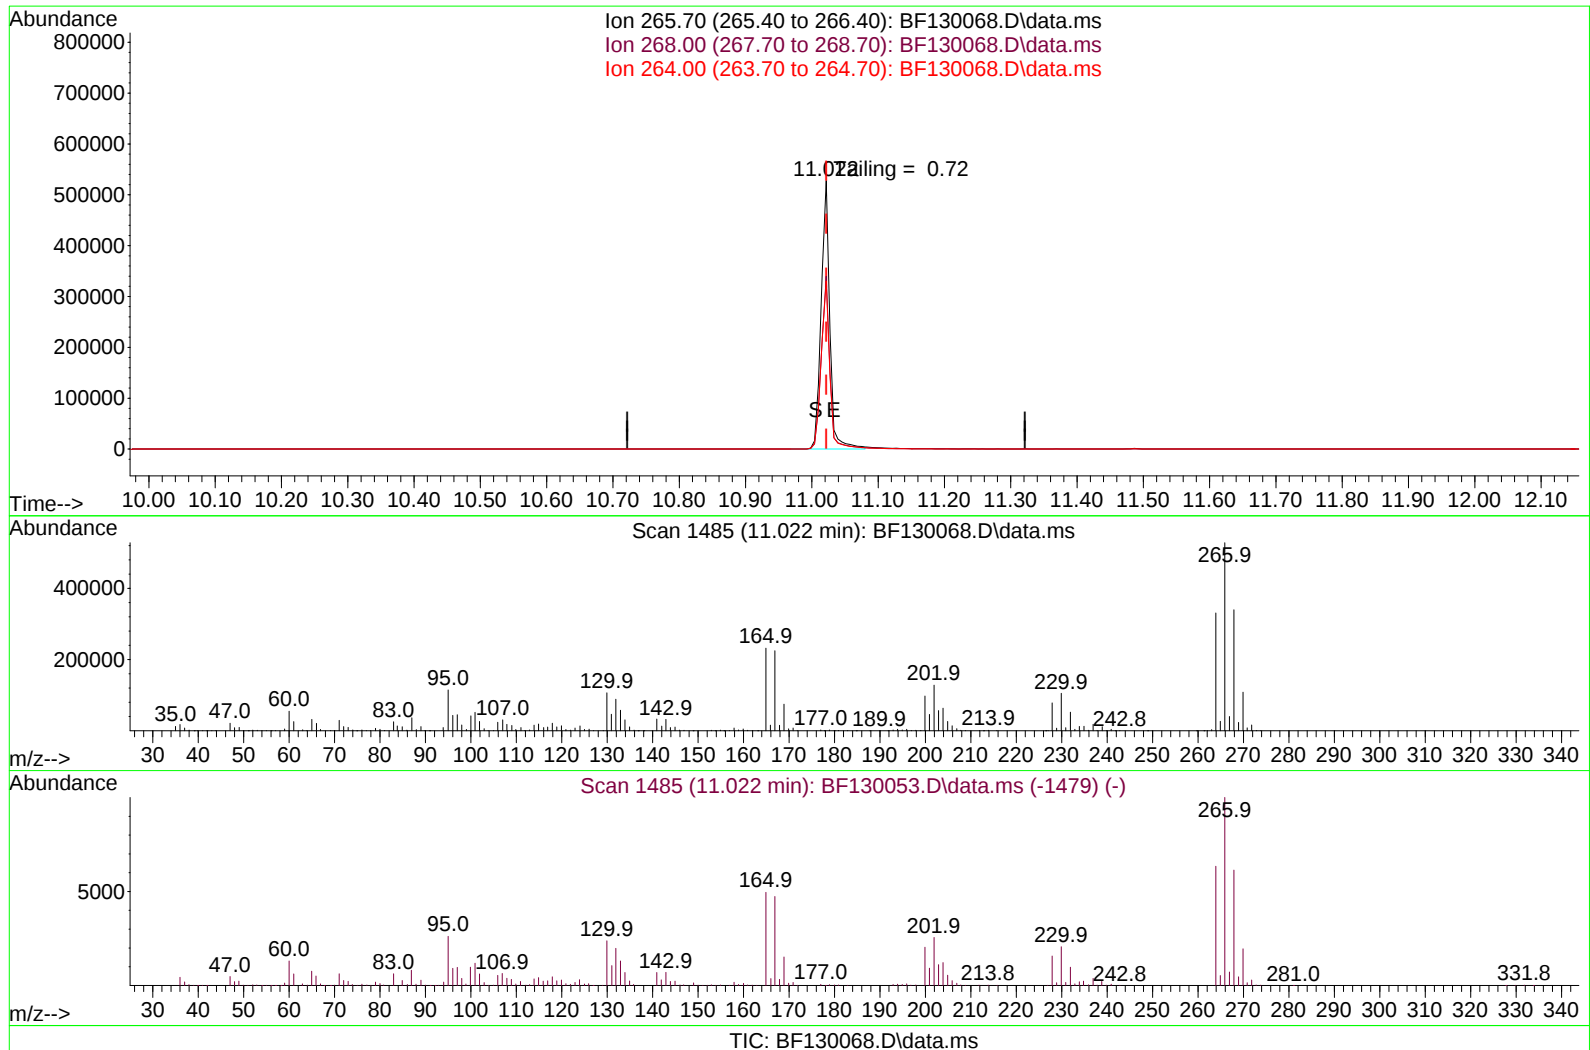

(70) Pentachlorophenol (C)

11.022min (+ 0.000) 256795.00 ng




response 487309

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	64.37
264.00	59.90	62.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090122\
 Data File : BF130068.D
 Acq On : 01 Sep 2022 09:13
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Sep 01 17:25:27 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 31 18:15:32 2022
 Response via : Initial Calibration

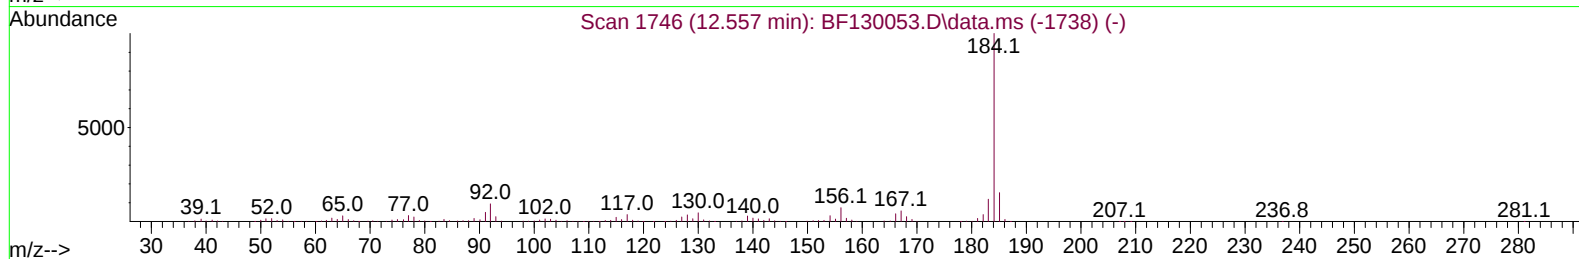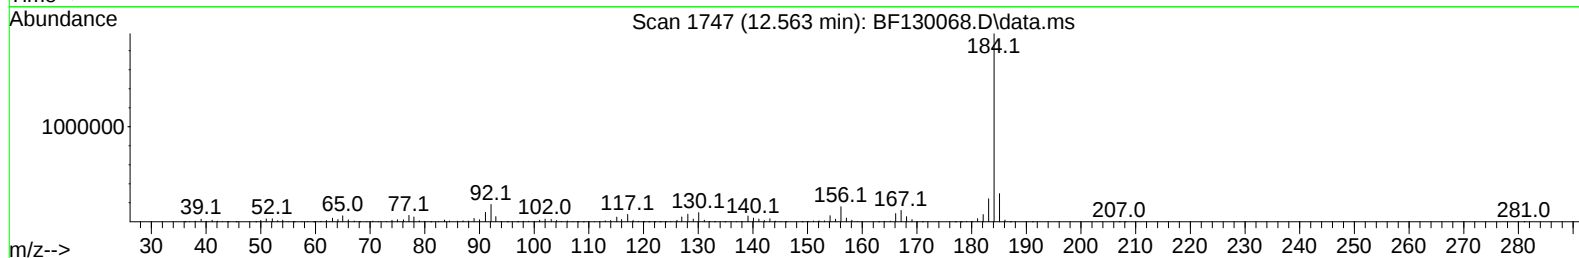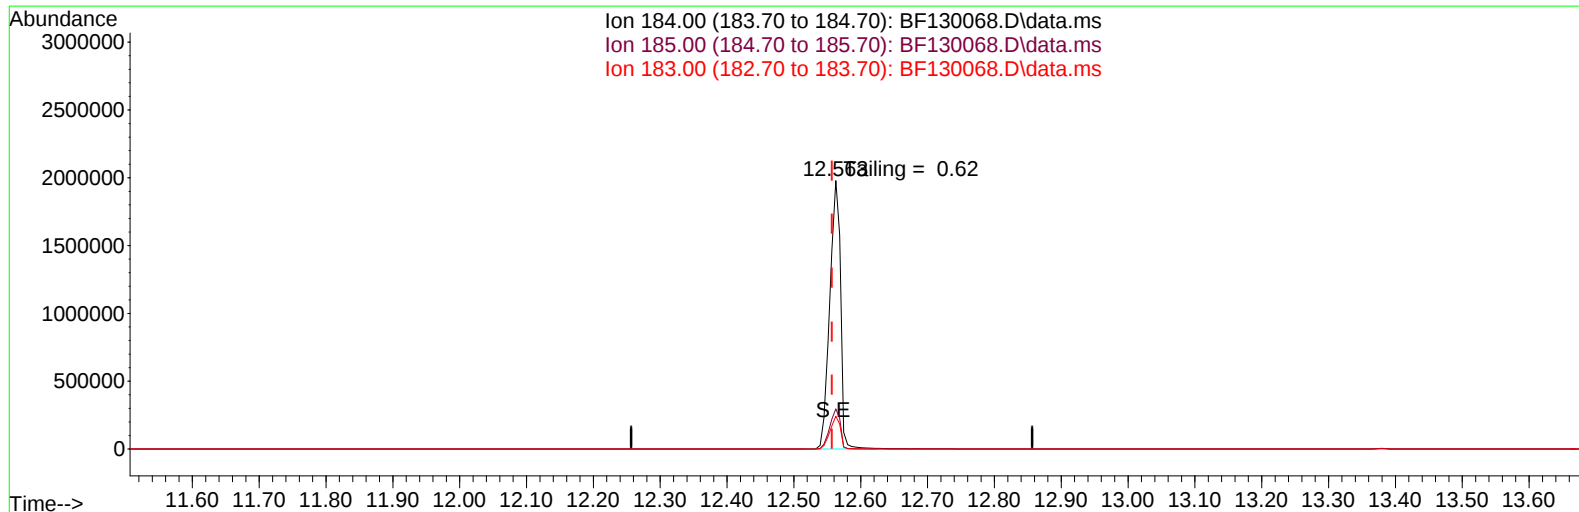

TIC: BF130068.D\data.ms

(77) Benzidine

12.563min (+ 0.006) 209128.26 ng

response 2230269

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	15.00
183.00	11.80	12.25
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/1/2022	BNA_F	<u>BF130068.D</u>
Compound Name	Response	Retention Time
DDT	995274	13.38
DDD	24088	13.07
DDE	3502	12.73
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
27590	1022864	2.70

Instrument :
BNA_F
ClientSampleId :
DFTPP