
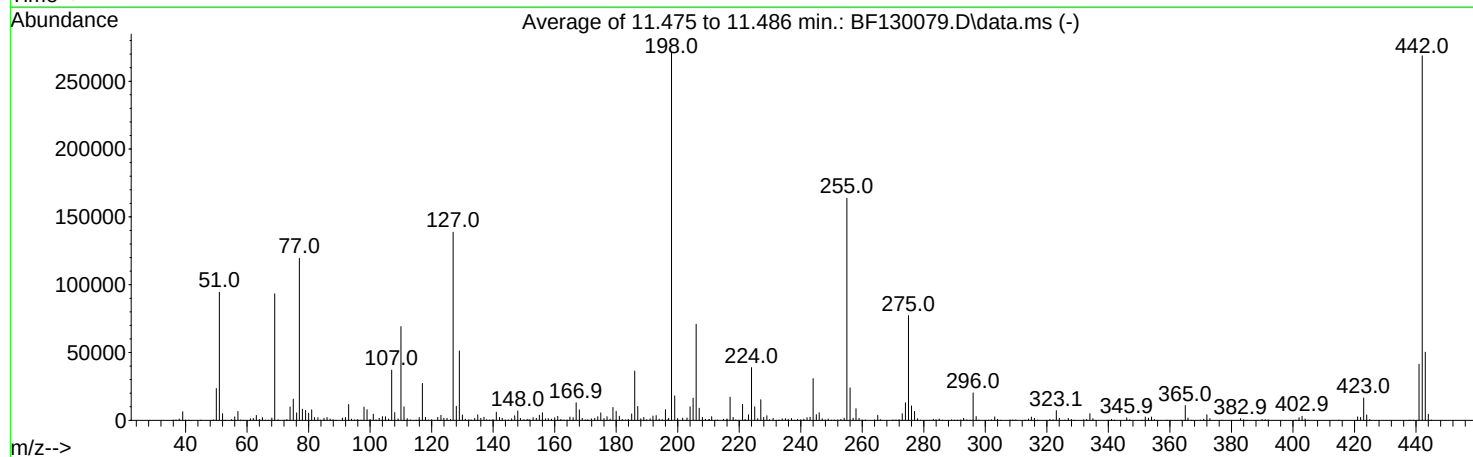


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090122\
 Data File : BF130079.D
 Acq On : 01 Sep 2022 15:53
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 31 18:15:32 2022

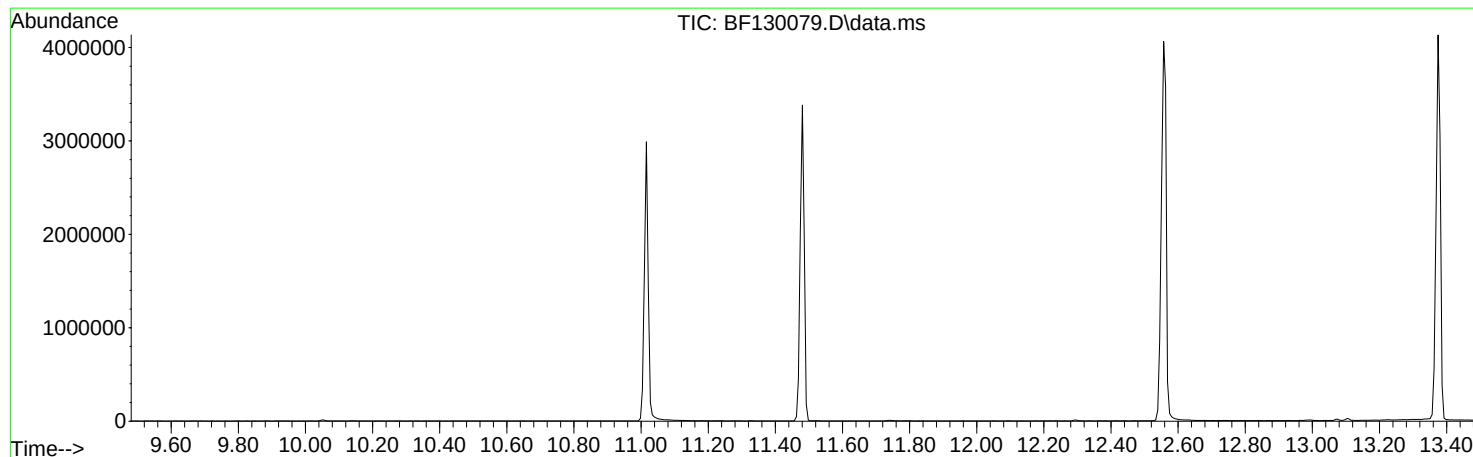




AutoFind: Scans 1562, 1563, 1564; Background Corrected with Scan 1556

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.8	94451	PASS
68	69	0.00	2	1.8	1689	PASS
69	198	0.00	100	34.4	93275	PASS
70	69	0.00	2	0.4	418	PASS
127	198	10	80	51.1	138704	PASS
197	198	0.00	2	0.6	1551	PASS
198	198	100	100	100.0	271275	PASS
199	198	5	9	6.7	18041	PASS
275	198	10	60	28.5	77291	PASS
365	198	1	100	4.0	10891	PASS
441	198	0.01	100	15.2	41349	PASS
442	442	50	100	100.0	268715	PASS
443	442	15	24	18.7	50248	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090122\
 Data File : BF130079.D
 Acq On : 01 Sep 2022 15:53
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Sep 02 05:06:15 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 31 18:15:32 2022
 Response via : Initial Calibration

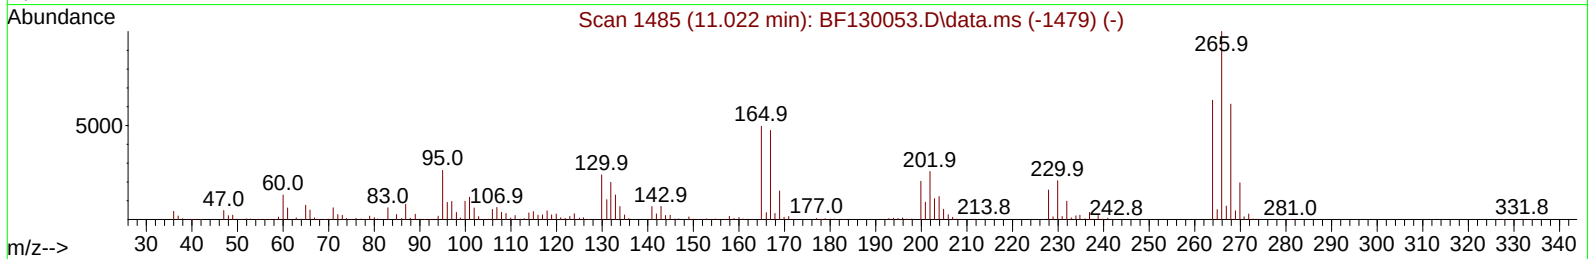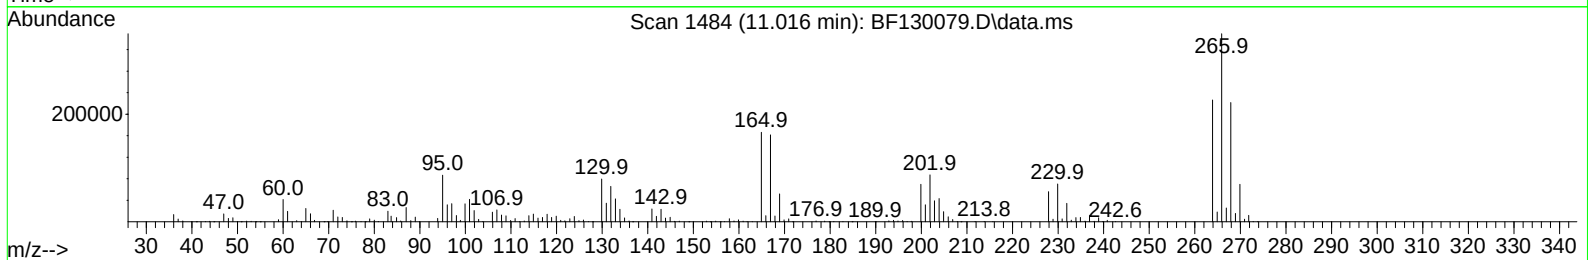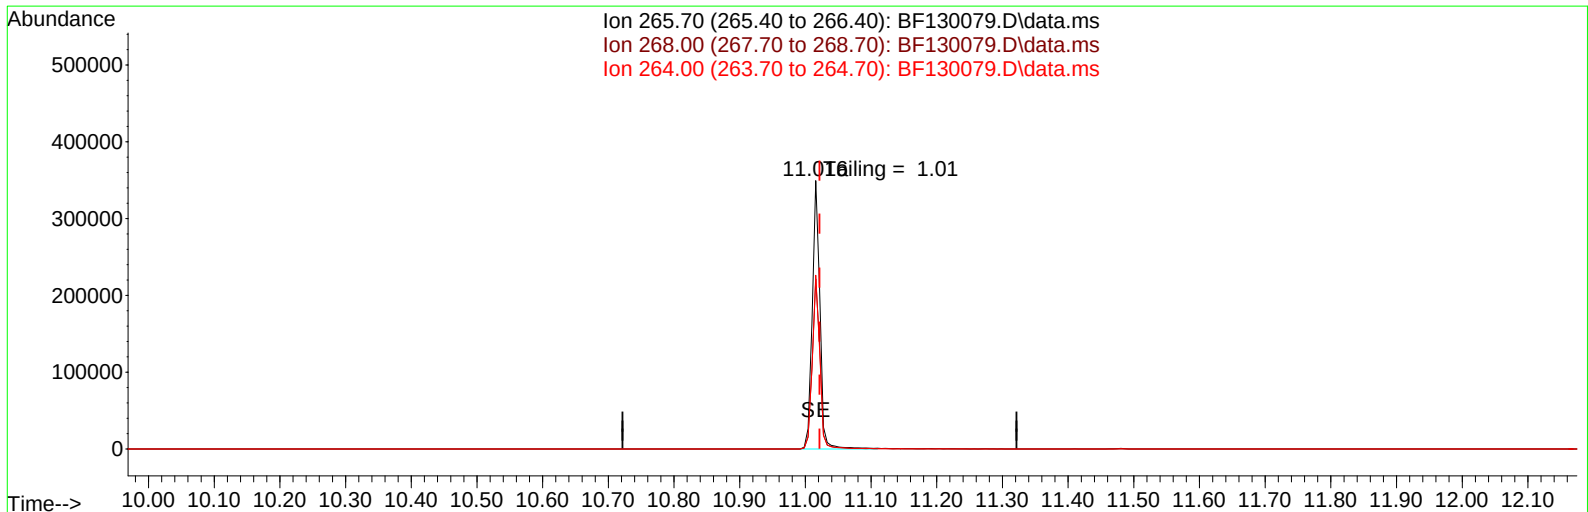

TIC: BF130079.D\data.ms

(70) Pentachlorophenol (C)

11.016min (-0.006) 526235.50 ng




response 288885

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	63.39
264.00	59.90	64.74
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090122\
Data File : BF130079.D
Acq On : 01 Sep 2022 15:53
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 02 05:06:15 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 31 18:15:32 2022
Response via : Initial Calibration

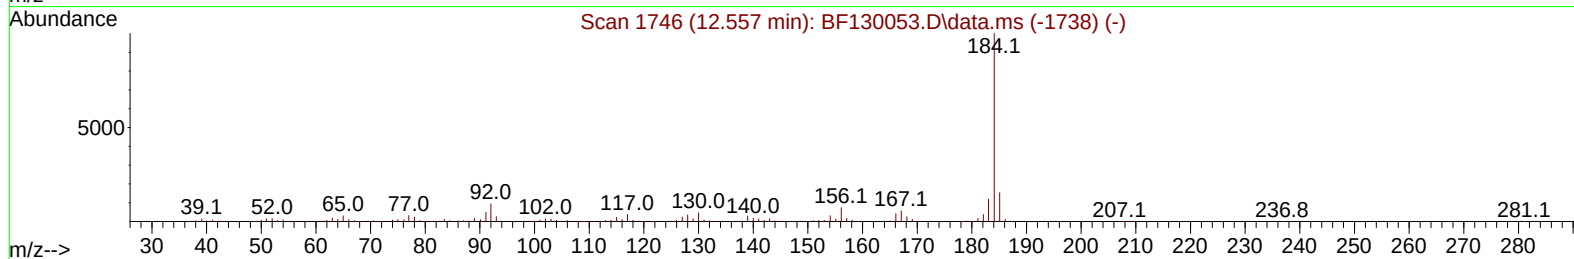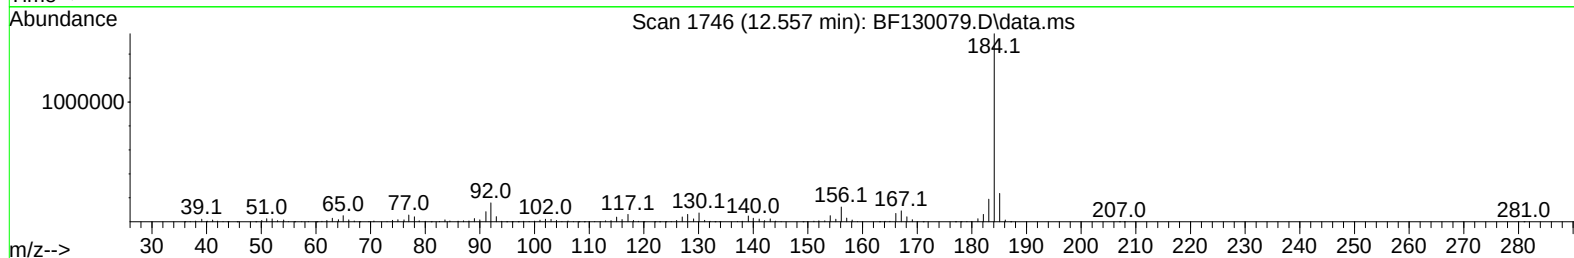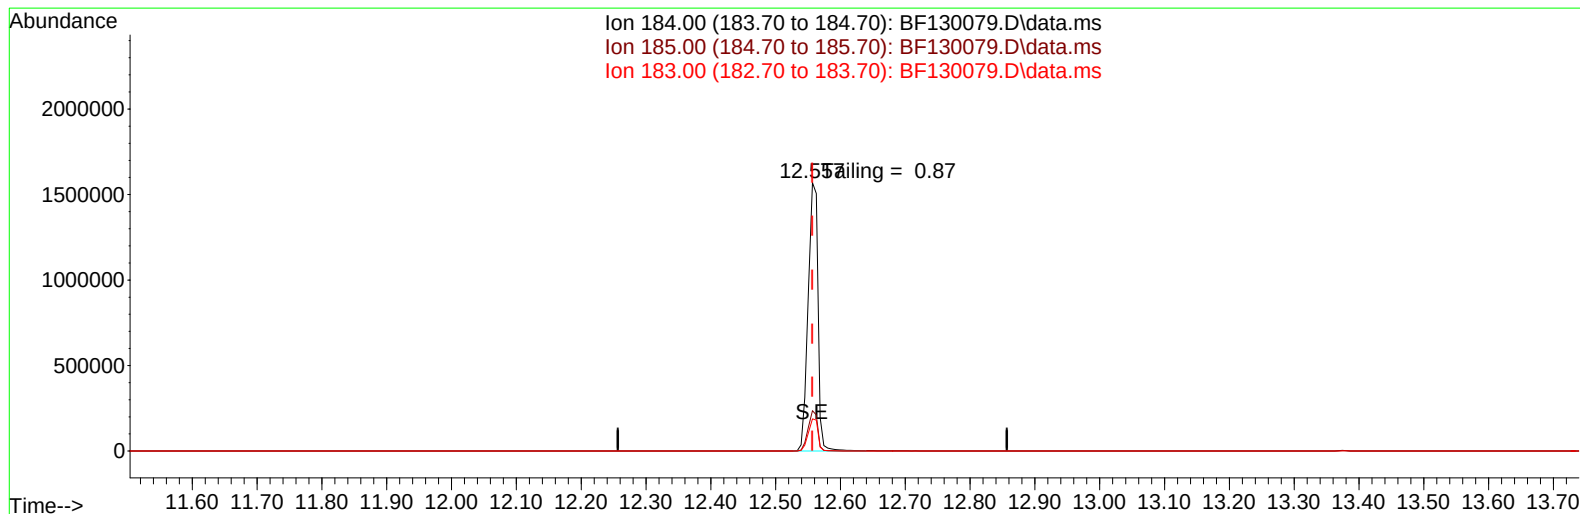

TIC: BF130079.D\data.ms

(77) Benzidine

12.557min (+ 0.000) 0.00 ng

response 1663952

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	15.07
183.00	11.80	11.98
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/1/2022	BNA_F	BF130079.D
Compound Name	Response	Retention Time
DDT	690765	13.374
DDD	6174	13.104
DDE	238	12.739
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6412	697177	0.92

Instrument :
BNA_F
ClientSampleId :
DFTPP