
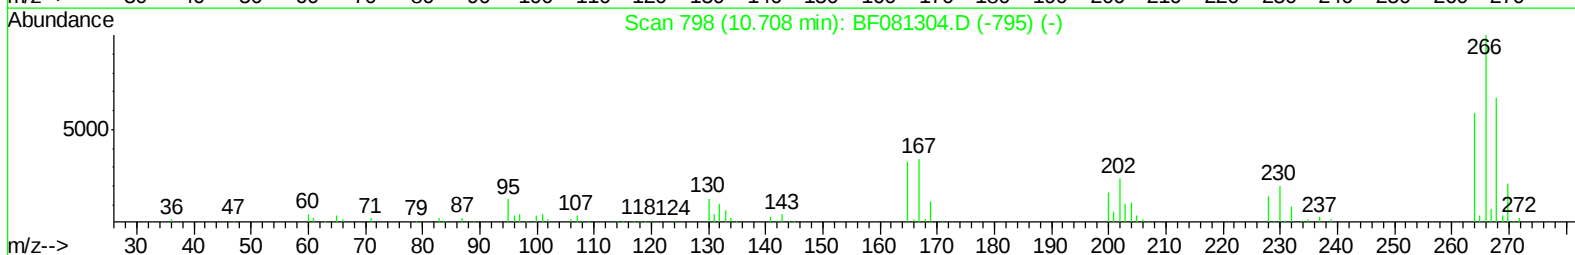
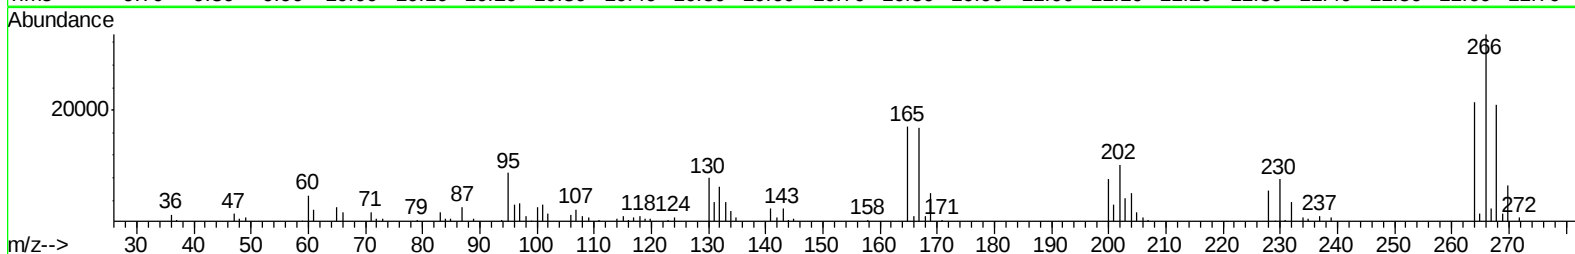


Data Path : Z:\HPCHEM1\BNA F\DATA\BF090215\
Data File : BF081337.D
Acq On : 2 Sep 2015 9:07
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 03 04:20:37 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF090115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 01 17:35:35 2015
Response via : Initial Calibration

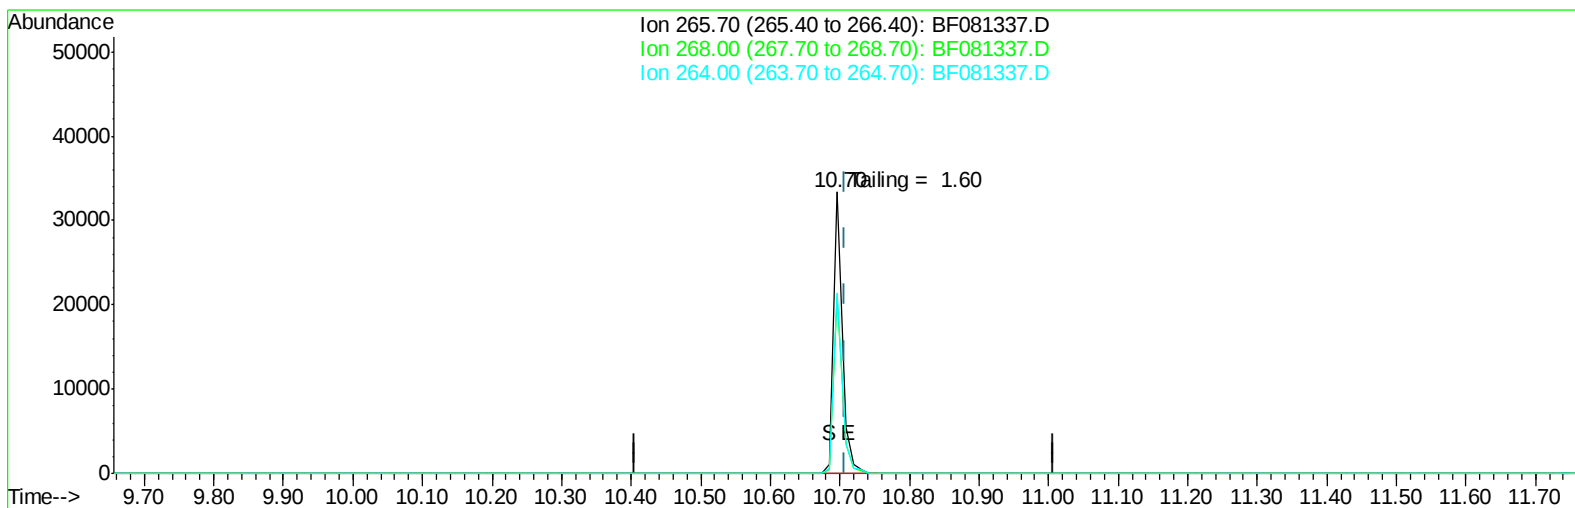

TIC: BF081337.D

(69) Pentachlorophenol (C)




10.696min (-0.011) 0.00ng

response 28478

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	62.68
264.00	62.70	64.29
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF090215\
Data File : BF081337.D
Acq On : 2 Sep 2015 9:07
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 03 04:20:37 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF090115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 01 17:35:35 2015
Response via : Initial Calibration

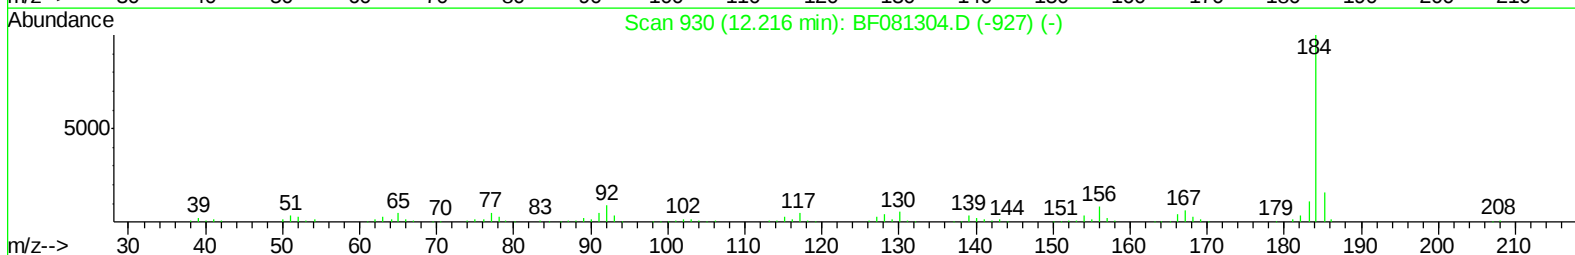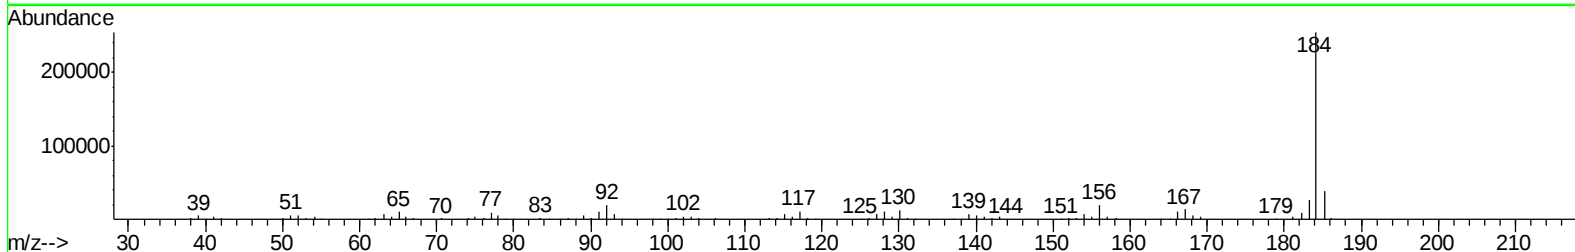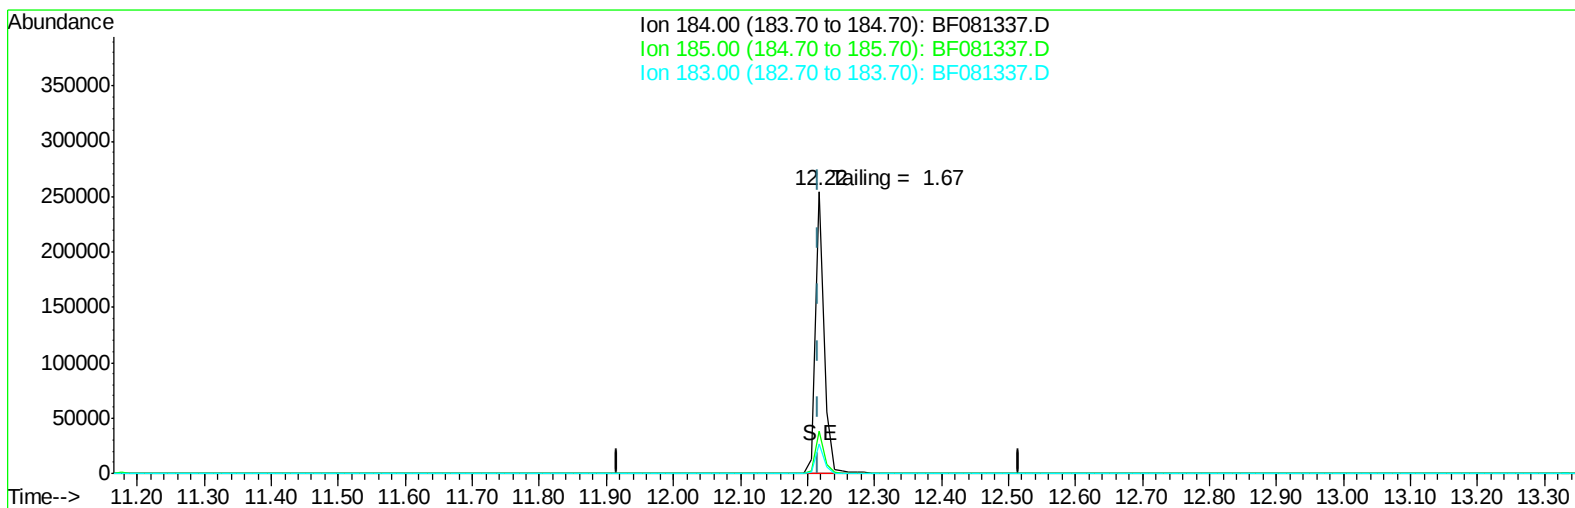

TIC: BF081337.D

(76) Benzidine

12.217min (+0.000) 0.00ng

response 228345

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	14.93
183.00	9.50	10.54
0.00	0.00	0.00