
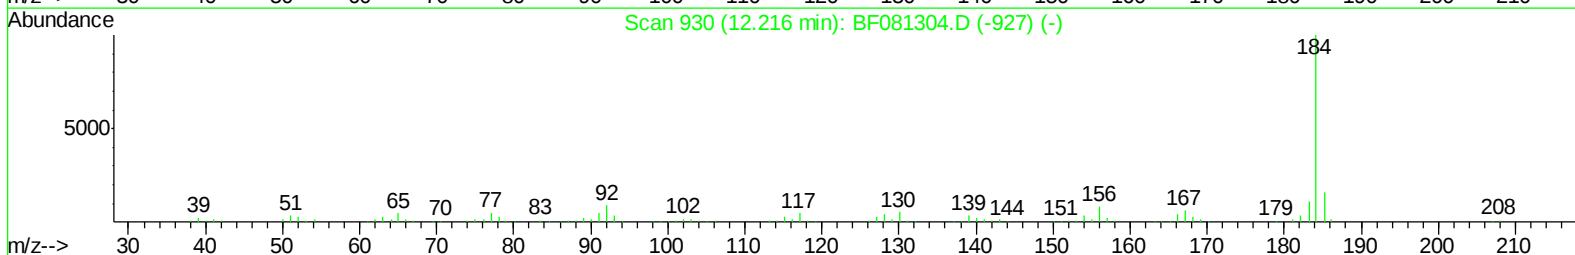
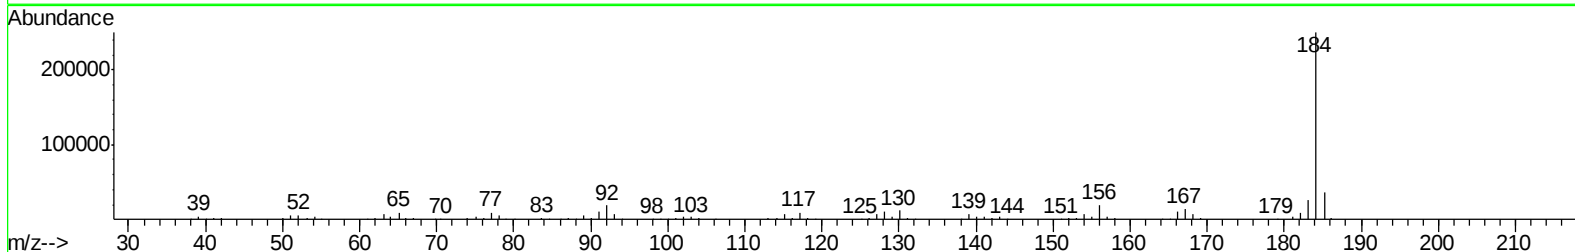


Data Path : Z:\HPCHEM1\BNA F\DATA\BF090215\
 Data File : BF081356.D
 Acq On : 2 Sep 2015 19:10
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 03 04:29:04 2015
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF090115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 01 17:35:35 2015
 Response via : Initial Calibration

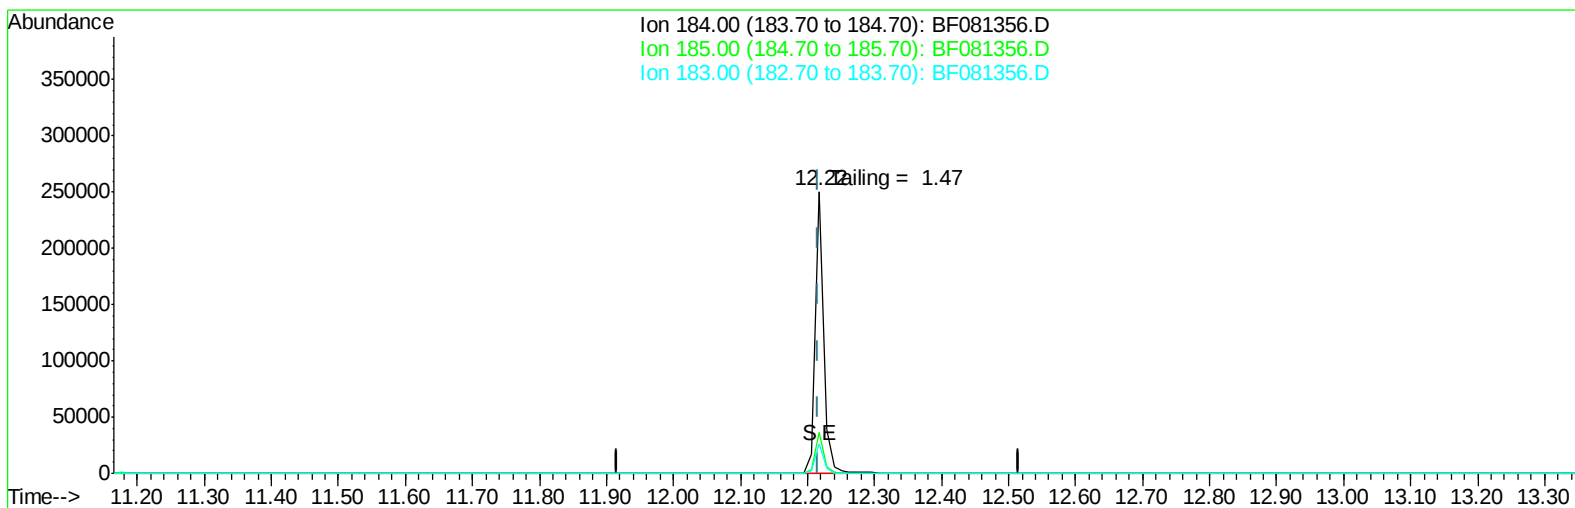

TIC: BF081356.D

(76) Benzidine




12.216min (+0.000) 0.00ng

response 219935

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	14.74
183.00	9.50	10.52
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF090215\
Data File : BF081356.D
Acq On : 2 Sep 2015 19:10
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 03 04:29:04 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF090115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 01 17:35:35 2015
Response via : Initial Calibration

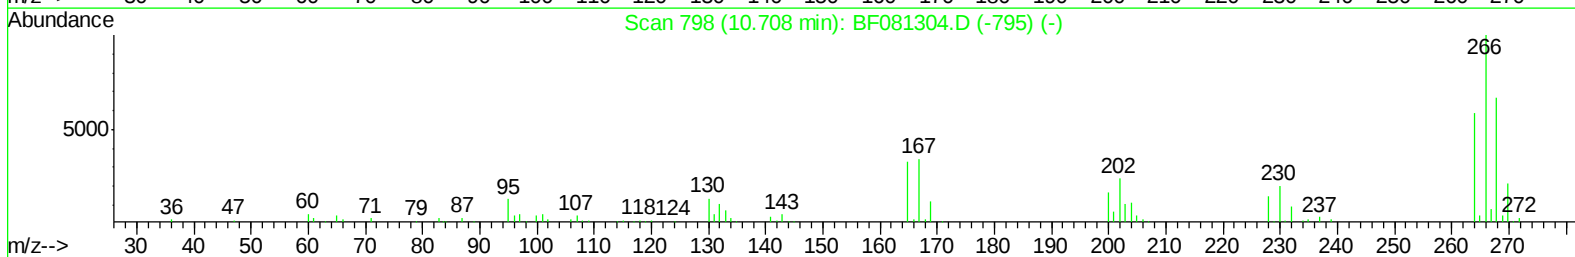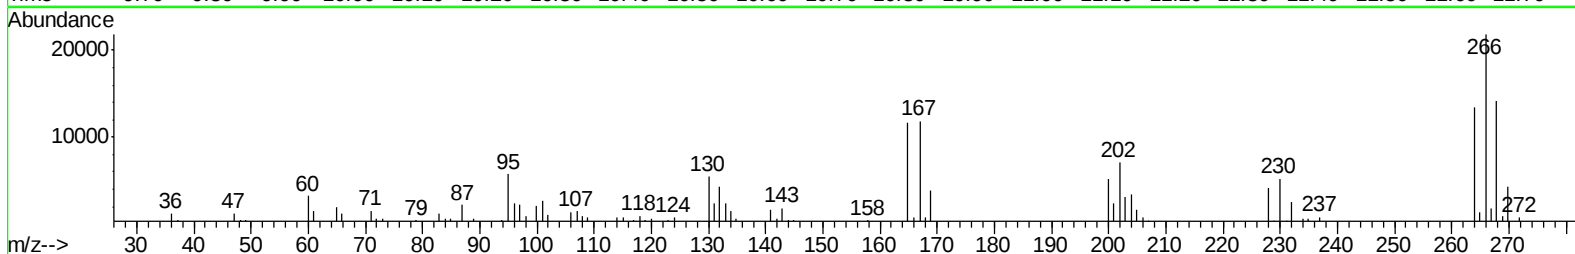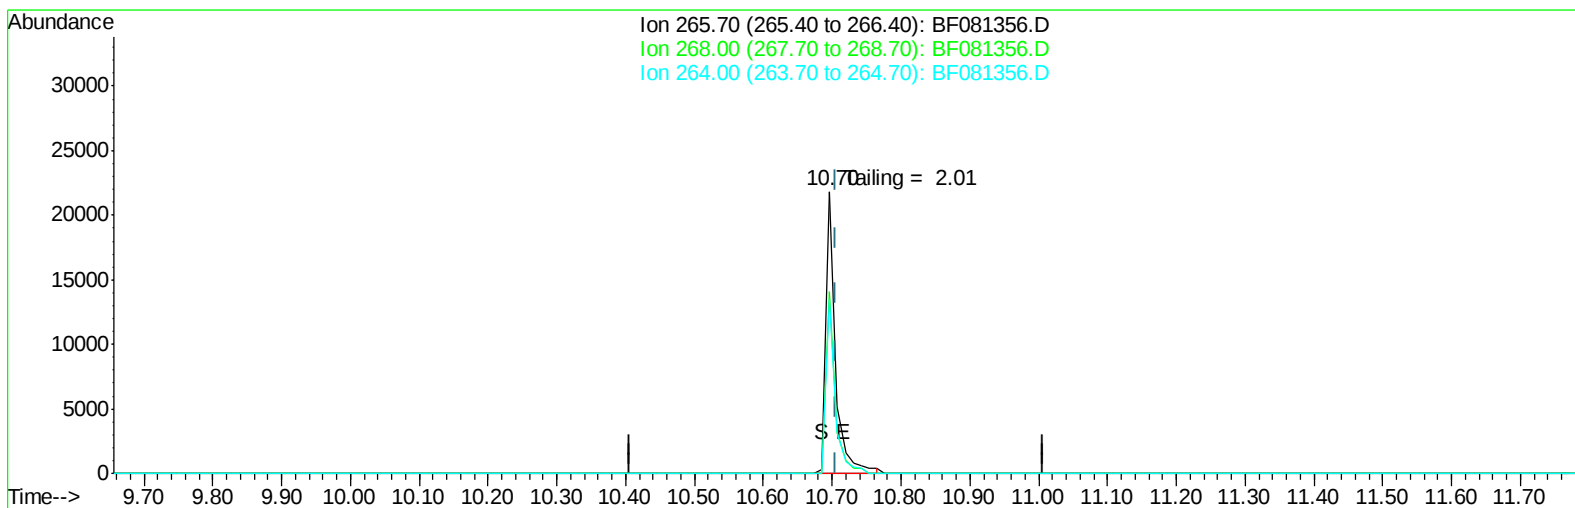

TIC: BF081356.D

(69) Pentachlorophenol (C)

10.696min (-0.011) 0.00ng

response 21295

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	64.59
264.00	62.70	61.73
0.00	0.00	0.00