


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF090215\
 Data File : BF081337.D
 Acq On : 2 Sep 2015 9:07
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF090115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 01 17:35:35 2015

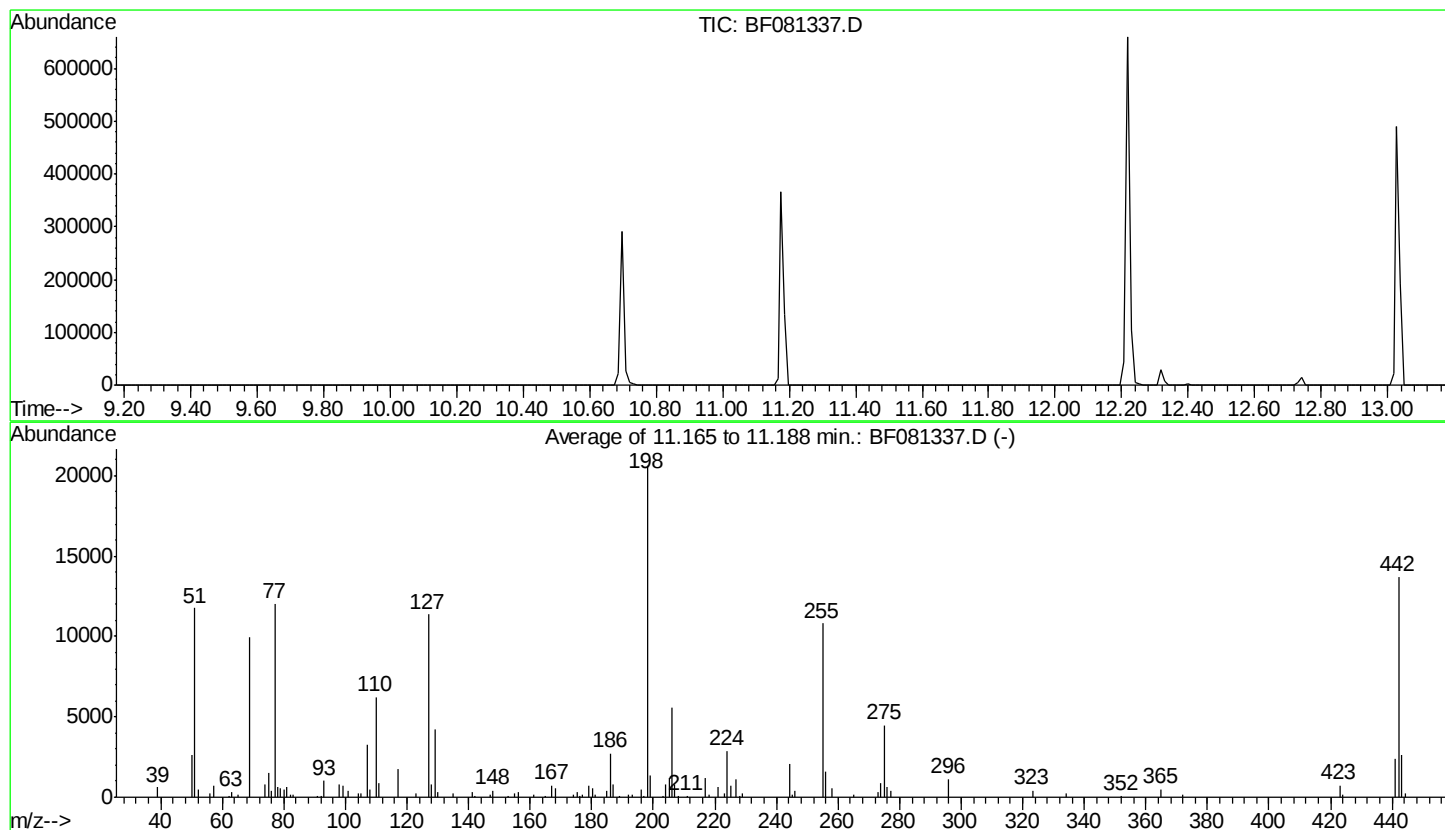

AutoFind: Scans 838, 839, 840; Background Corrected with Scan 835

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.1	11785	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	48.2	9946	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	55.0	11353	PASS
197	198	0.00	2	0.6	119	PASS
198	198	100	100	100.0	20628	PASS
199	198	5	9	6.6	1357	PASS
275	198	10	60	21.7	4475	PASS
365	198	1	100	2.5	520	PASS
441	442	0.01	24	17.6	2407	PASS
442	198	50	100	66.5	13709	PASS
443	442	15	24	19.1	2621	PASS