

Data Path : Z:\HPCHEM1\BNA F\DATA\BF090216\
 Data File : BF089977.D
 Acq On : 2 Sep 2016 16:15
 Operator : UM/SJ
 Sample : H4675-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Sep 02 17:31:49 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF083116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 02 13:29:08 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.64	152	188320	20.00	ng	0.00
21) Naphthalene-d8	7.92	136	706645	20.00	ng	-0.01
38) Acenaphthene-d10	9.67	164	357721	20.00	ng	0.00
63) Phenanthrene-d10	11.13	188	588860	20.00	ng	-0.01
75) Chrysene-d12	13.75	240	479900	20.00	ng	-0.01
86) Perylene-d12	15.10	264	424268	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.22	112	1301972	110.66	ng	0.01
7) Phenol-d6	6.28	99	1664247	116.41	ng	0.00
23) Nitrobenzene-d5	7.20	82	821085	67.39	ng	-0.01
41) 2,4,6-Tribromophenol	10.44	330	320568	90.83	ng	-0.01
44) 2-Fluorobiphenyl	9.00	172	1647582	75.61	ng	0.00
78) Terphenyl-d14	12.72	244	1287758	66.29	ng	-0.01
Target Compounds						
19) n-Nitroso-di-n-propylamine	7.20	70	107542	11.54	ng	# 83
25) Isophorone	7.20	82	684326	27.62	ng	# 65
49) Dimethylphthalate	9.39	163	798100	30.87	ng	100
56) 2,4-Dinitrotoluene	9.67	165	45715	6.27	ng	# 29
66) 4-Bromophenyl-phenylether	10.44	248	21444	3.62	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF090216\
Data File : BF089977.D
Acq On : 2 Sep 2016 16:15
Operator : UM/SJ
Sample : H4675-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Sep 02 17:31:49 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF083116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 02 13:29:08 2016
Response via : Initial Calibration

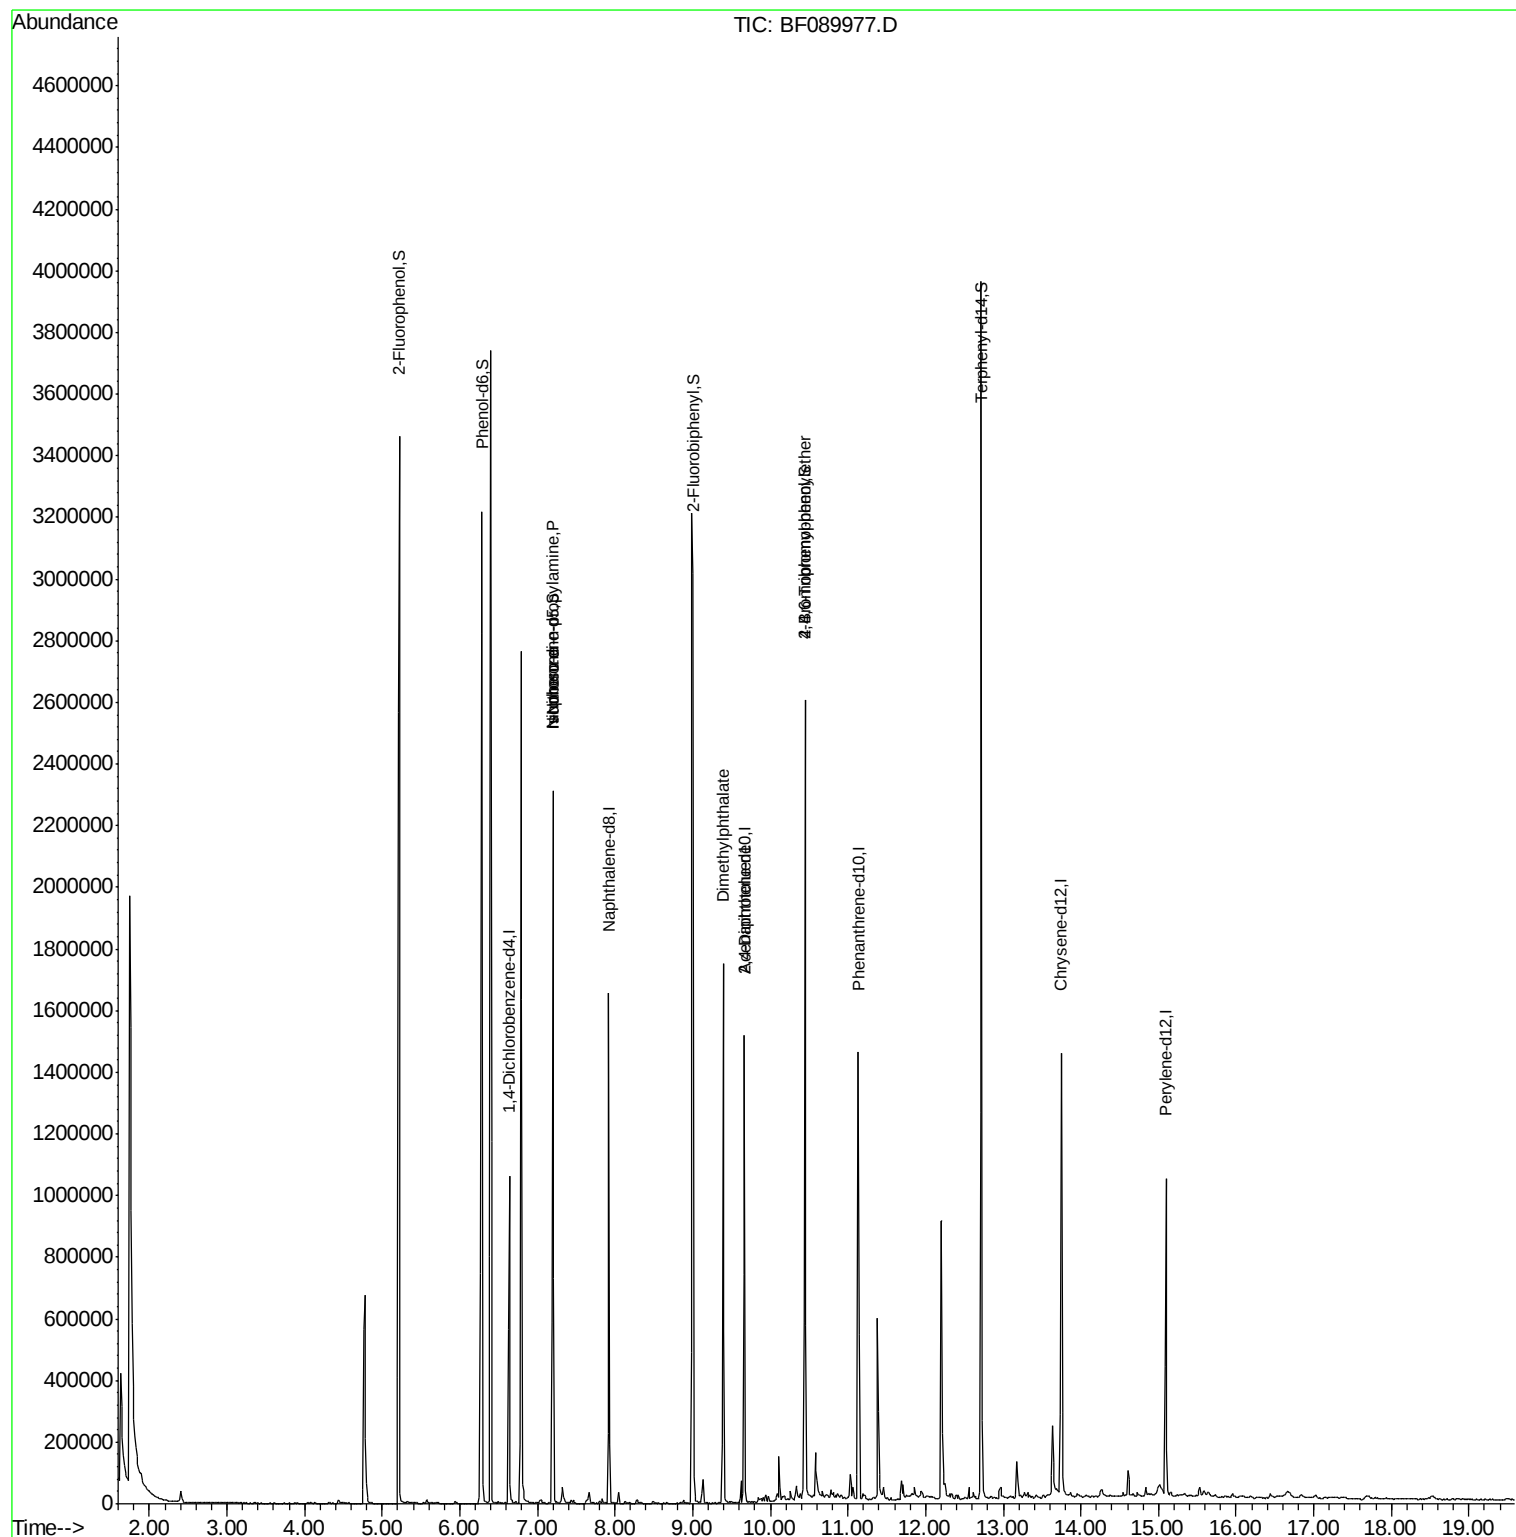

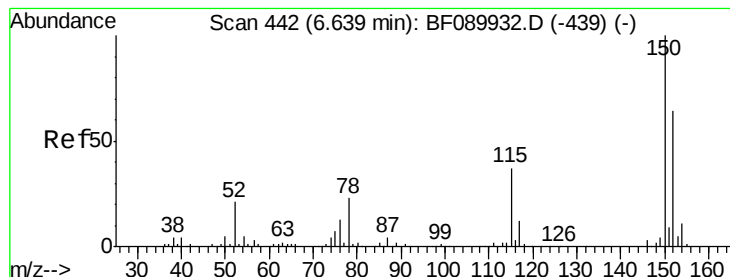

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.64 min Scan# 442

Delta R.T. 0.00 min

Lab File: BF089977.D

Acq: 2 Sep 2016 16:15

Instrument :

BNA_F

ClientSampleId :


Tot Ion:152 Resp: 188320

Ion Ratio Lower Upper

152 100

150 152.2 127.4 191.2




115 51.9 46.3 69.5

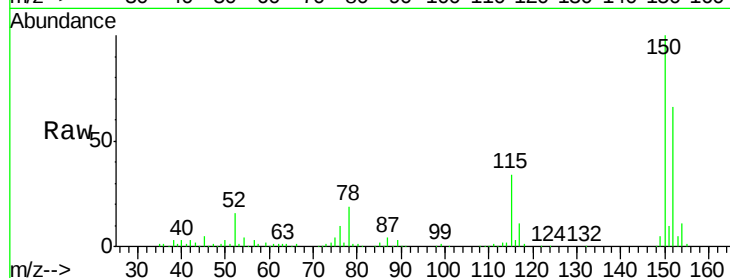

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

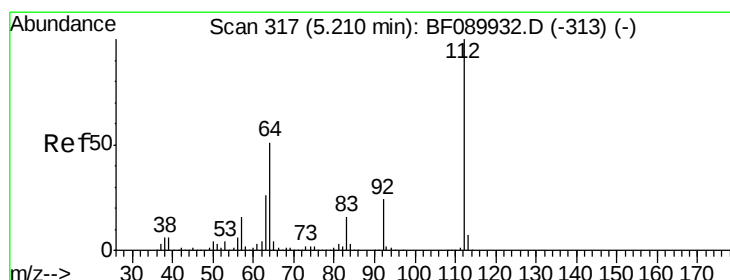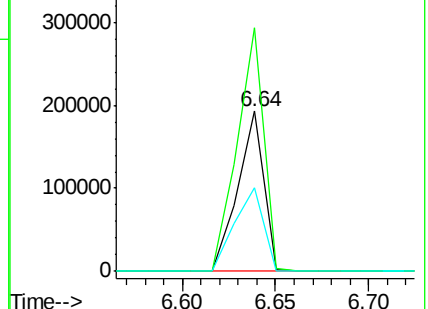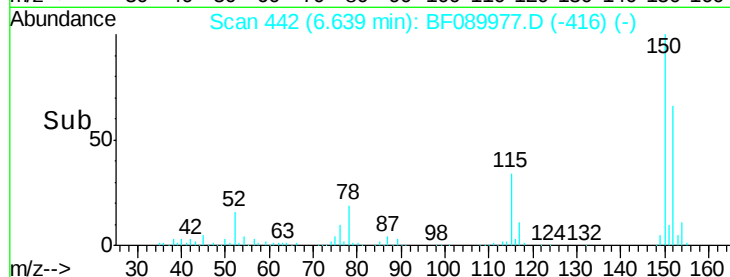

#5

2-Fluorophenol

Concen: 110.66 ng

RT: 5.22 min Scan# 318

Delta R.T. 0.01 min

Lab File: BF089977.D

Acq: 2 Sep 2016 16:15


Tgt Ion:112 Resp: 1301972

Ion Ratio Lower Upper

112 100

64 53.2 41.1 61.7



63 27.8 21.2 31.8



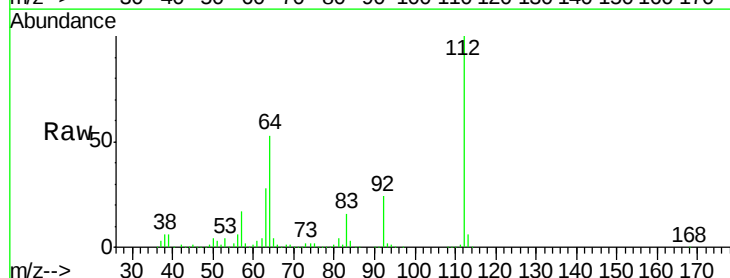


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

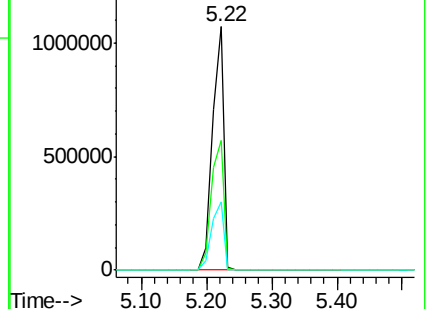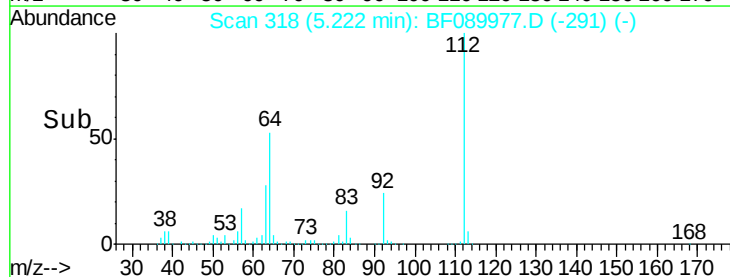

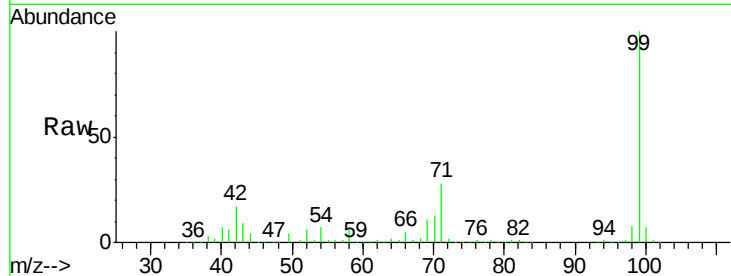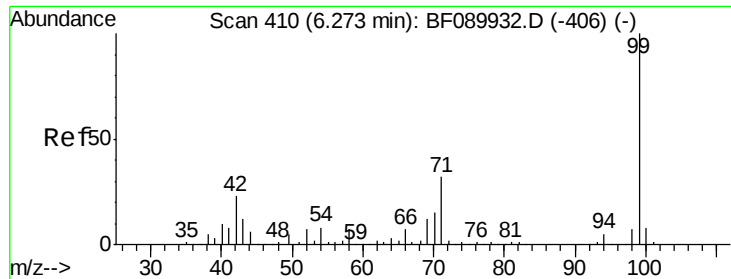

#7

Phenol-d6

Concen: 116.41 ng

RT: 6.28 min Scan# 411

Delta R.T. 0.00 min

Lab File: BF089977.D

Acq: 2 Sep 2016 16:15





Instrument :

BNA_F

ClientSampleId :

Tot Ion: 99 Resp: 1664247

Ion	Ratio	Lower	Upper
99	100		
42	17.0	18.6	27.8#
71	28.5	25.8	38.6

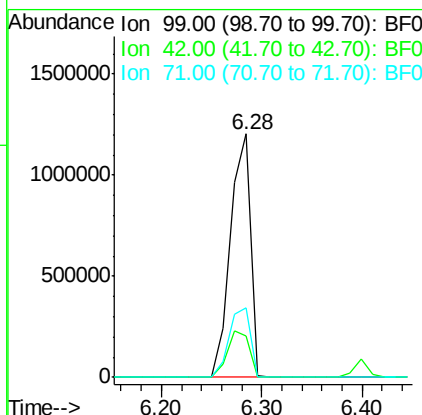

#19

n-Nitroso-di-n-propylamine

Concen: 11.54 ng

RT: 7.20 min Scan# 491


Delta R.T. 0.13 min


Lab File: BF089977.D

Acq: 2 Sep 2016 16:15

Tgt Ion: 70 Resp: 107542

Ion	Ratio	Lower	Upper
70	100		
42	58.1	52.1	78.1
101	0.0	7.4	11.2#
130	2.1	17.0	25.4#

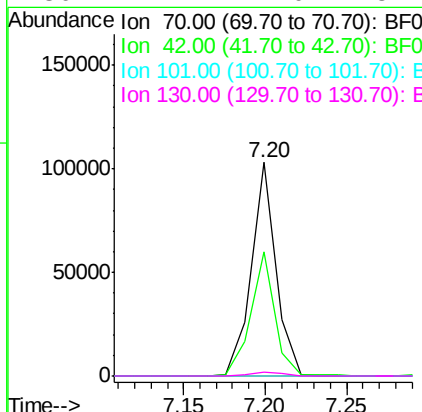



#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.92 min Scan# 554

Delta R.T. -0.01 min

Lab File: BF089977.D

Acq: 2 Sep 2016 16:15

Instrument :

BNA_F

ClientSampleId :

Tot Ion:136 Resp: 706645


Ion Ratio Lower Upper

136 100

137 11.2 8.3 12.5

54 9.5 4.8 7.2#

68 6.7 3.7 5.5#



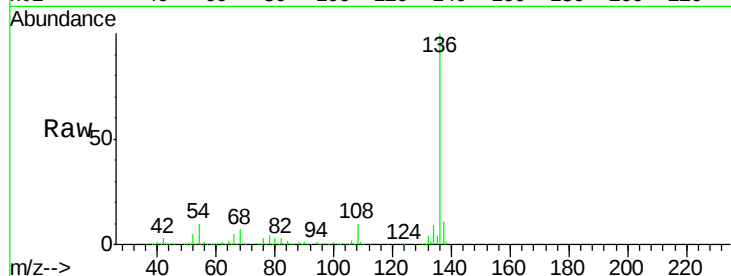


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

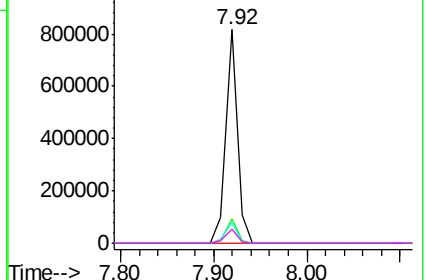

#23

Nitrobenzene-d5

Concen: 67.39 ng

RT: 7.20 min Scan# 491

Delta R.T. -0.01 min

Lab File: BF089977.D

Acq: 2 Sep 2016 16:15


Tgt Ion: 82 Resp: 821085

Ion Ratio Lower Upper

82 100

128 44.8 37.8 56.8



54 60.8 46.9 70.3




Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF0

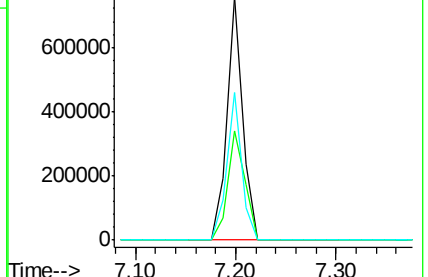

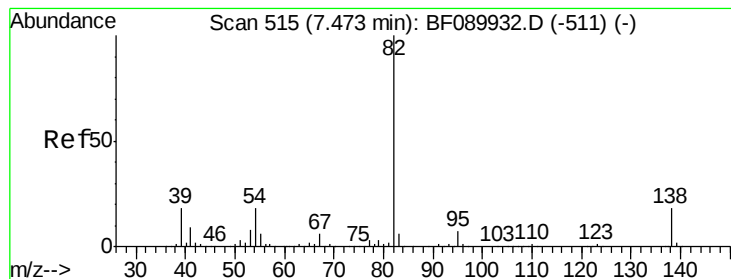

#25

Isophorone

Concen: 27.62 ng

RT: 7.20 min Scan# 491

Delta R.T. -0.27 min

Lab File: BF089977.D

Acq: 2 Sep 2016 16:15

Instrument :

BNA_F

ClientSampled :


Tot Ion: 82 Resp: 684326

Ion Ratio Lower Upper




82 100

95 0.0 5.5 8.3#

138 0.0 14.4 21.6#



Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 95.00 (94.70 to 95.70): BF0
Ion 138.00 (137.70 to 138.70): BF0

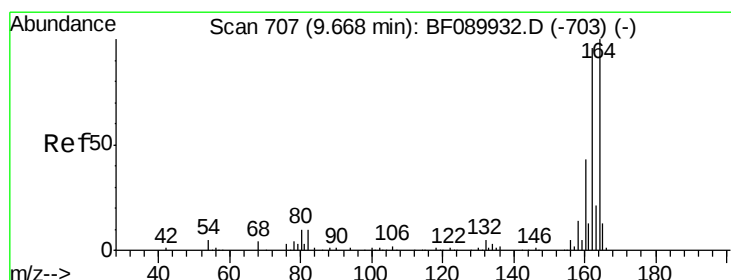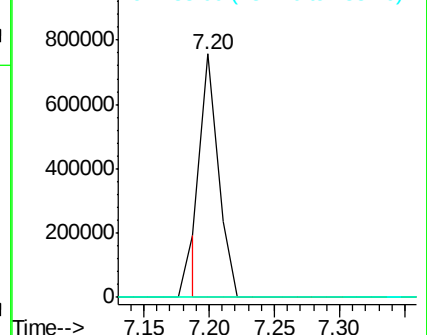

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.67 min Scan# 707

Delta R.T. 0.00 min

Lab File: BF089977.D

Acq: 2 Sep 2016 16:15


Tgt Ion:164 Resp: 357721

Ion Ratio Lower Upper



164 100


162 99.4 77.1 115.7

160 45.2 35.3 52.9



Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

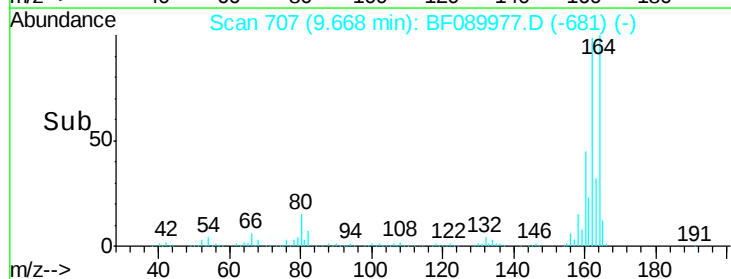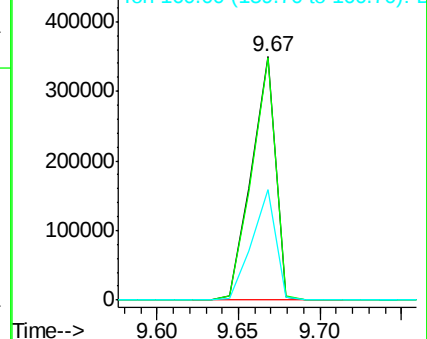







#41
 2,4,6-Tribromophenol
 Concen: 90.83 ng
 RT: 10.44 min Scan# 775
 Delta R.T. -0.01 min
 Lab File: BF089977.D
 Acq: 2 Sep 2016 16:15

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
330	100		
332	97.2	78.6	117.8
141	34.3	23.3	34.9

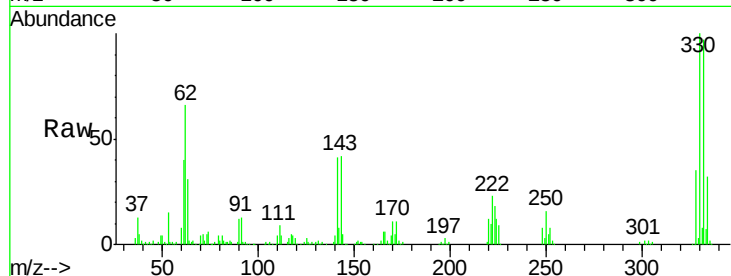


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E


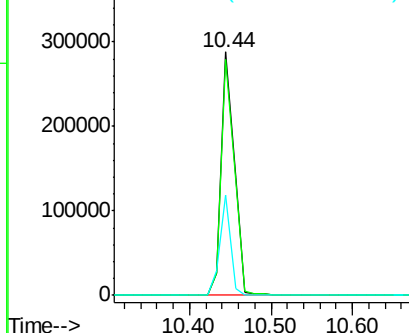



#44
 2-Fluorobiphenyl
 Concen: 75.61 ng
 RT: 9.00 min Scan# 649
 Delta R.T. 0.00 min
 Lab File: BF089977.D
 Acq: 2 Sep 2016 16:15

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.5	29.4	44.2
170	24.3	20.1	30.1



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E




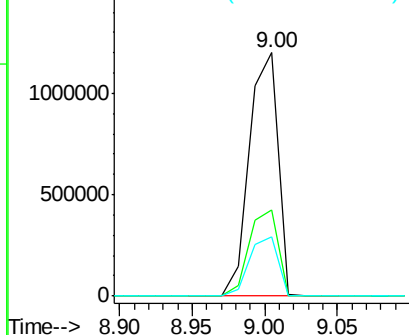




#49
Dimethylphthalate
Concen: 30.87 ng
RT: 9.39 min Scan# 683
Delta R.T. -0.02 min
Lab File: BF089977.D
Acq: 2 Sep 2016 16:15




Instrument :
BNA_F
ClientSampled :


Tot Ion:163 Resp: 798100
Ion Ratio Lower Upper
163 100
194 3.4 2.7 4.1
164 11.3 9.0 13.4

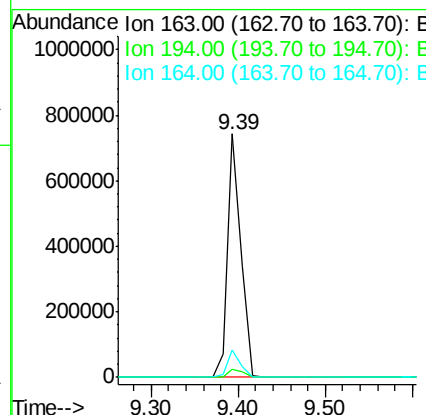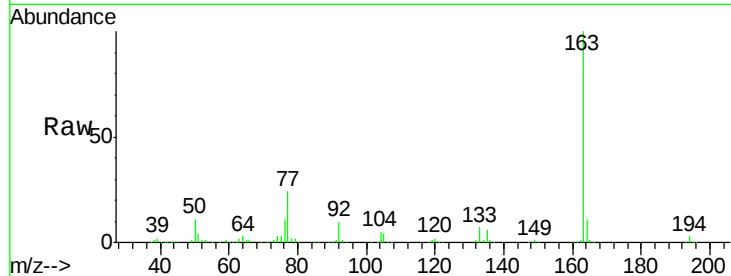

#56
2,4-Dinitrotoluene
Concen: 6.27 ng
RT: 9.67 min Scan# 707
Delta R.T. -0.19 min
Lab File: BF089977.D
Acq: 2 Sep 2016 16:15

Tgt Ion:165 Resp: 45715
Ion Ratio Lower Upper
165 100
63 1.4 32.5 48.7#
89 1.3 48.3 72.5#
182 0.0 1.7 2.5#

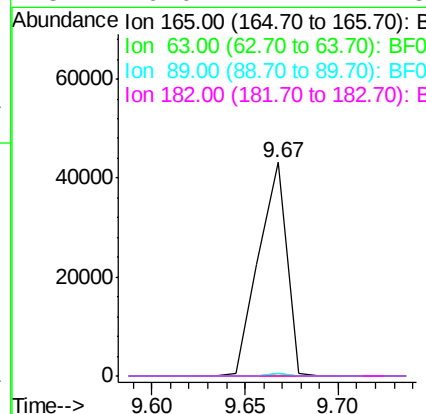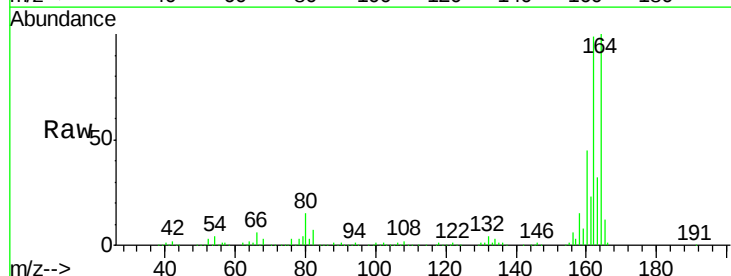







#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.13 min Scan# 835
Delta R.T. -0.01 min
Lab File: BF089977.D
Acq: 2 Sep 2016 16:15

Instrument :
BNA_F
ClientSampleId :

Tot Ion:188 Resp: 588860
Ion Ratio Lower Upper
188 100
94 11.5 5.9 8.9#
80 12.5 5.8 8.8#

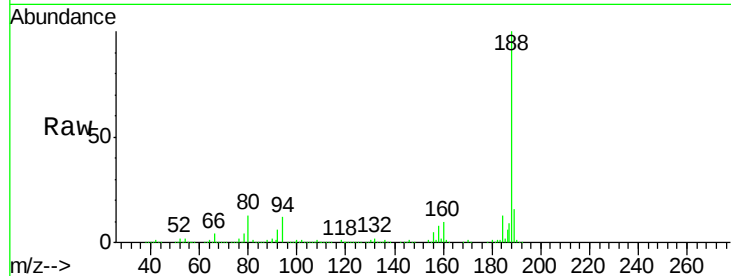


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0


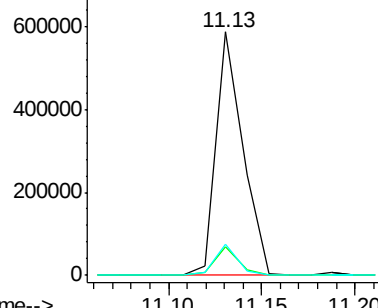



#66
4-Bromophenyl-phenylether
Concen: 3.62 ng
RT: 10.44 min Scan# 775
Delta R.T. -0.25 min
Lab File: BF089977.D
Acq: 2 Sep 2016 16:15

Tgt Ion:248 Resp: 21444
Ion Ratio Lower Upper
248 100
250 197.2 77.3 115.9#
141 520.4 55.8 83.8#



Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E

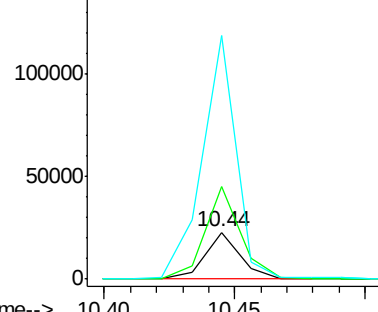

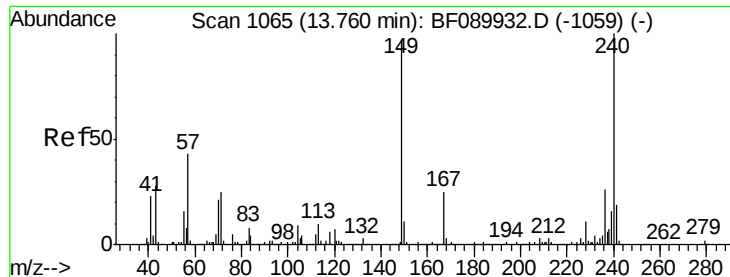

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.75 min Scan# 1064

Delta R.T. -0.01 min

Lab File: BF089977.D

Acq: 2 Sep 2016 16:15

Instrument :

BNA_F

ClientSampleId :


Tot Ion:240 Resp: 479900

Ion Ratio Lower Upper

240 100

120 11.9 5.7 8.5#




236 26.4 21.3 31.9

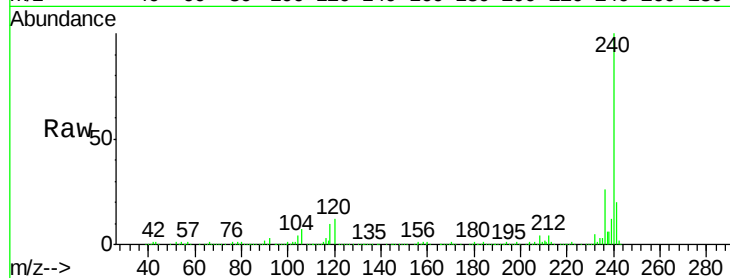

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

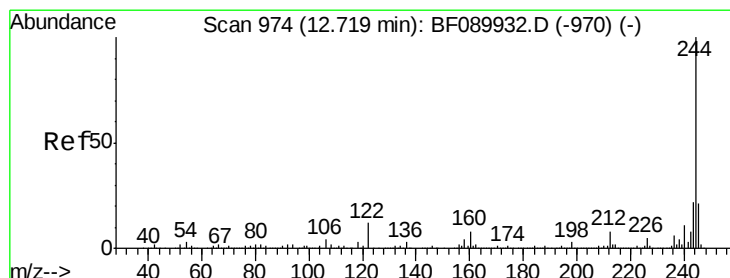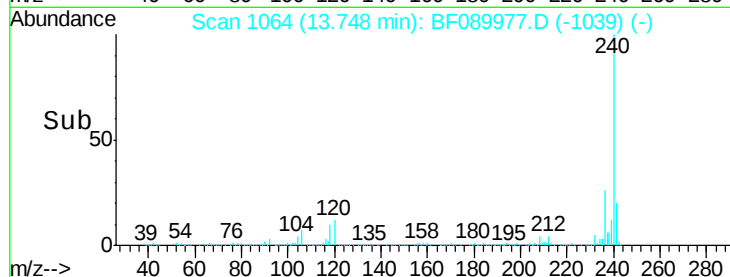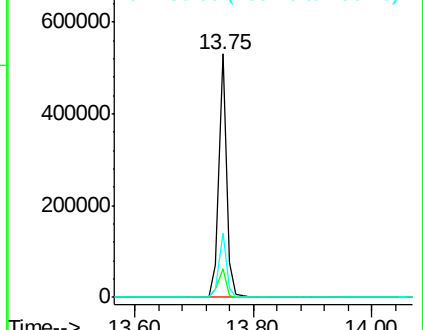

#78

Terphenyl-d14

Concen: 66.29 ng

RT: 12.72 min Scan# 974

Delta R.T. -0.01 min

Lab File: BF089977.D

Acq: 2 Sep 2016 16:15


Tgt Ion:244 Resp: 1287758

Ion Ratio Lower Upper

244 100

212 7.6 6.1 9.1



122 11.2 9.6 14.4



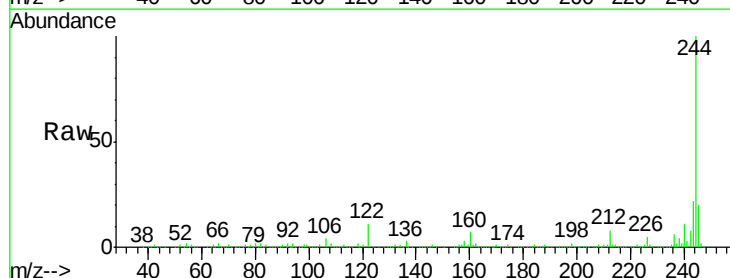


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

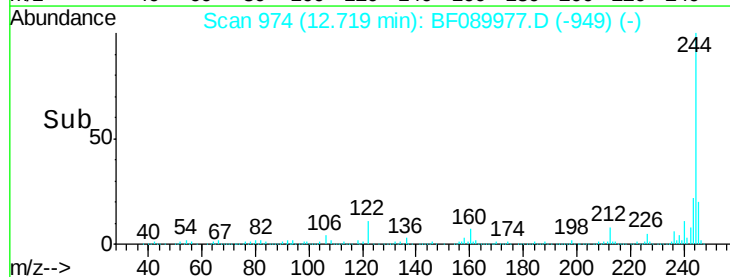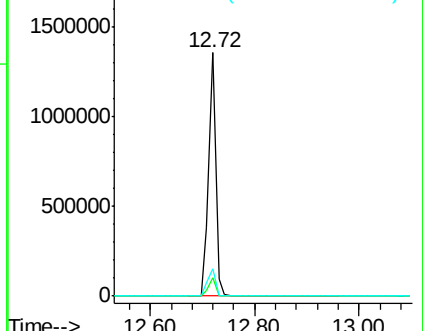

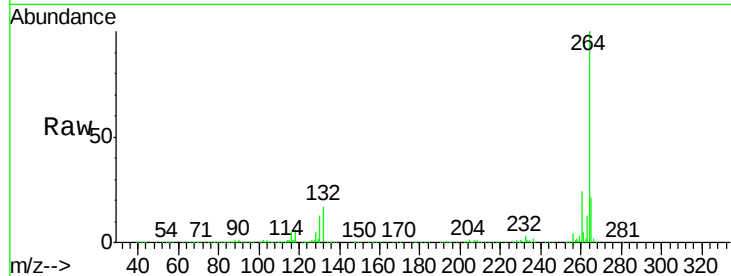

#86
Pervlene-d12
Concen: 20.00 ng
RT: 15.10 min Scan# 1182
Delta R.T. 0.00 min
Lab File: BF089977.D
Acq: 2 Sep 2016 16:15

Instrument :
BNA_F
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.7	19.4	29.0
265	21.1	17.4	26.2

