
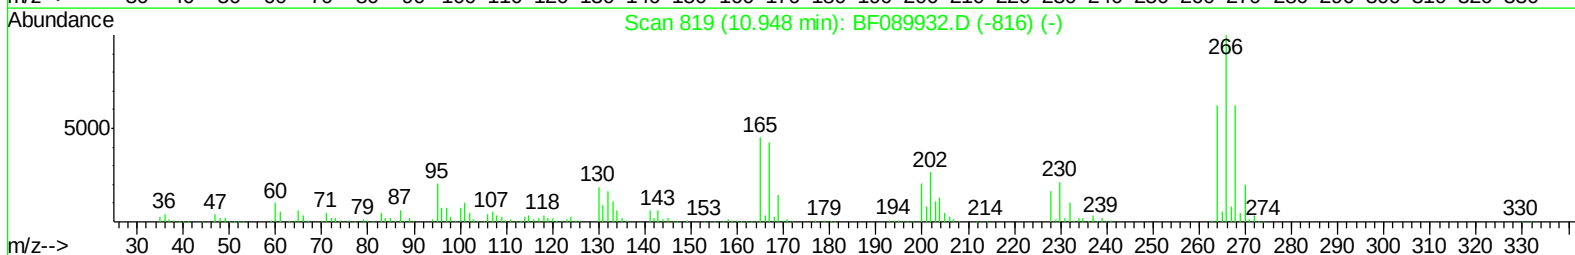
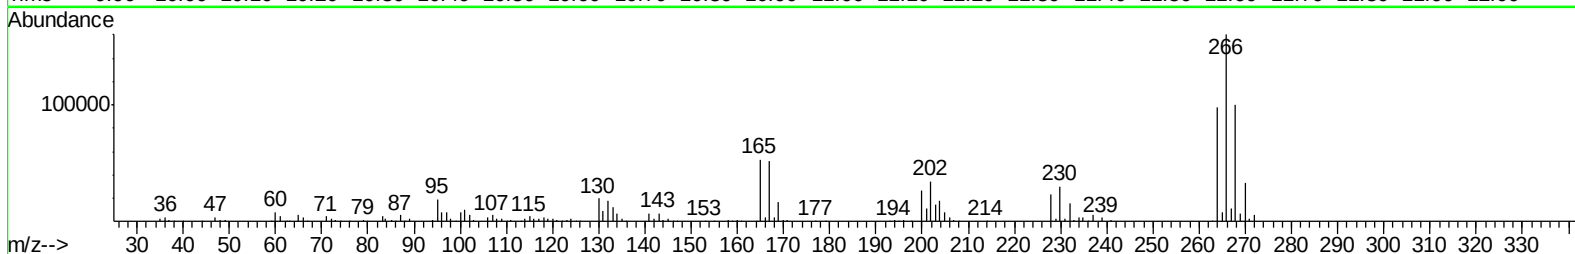


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF090216\
Data File : BF089971.D
Acq On : 2 Sep 2016 12:26
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 02 23:21:05 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF083116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 02 13:29:08 2016
Response via : Initial Calibration

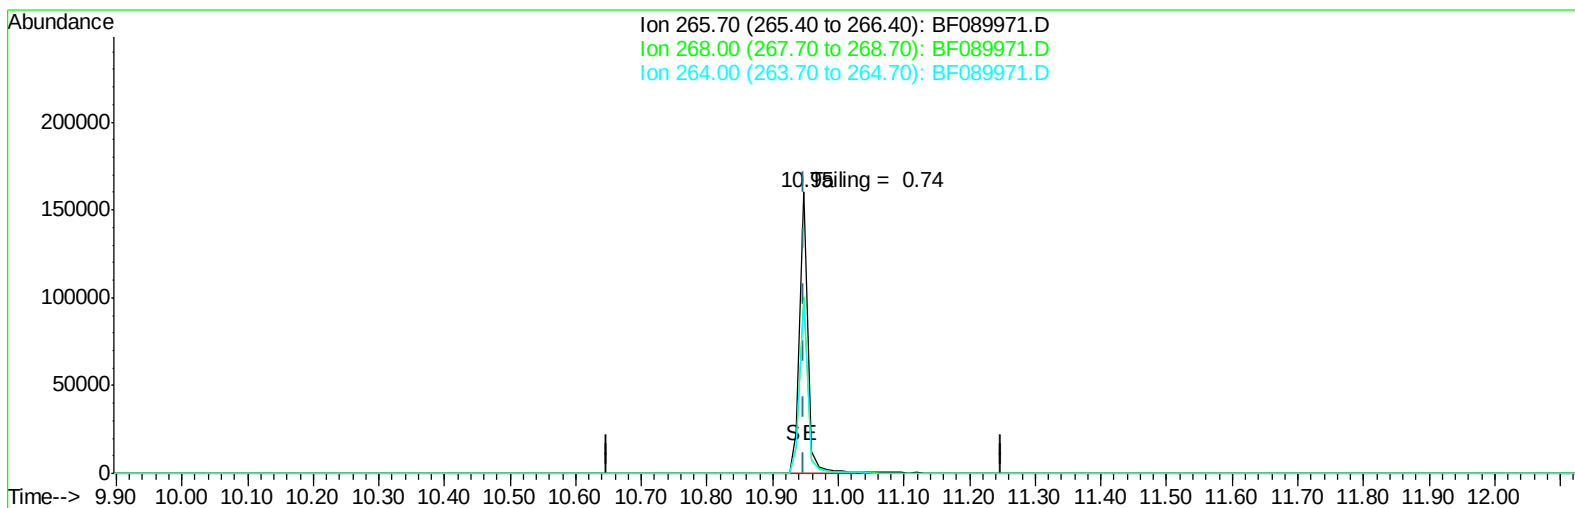

TIC: BF089971.D

(69) Pentachlorophenol (C)




10.948min (+0.000) 42512.34ng

response 144916

Ion	Exp%	Act%
265.70	100	100
268.00	63.80	62.68
264.00	63.20	61.16
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF090216\
Data File : BF089971.D
Acq On : 2 Sep 2016 12:26
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 02 23:21:05 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF083116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 02 13:29:08 2016
Response via : Initial Calibration

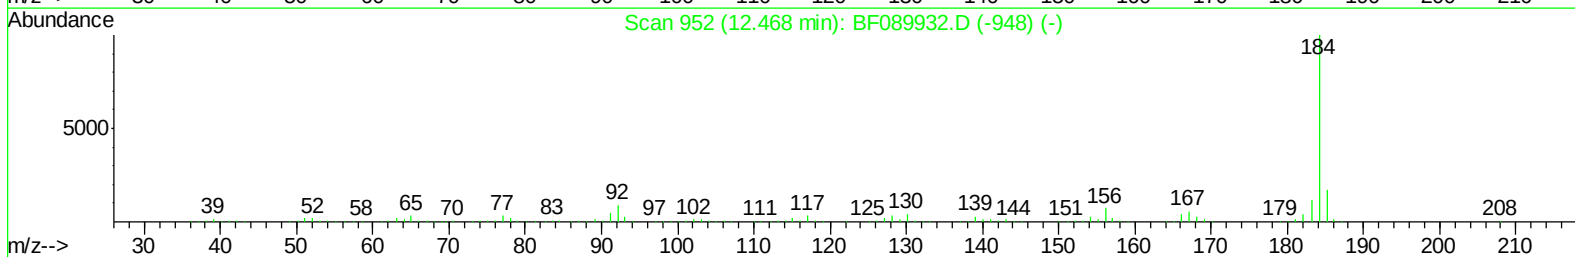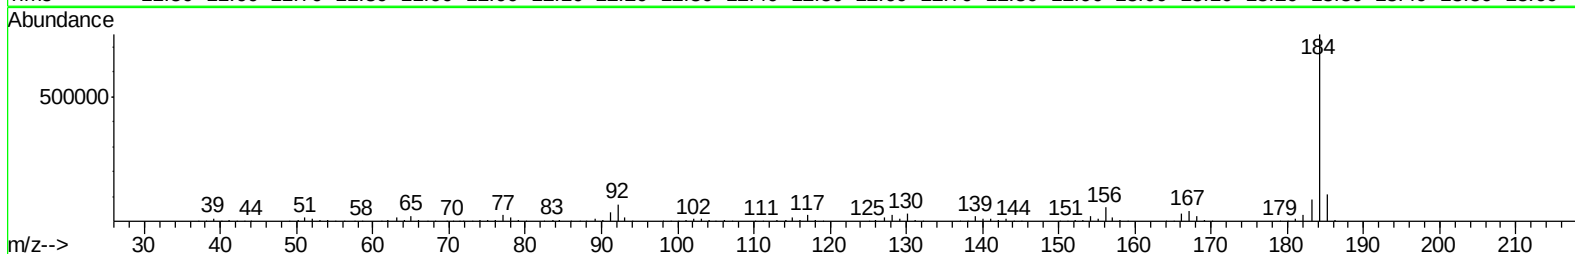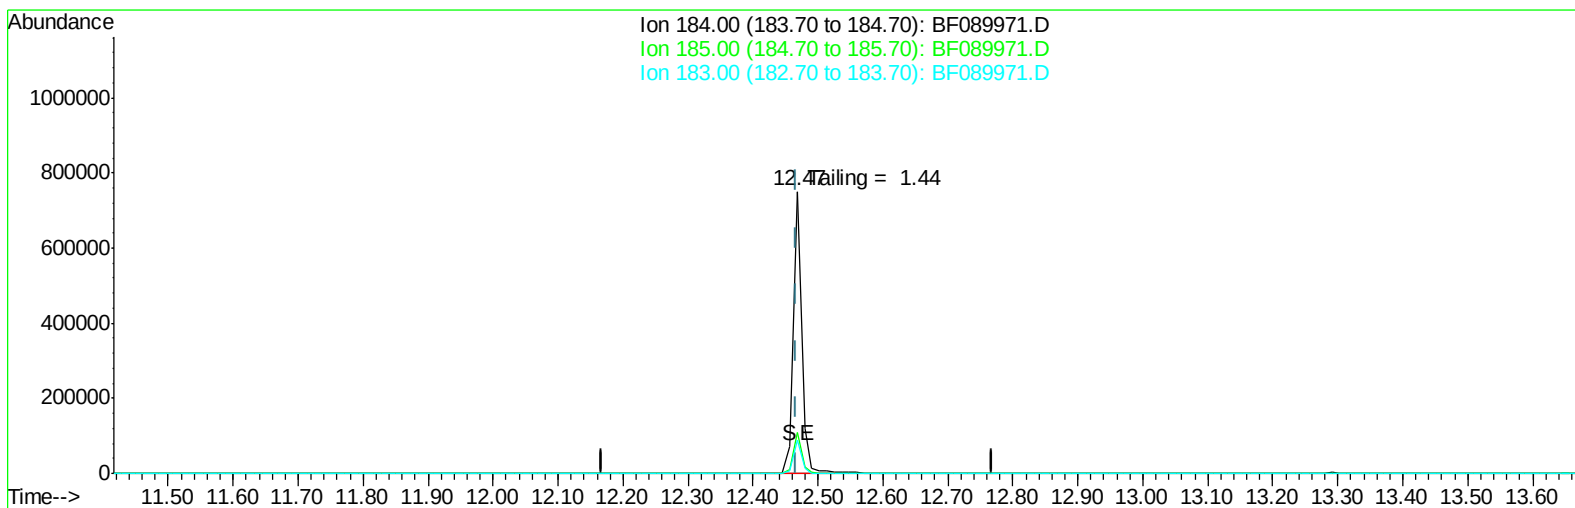

TIC: BF089971.D

(76) Benzidine

12.468min (+0.000) 17427.84ng

response 679367

Ion	Exp%	Act%
184.00	100	100
185.00	17.30	14.59
183.00	12.00	11.71
0.00	0.00	0.00