


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF090216\
 Data File : BF089971.D
 Acq On : 2 Sep 2016 12:26
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF083116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 02 13:29:08 2016

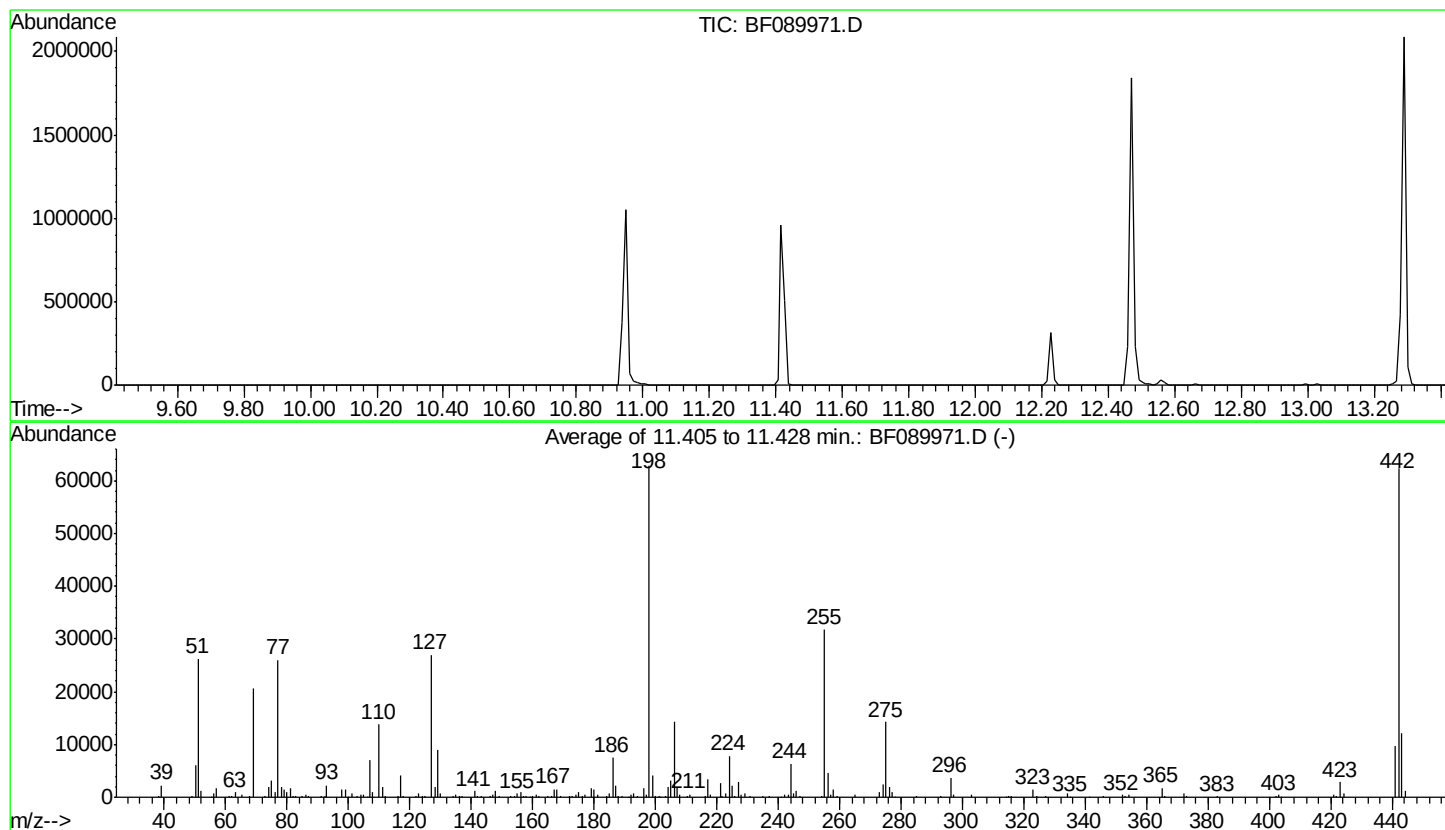

AutoFind: Scans 859, 860, 861; Background Corrected with Scan 856

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.8	26283	PASS
68	69	0.00	2	1.1	218	PASS
69	198	0.00	100	33.0	20720	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.9	26975	PASS
197	198	0.00	2	0.8	525	PASS
198	198	100	100	100.0	62862	PASS
199	198	5	9	6.7	4214	PASS
275	198	10	60	22.7	14266	PASS
365	198	1	100	2.8	1733	PASS
441	442	0.01	24	15.7	9821	PASS
442	198	50	100	99.4	62490	PASS
443	442	15	24	19.4	12115	PASS