
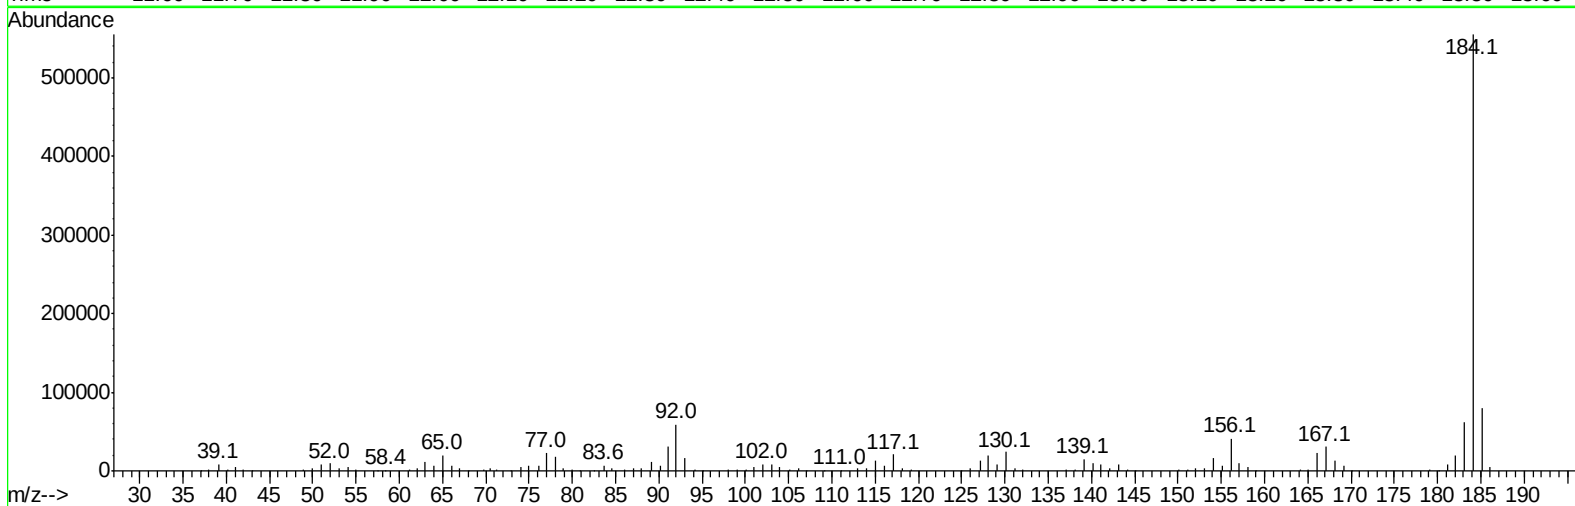


Data Path : Z:\HPCHEM1\BNA F\DATA\BF090217\
Data File : BF098243.D
Acq On : 2 Sep 2017 13:57
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 04 08:47:04 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 21 15:59:04 2017
Response via : Initial Calibration

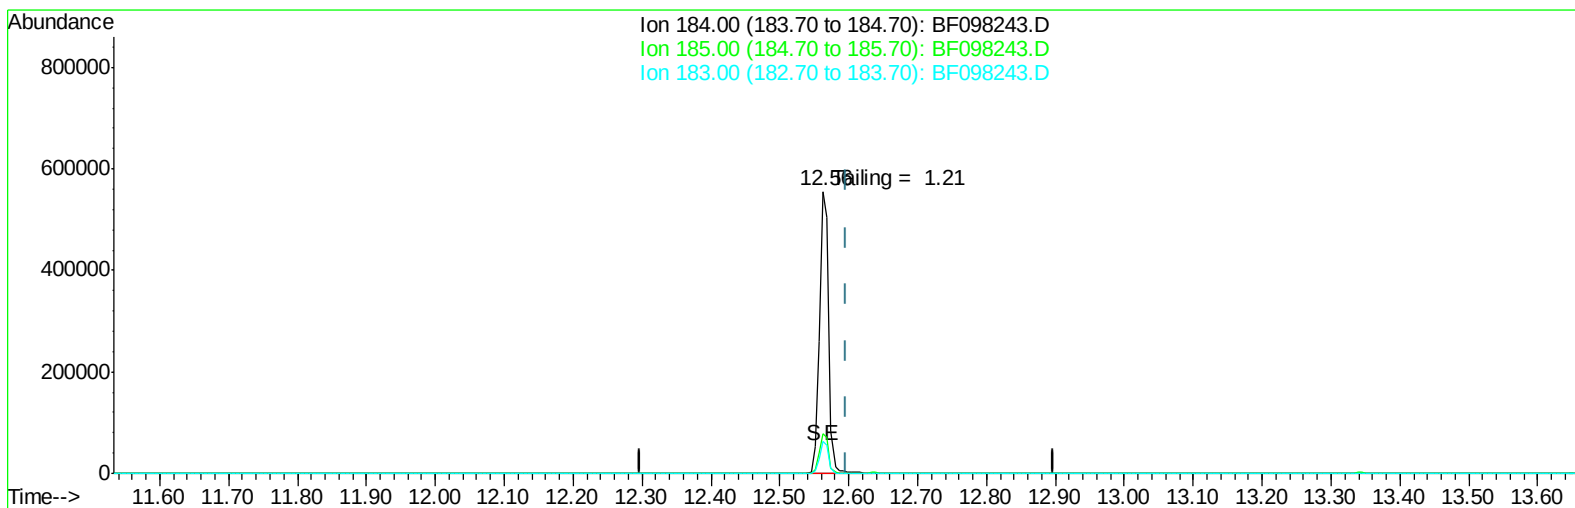

TIC: BF098243.D

(76) Benzidine



12.563min (-0.035) 0.00ng

response 529067

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.32#
183.00	12.20	11.25
0.00	0.00	0.00

```
Data Path : Z:\HPCHEM1\BNA F\DATA\BF090217\  
Data File : BF098243.D  
Acq On    : 2 Sep 2017 13:57  
Operator  : SJ/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1 Sample Multiplier: 1
```

Quant Time: Sep 04 08:47:04 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 21 15:59:04 2017
Response via : Initial Calibration

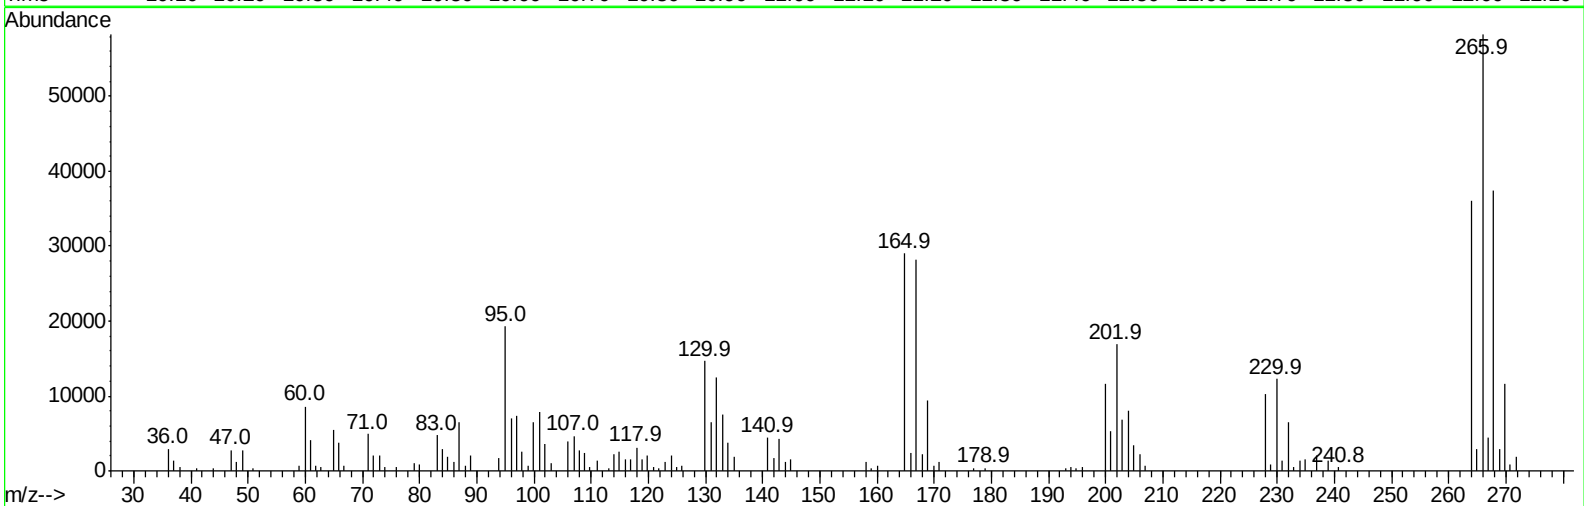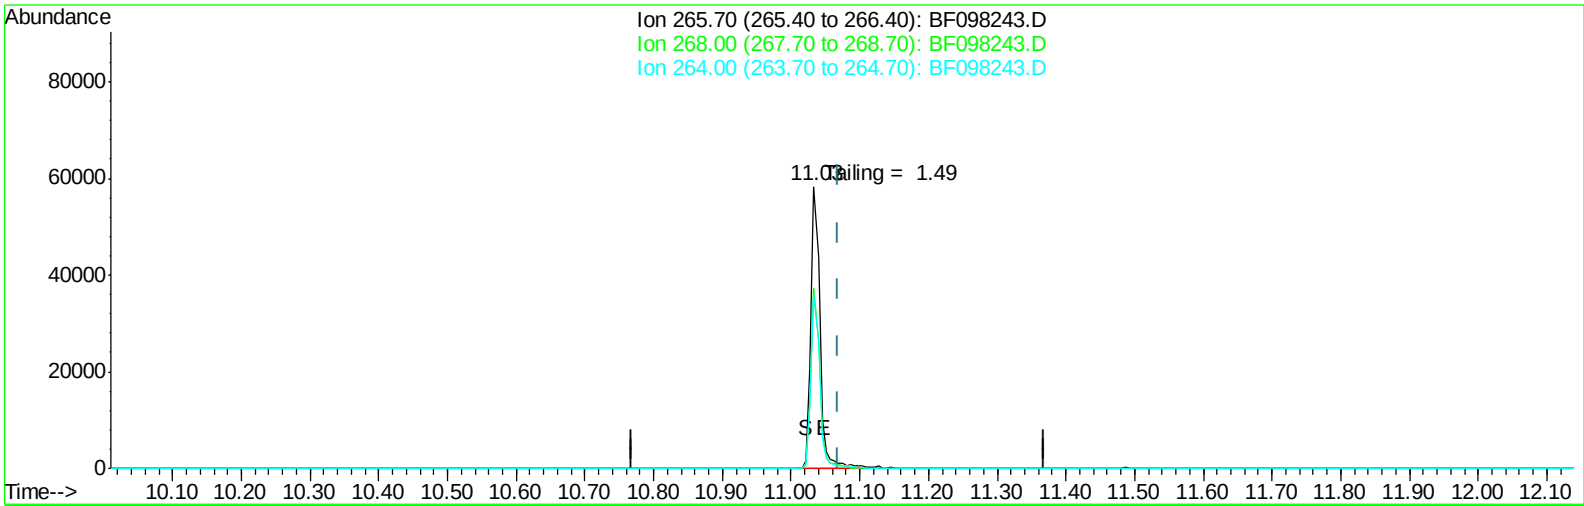

TIC: BF098243.D

(69) Pentachlorophenol (C)

11.033min (-0.035) 25984.60ng

response 52277

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.25
264.00	64.60	61.88
0.00	0.00	0.00