

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF090217\
 Data File : BF098265.D
 Acq On : 3 Sep 2017 00:16
 Operator : SJ/JU
 Sample : I5073-08 5X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP-3-4-COMP

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.881	473	475	484	rBV	34376	35803	4.82%	0.483%
2	5.310	544	548	562	rBV	559469	516285	69.48%	6.966%
3	6.345	721	724	736	rBV	601762	537550	72.34%	7.253%
4	6.475	743	746	750	rBV	584038	526573	70.86%	7.105%
5	6.710	782	786	790	rBV	760134	607405	81.74%	8.195%
6	6.863	809	812	821	rBV	417389	351472	47.30%	4.742%
7	7.275	878	882	889	rBV	316641	289768	38.99%	3.910%
8	7.992	1000	1004	1020	rBV	870906	743106	100.00%	10.026%
9	9.069	1183	1187	1204	rBV	619220	505896	68.08%	6.826%
10	9.469	1252	1255	1260	rBV	40043	37298	5.02%	0.503%
11	9.745	1298	1302	1312	rBB2	780851	667310	89.80%	9.004%
12	10.533	1433	1436	1445	rBB	236214	208850	28.11%	2.818%
13	11.227	1550	1554	1558	rBV	714333	610689	82.18%	8.240%
14	12.439	1757	1760	1764	rBV	30471	24395	3.28%	0.329%
15	12.668	1794	1799	1802	rBV	26403	27379	3.68%	0.369%
16	12.810	1819	1823	1827	rBV	502885	408677	55.00%	5.514%
17	12.998	1848	1855	1857	rVB4	5565	8670	1.17%	0.117%
18	13.504	1937	1941	1945	rBV4	10128	12591	1.69%	0.170%
19	13.715	1974	1977	1982	rBV6	25114	33772	4.54%	0.456%
20	13.862	1995	2002	2005	rBV	776767	702825	94.58%	9.483%
21	14.874	2171	2174	2177	rBV2	23642	31357	4.22%	0.423%
22	15.274	2238	2242	2251	rBV	411368	523910	70.50%	7.069%


Sum of corrected areas: 7411581

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF090217\
Data File : BF098265.D
Acq On : 3 Sep 2017 00:16
Operator : SJ/JU
Sample : I5073-08 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampled :
TP-3-4-COMP

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

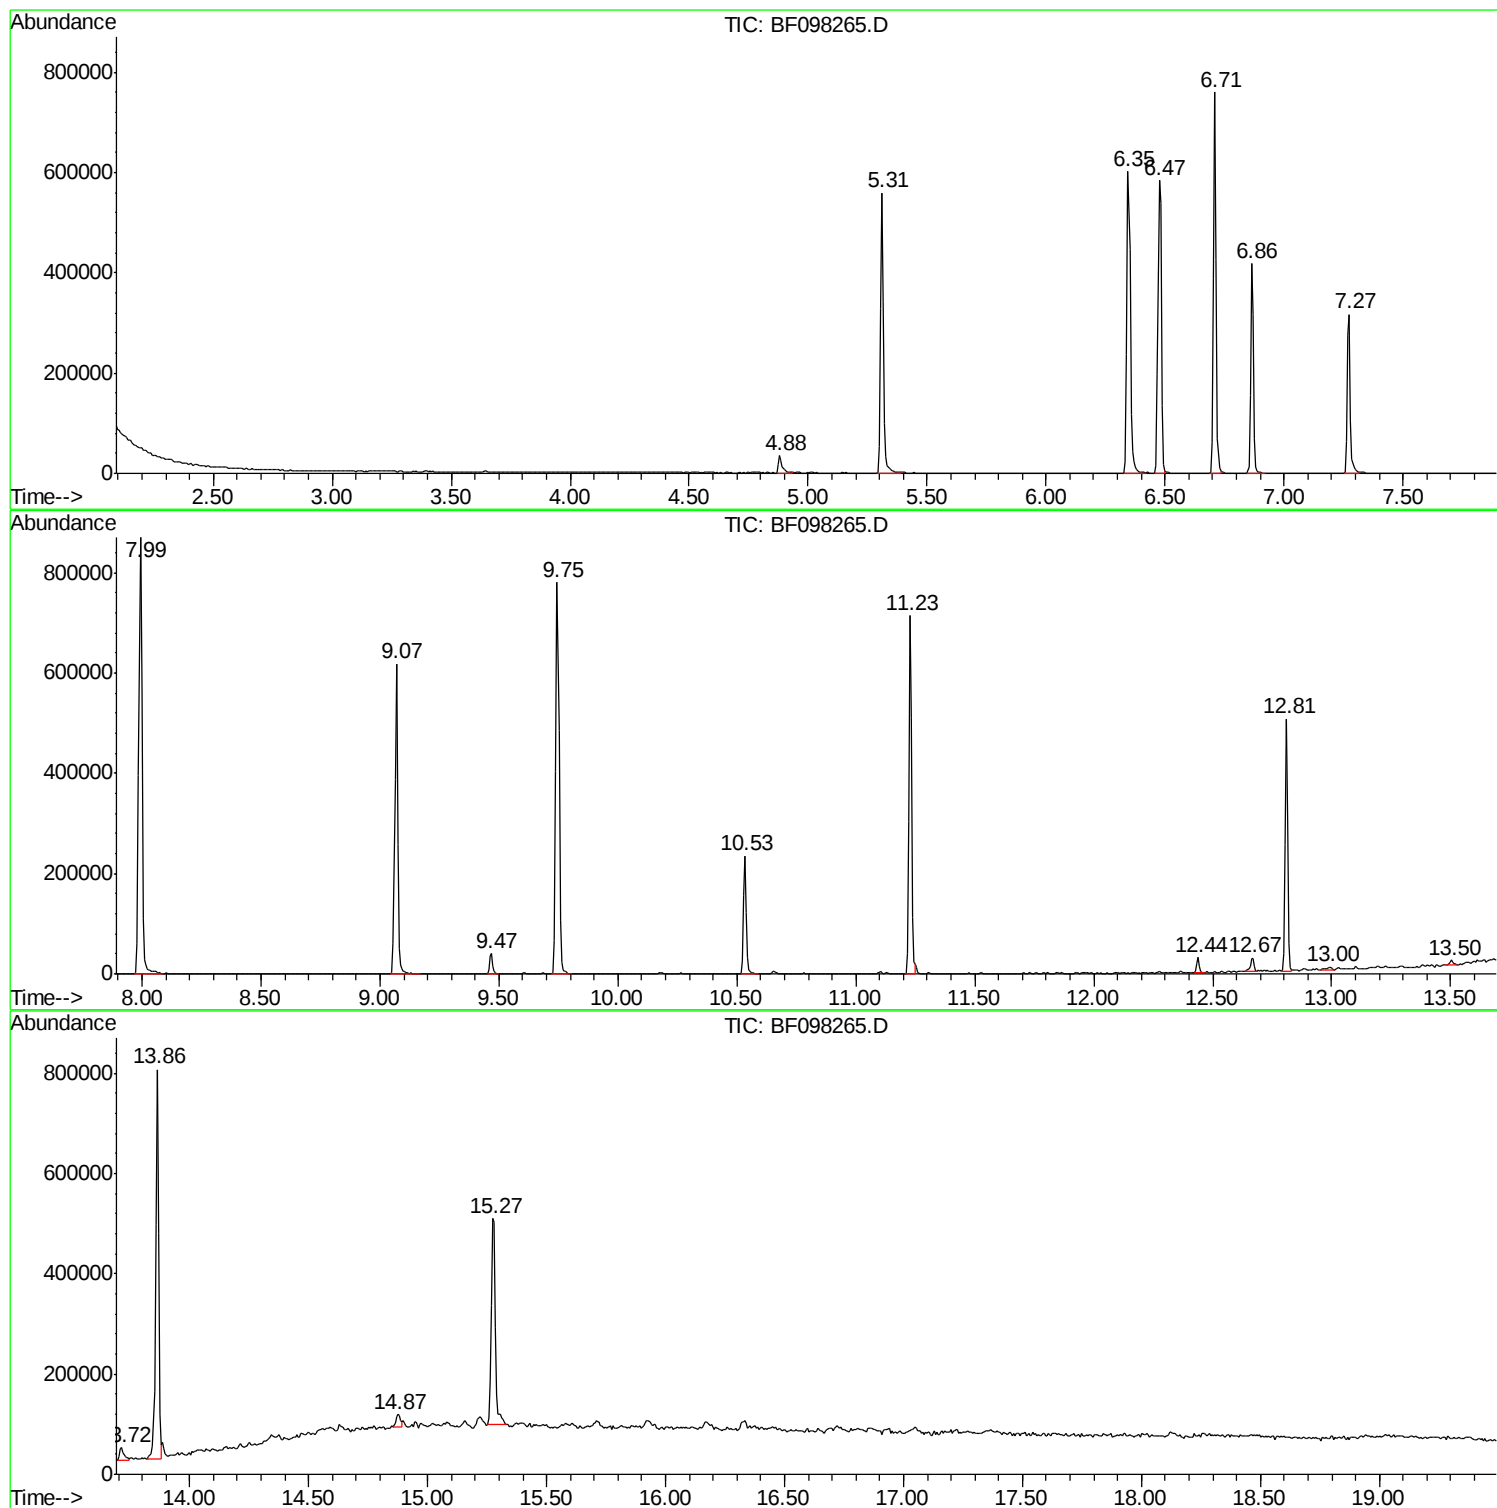

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF090217\
Data File : BF098265.D
Acq On : 3 Sep 2017 00:16
Operator : SJ/JU
Sample : I5073-08 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-3-4-COMP









Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.47 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.47	17.34 ng	526573	1,4-Dichlorobenzene-d4	6.71

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12
3		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10
4		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9
5		1-Methylpyrrolo[1,2-a]pyrazine	132	C8H8N2	064608-59-9	9

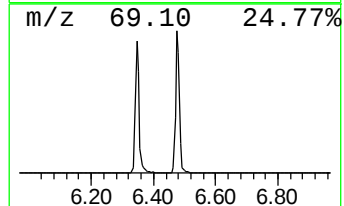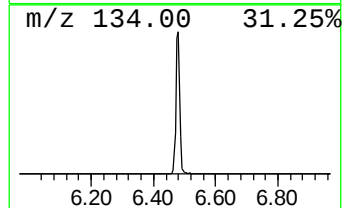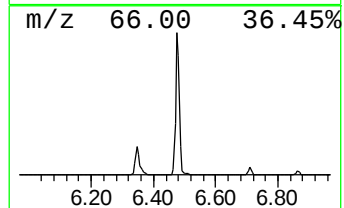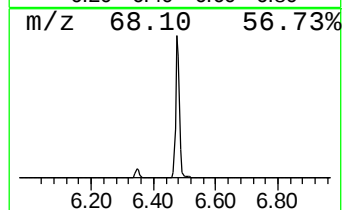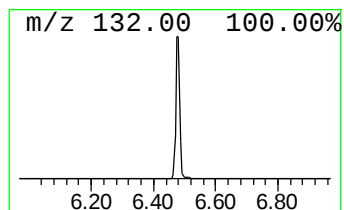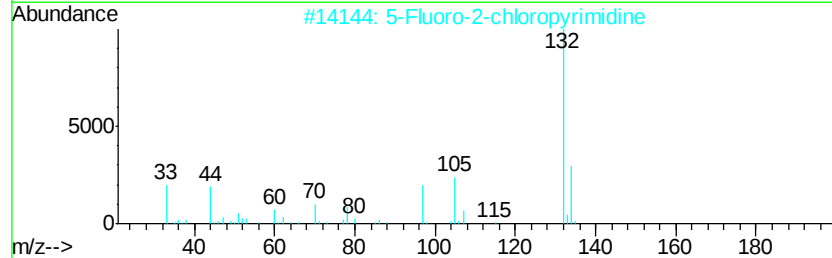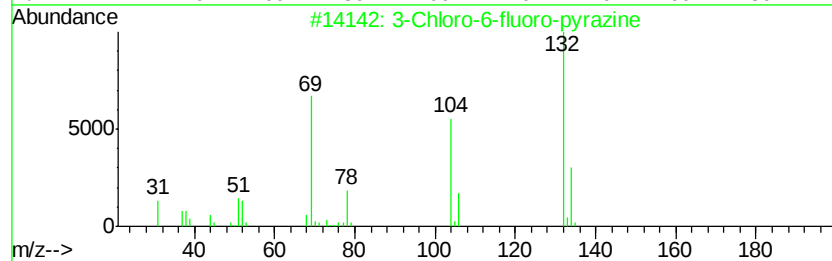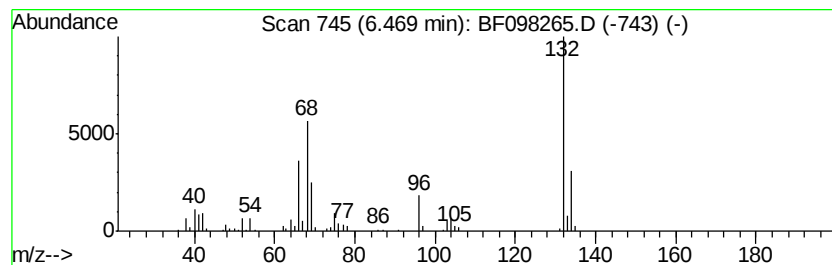

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF090217\
Data File : BF098265.D
Acq On : 3 Sep 2017 00:16
Operator : SJ/JU
Sample : I5073-08 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-3-4-COMP

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.47	6.47	17.3	ng	526573	1	6.71	607405	20.0