
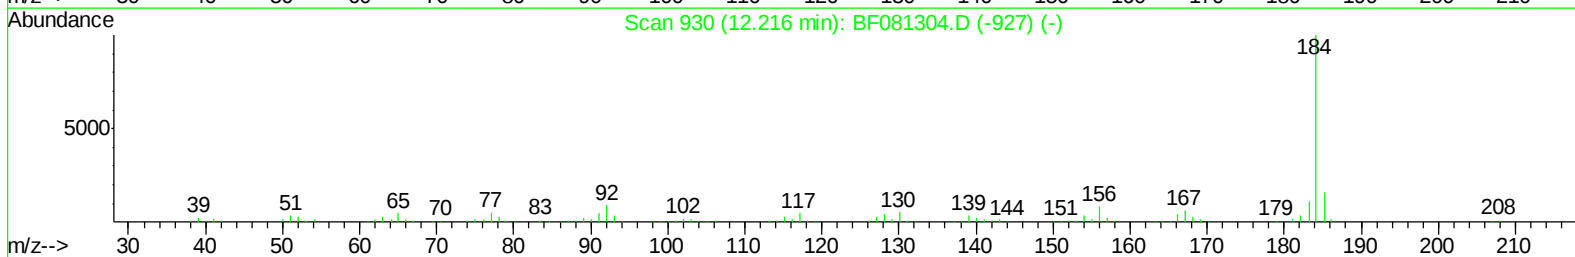
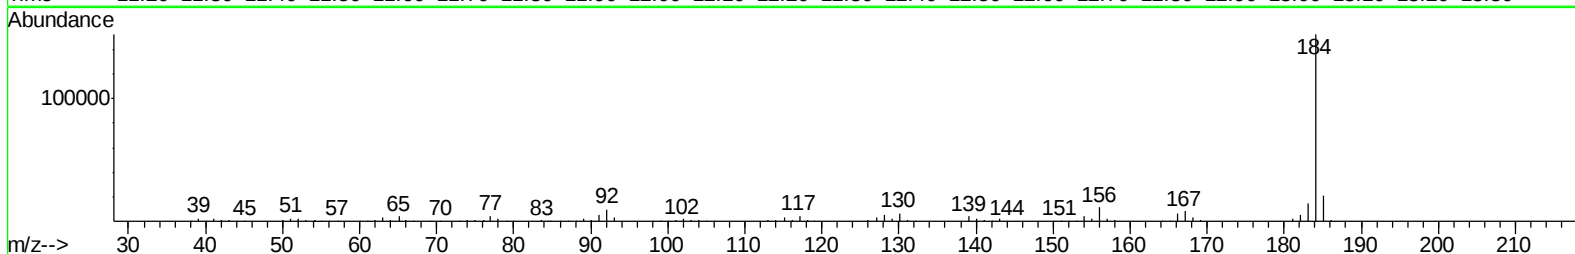


Data Path : Z:\HPCHEM1\BNA F\DATA\BF090315\
Data File : BF081377.D
Acq On : 3 Sep 2015 14:56
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 04 06:49:20 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF090115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 04 02:03:29 2015
Response via : Initial Calibration

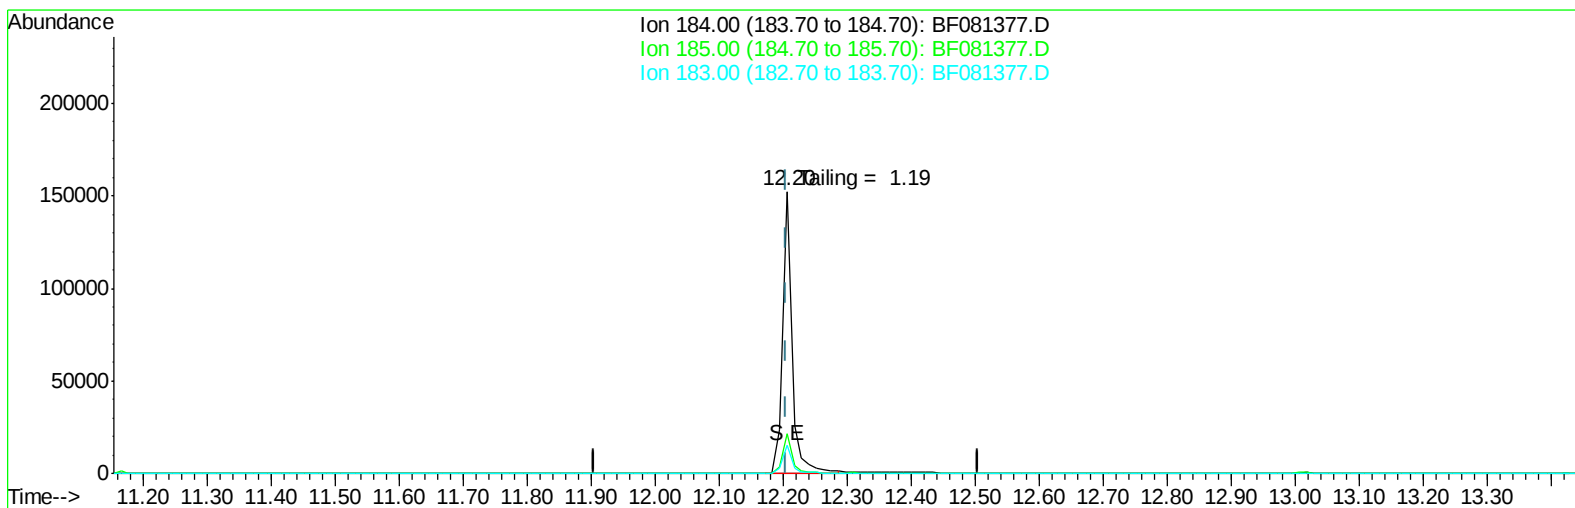

TIC: BF081377.D

(76) Benzidine




12.205min (-0.000) 0.00ng

response 156764

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	13.91
183.00	9.50	9.97
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF090315\
 Data File : BF081377.D
 Acq On : 3 Sep 2015 14:56
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 04 06:49:20 2015
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF090115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 04 02:03:29 2015
 Response via : Initial Calibration

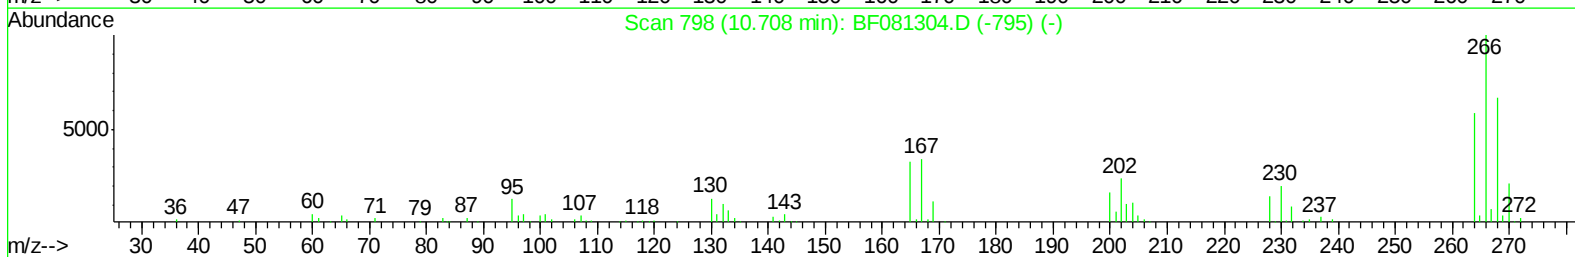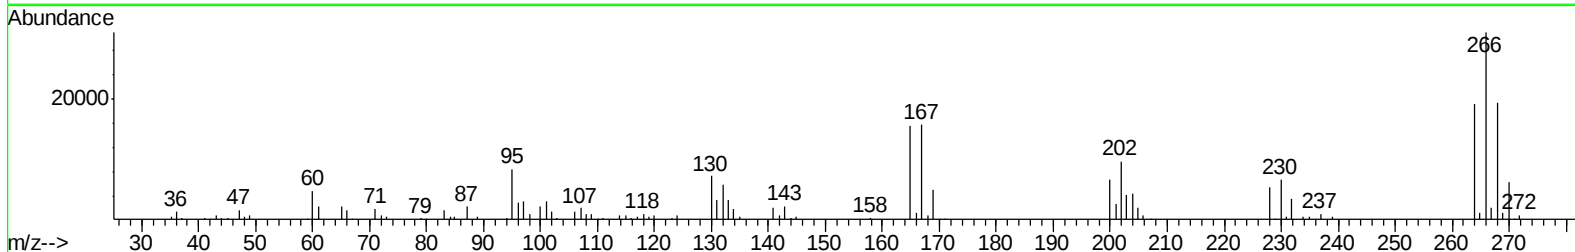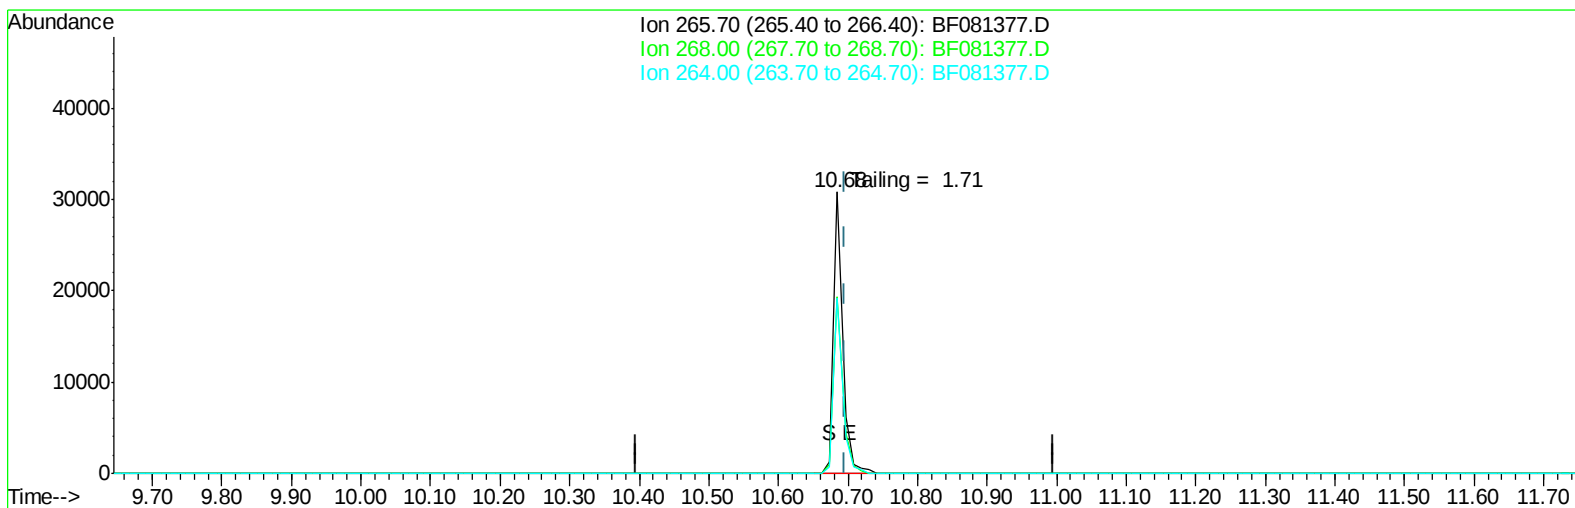

TIC: BF081377.D

(69) Pentachlorophenol (C)

10.685min (-0.011) 0.00ng

response 27634

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	62.56
264.00	62.70	62.32
0.00	0.00	0.00