


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF090315\
 Data File : BF081377.D
 Acq On : 3 Sep 2015 14:56
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF090115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 01 17:35:35 2015

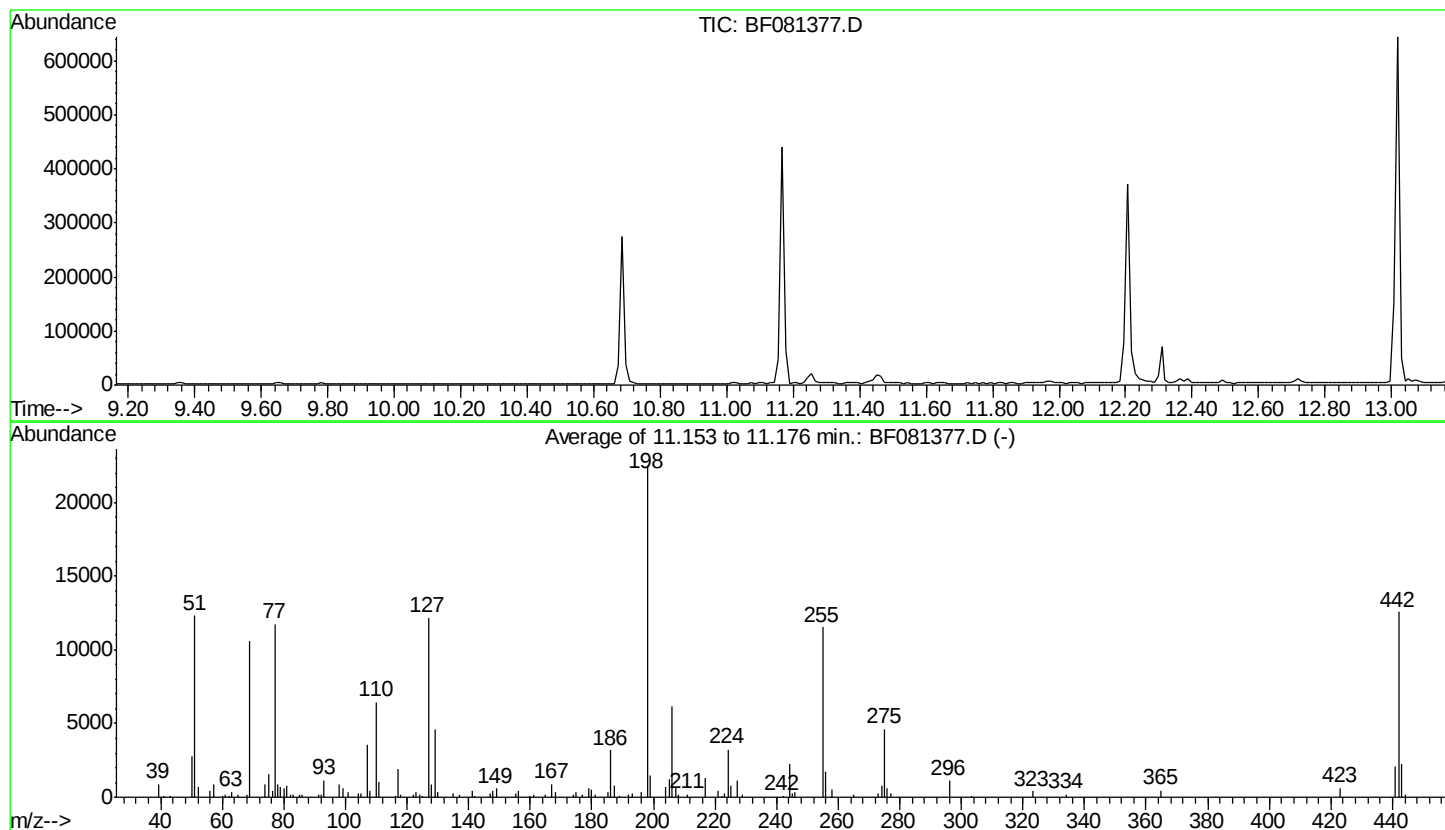

AutoFind: Scans 837, 838, 839; Background Corrected with Scan 834

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.8	12327	PASS
68	69	0.00	2	1.5	159	PASS
69	198	0.00	100	47.2	10620	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.1	12168	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	22512	PASS
199	198	5	9	6.7	1518	PASS
275	198	10	60	20.5	4617	PASS
365	198	1	100	2.1	477	PASS
441	442	0.01	24	16.4	2064	PASS
442	198	50	100	56.0	12598	PASS
443	442	15	24	18.3	2305	PASS