


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF090315\
Data File : BF081396.D
Acq On : 4 Sep 2015 1:30
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF090115.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Sep 01 17:35:35 2015

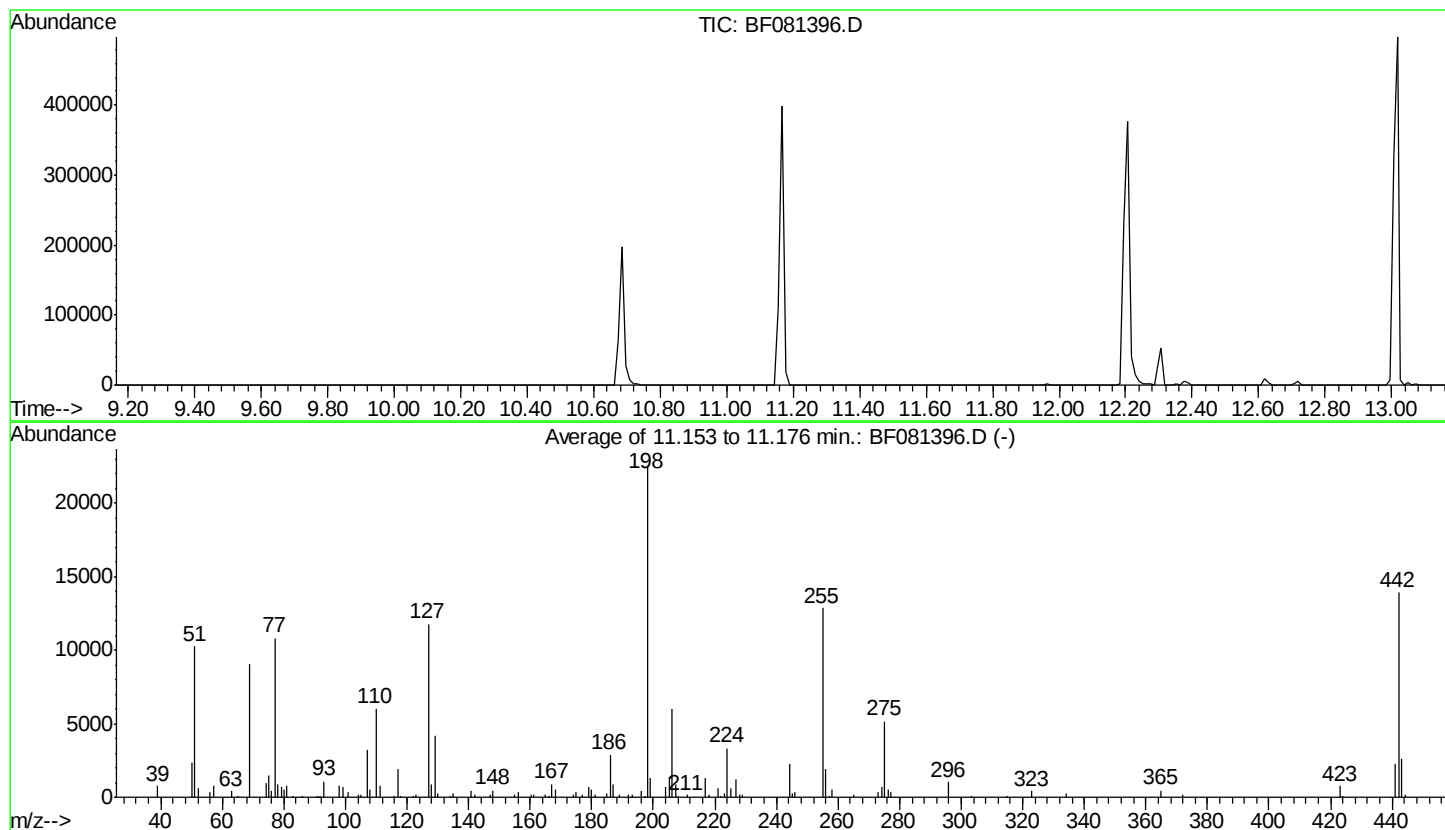

AutoFind: Scans 837, 838, 839; Background Corrected with Scan 834

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.4	10240	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	40.1	9053	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.2	11769	PASS
197	198	0.00	2	0.5	112	PASS
198	198	100	100	100.0	22566	PASS
199	198	5	9	5.9	1340	PASS
275	198	10	60	22.8	5149	PASS
365	198	1	100	2.1	469	PASS
441	442	0.01	24	16.0	2229	PASS
442	198	50	100	61.6	13905	PASS
443	442	15	24	18.6	2580	PASS