
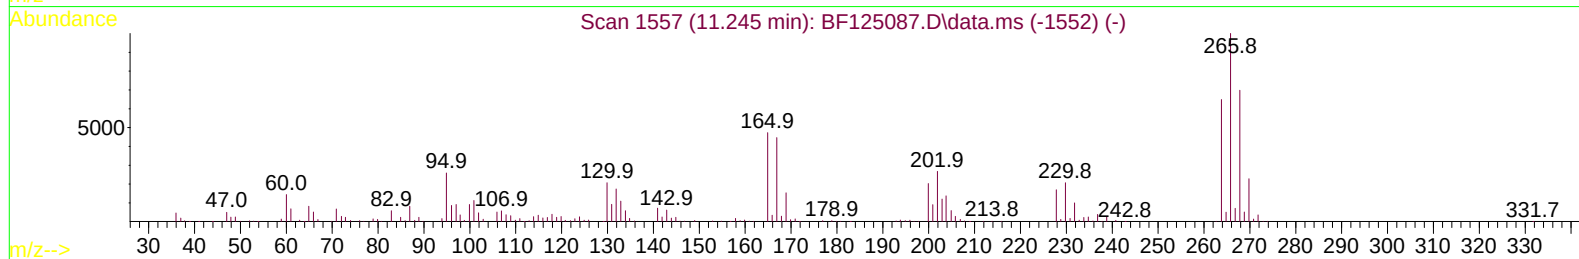
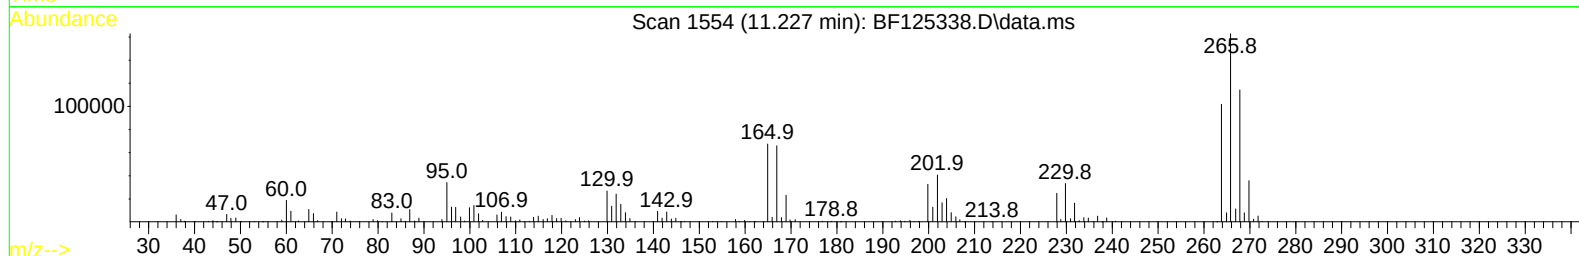


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090321\
Data File : BF125338.D
Acq On : 3 Sep 2021 10:04
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 03 11:49:34 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 24 12:39:21 2021
Response via : Initial Calibration

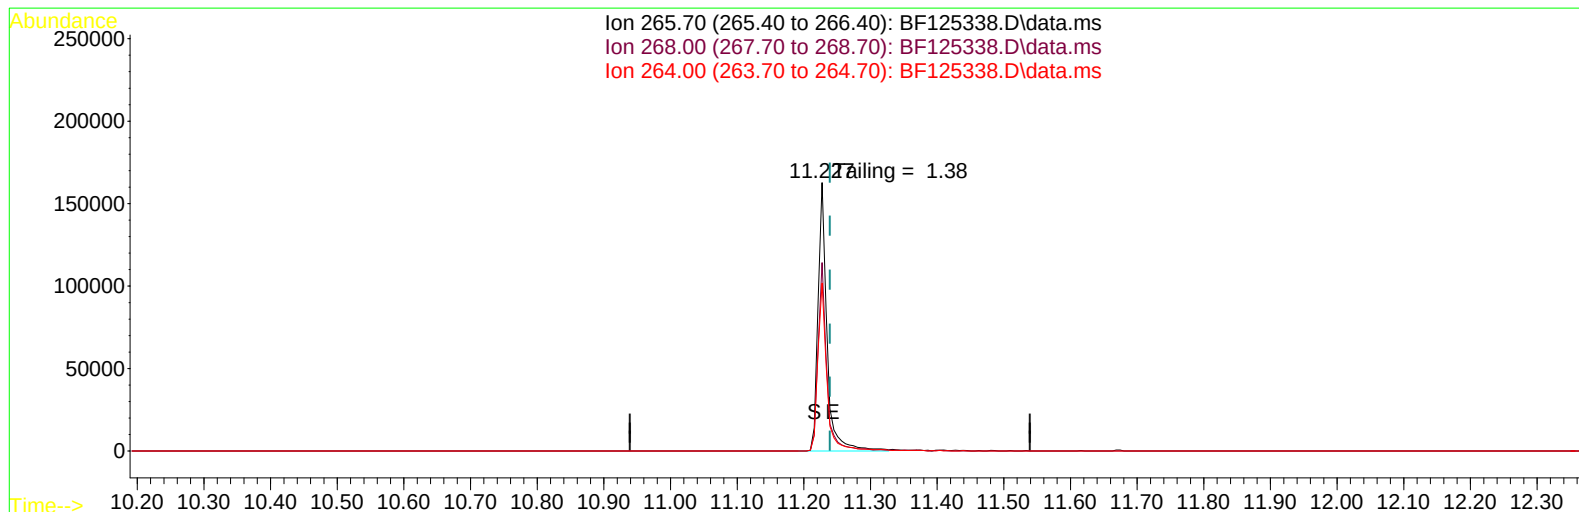

TIC: BF125338.D\data.ms

(70) Pentachlorophenol (C)




11.227min (-0.012) 29365.33 ng

response 154412

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	70.18
264.00	69.90	62.57
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090321\
Data File : BF125338.D
Acq On : 3 Sep 2021 10:04
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 03 11:49:34 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 24 12:39:21 2021
Response via : Initial Calibration

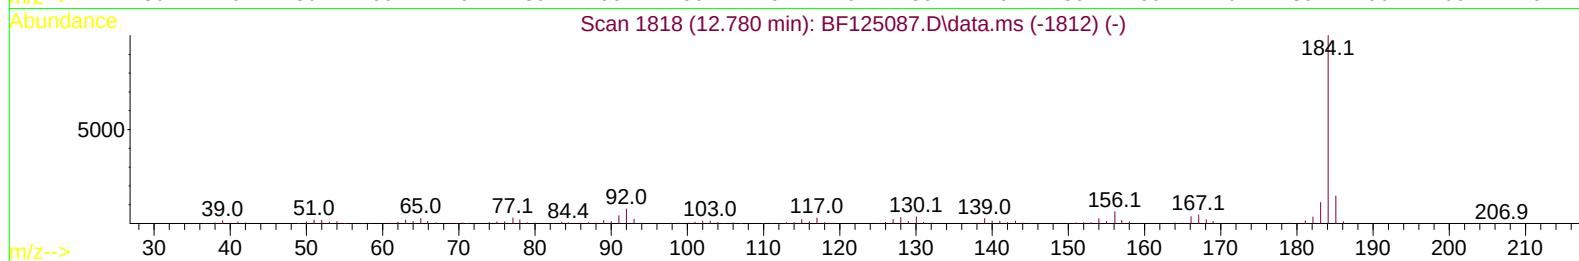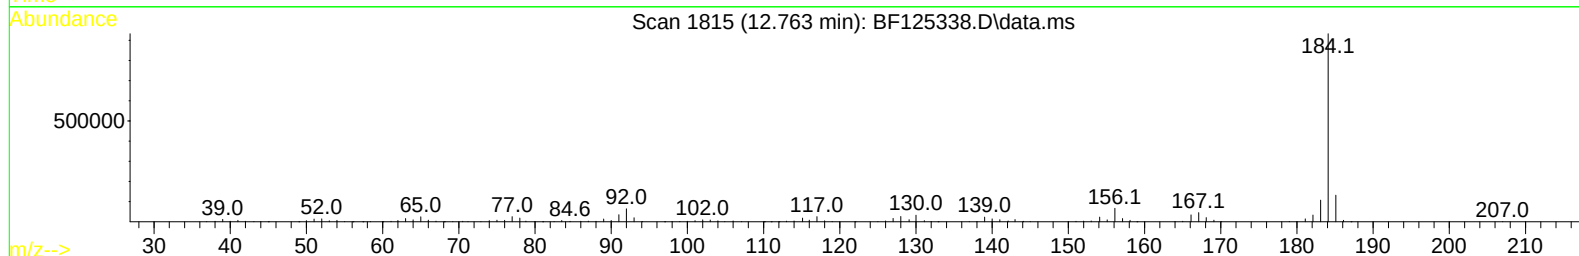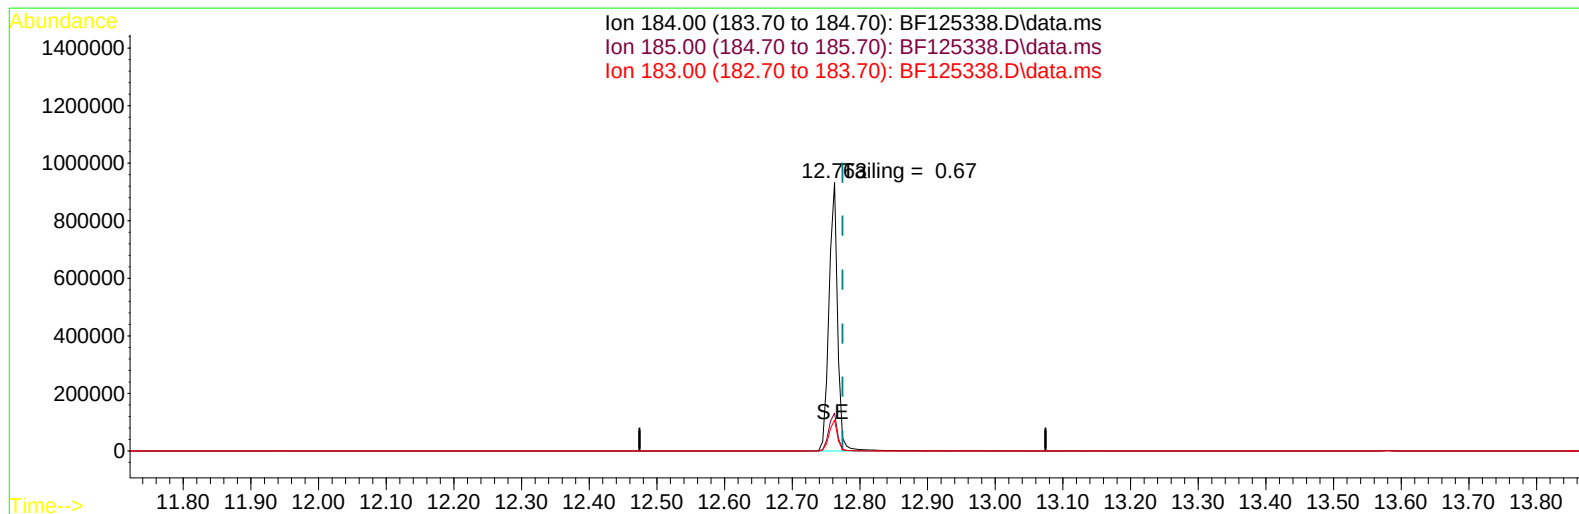

TIC: BF125338.D\data.ms

(77) Benzidine

12.763min (-0.012) 0.00 ng

response 823188

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.14
183.00	10.10	11.56
0.00	0.00	0.00