


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090321\
 Data File : BF125338.D
 Acq On : 3 Sep 2021 10:04
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 03 11:56:34 2021

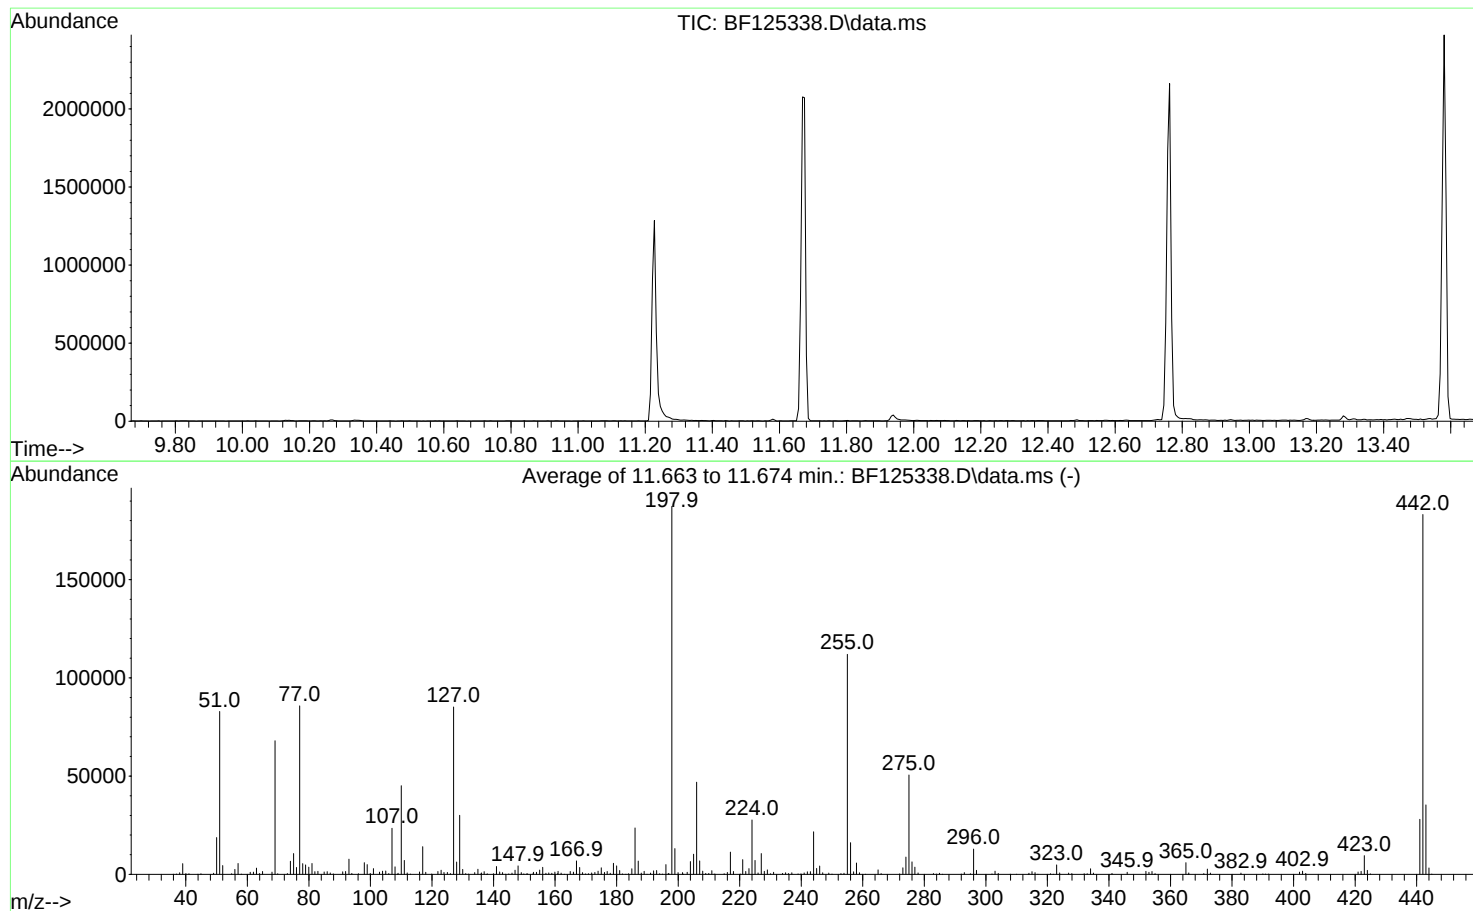

AutoFind: Scans 1628, 1629, 1630; Background Corrected with Scan 1624

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.3	82877	PASS
68	69	0.00	2	1.7	1140	PASS
69	198	0.00	100	36.3	67971	PASS
70	69	0.00	2	0.5	312	PASS
127	198	10	80	45.5	85205	PASS
197	198	0.00	2	0.2	463	PASS
198	198	100	100	100.0	187208	PASS
199	198	5	9	7.0	13077	PASS
275	198	10	60	27.0	50552	PASS
365	198	1	100	3.2	5949	PASS
441	198	0.01	100	14.9	27985	PASS
442	442	50	100	100.0	183117	PASS
443	442	15	24	19.3	35370	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
9/3/2021	BNA_F	<u>BF125338.D</u>
Compound Name	Response	Retention Time
DDT	411890	13.58
DDD	6257	13.28
DDE	920	12.93
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7177	419067	1.71

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090321\
Data File : BF125338.D
Acq On : 3 Sep 2021 10:04
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 03 11:49:34 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 24 12:39:21 2021
Response via : Initial Calibration

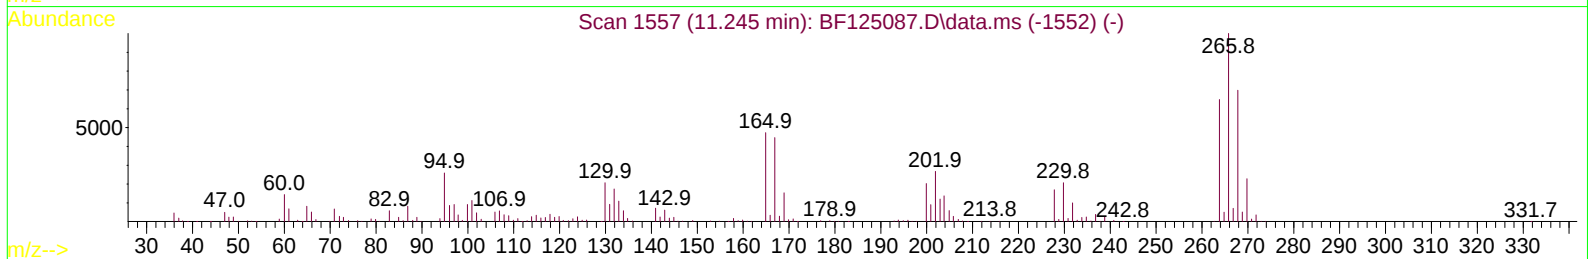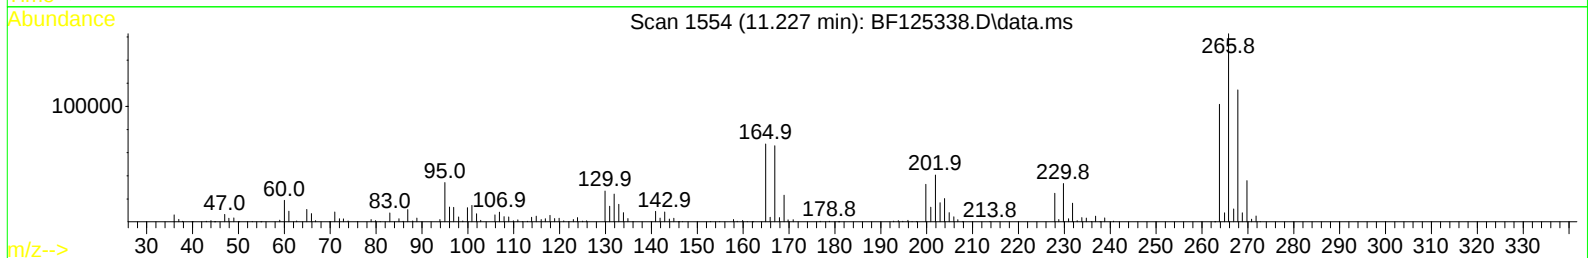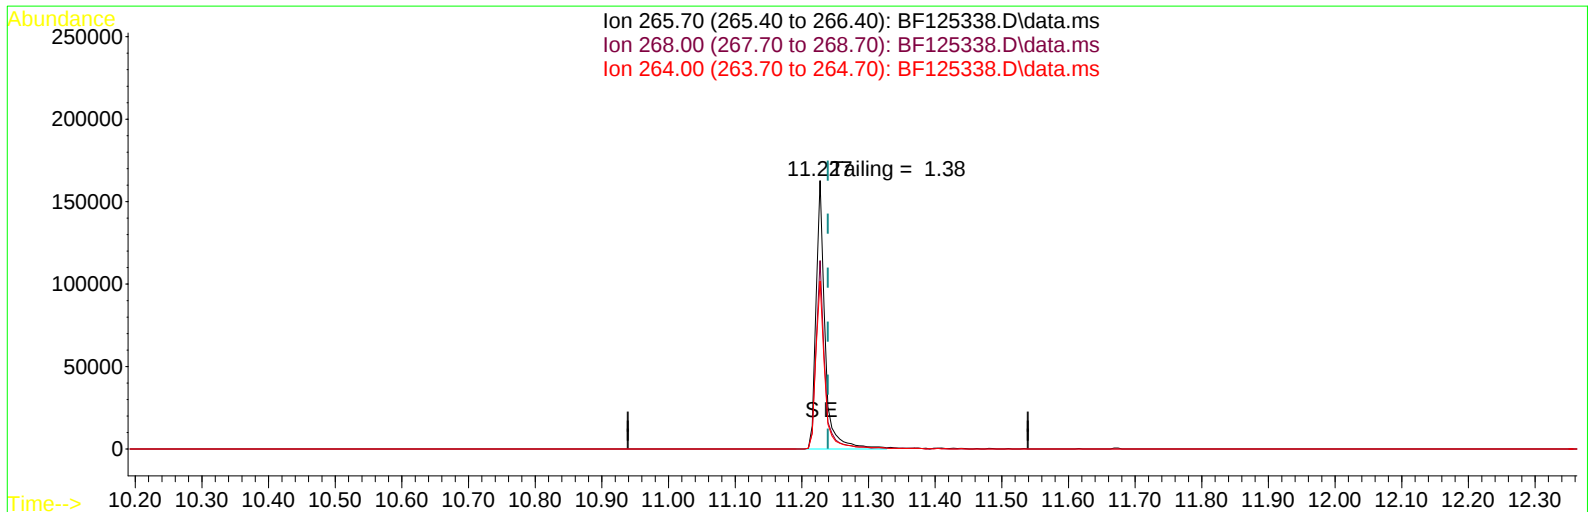

TIC: BF125338.D\data.ms

(70) Pentachlorophenol (C)

11.227min (-0.012) 29365.33 ng




response 154412

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	70.18
264.00	69.90	62.57
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090321\
Data File : BF125338.D
Acq On : 3 Sep 2021 10:04
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 03 11:49:34 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 24 12:39:21 2021
Response via : Initial Calibration

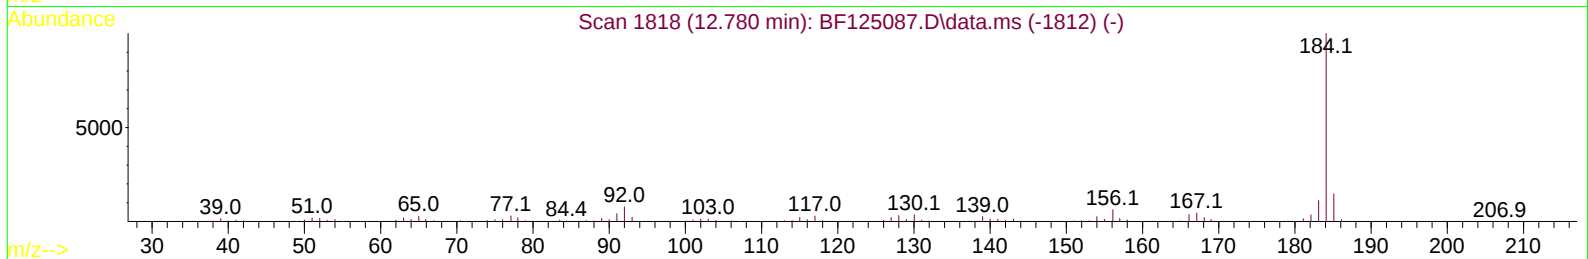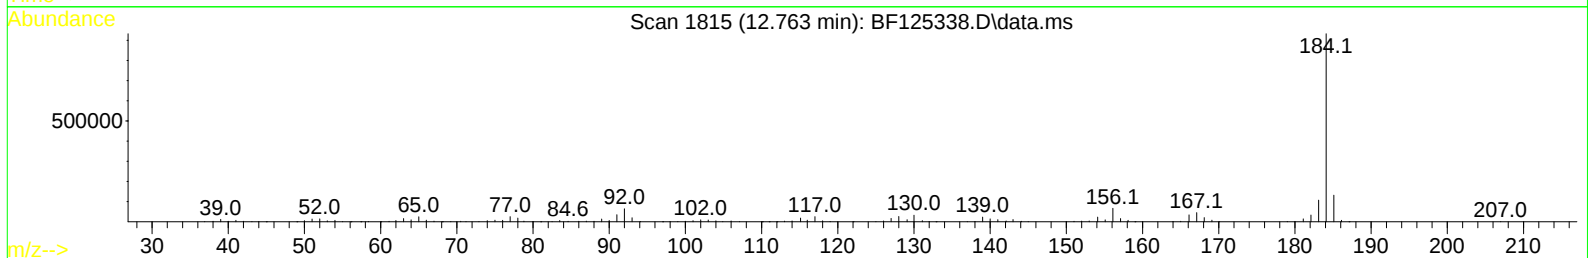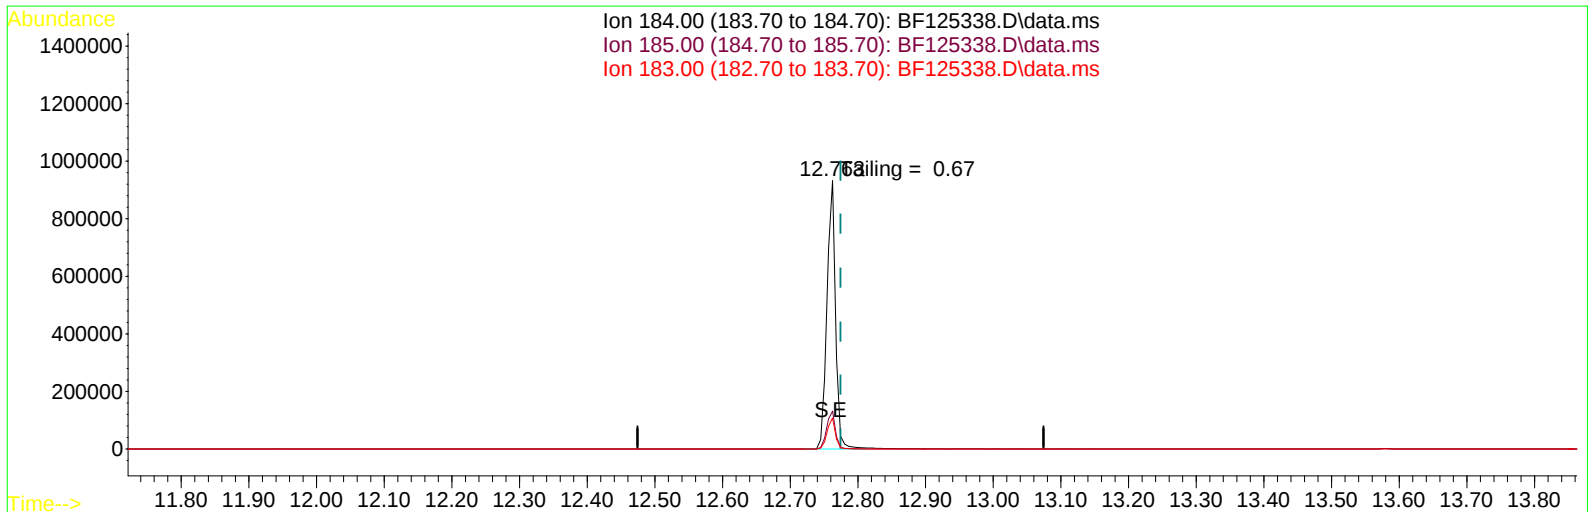

TIC: BF125338.D\data.ms

(77) Benzidine

12.763min (-0.012) 0.00 ng

response 823188

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.14
183.00	10.10	11.56
0.00	0.00	0.00