
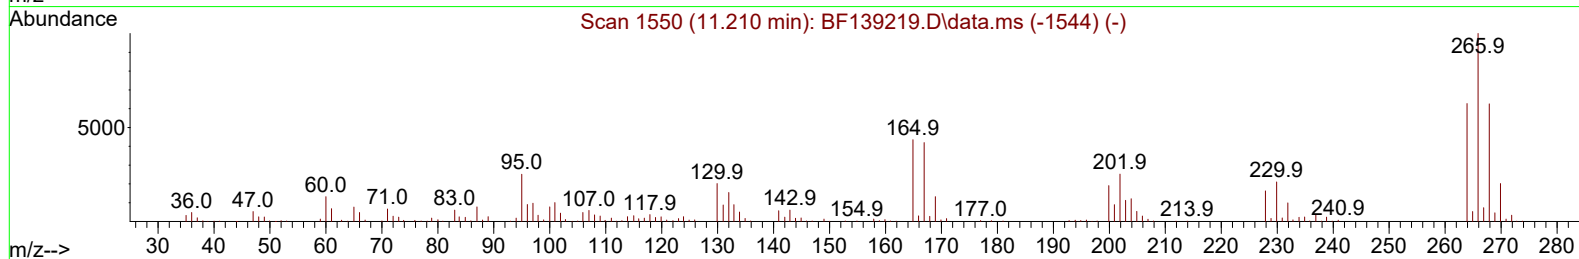
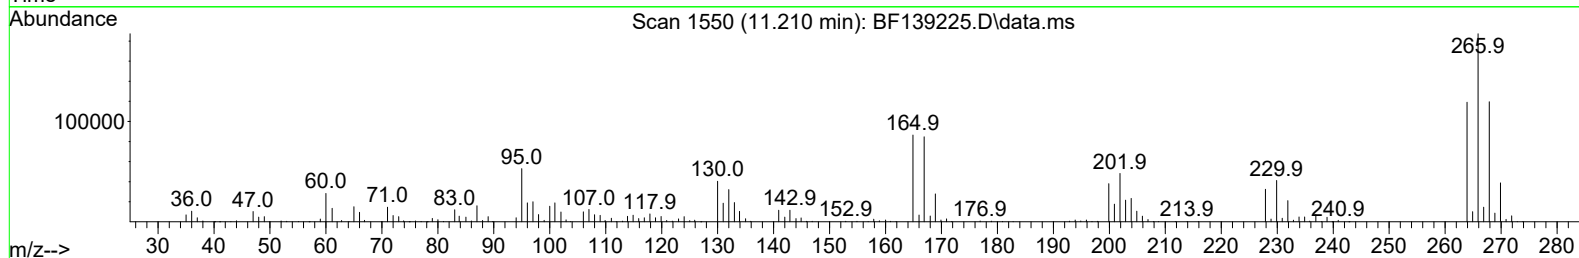


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090324\
Data File : BF139225.D
Acq On : 03 Sep 2024 09:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 03 11:15:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 29 15:46:29 2024
Response via : Initial Calibration

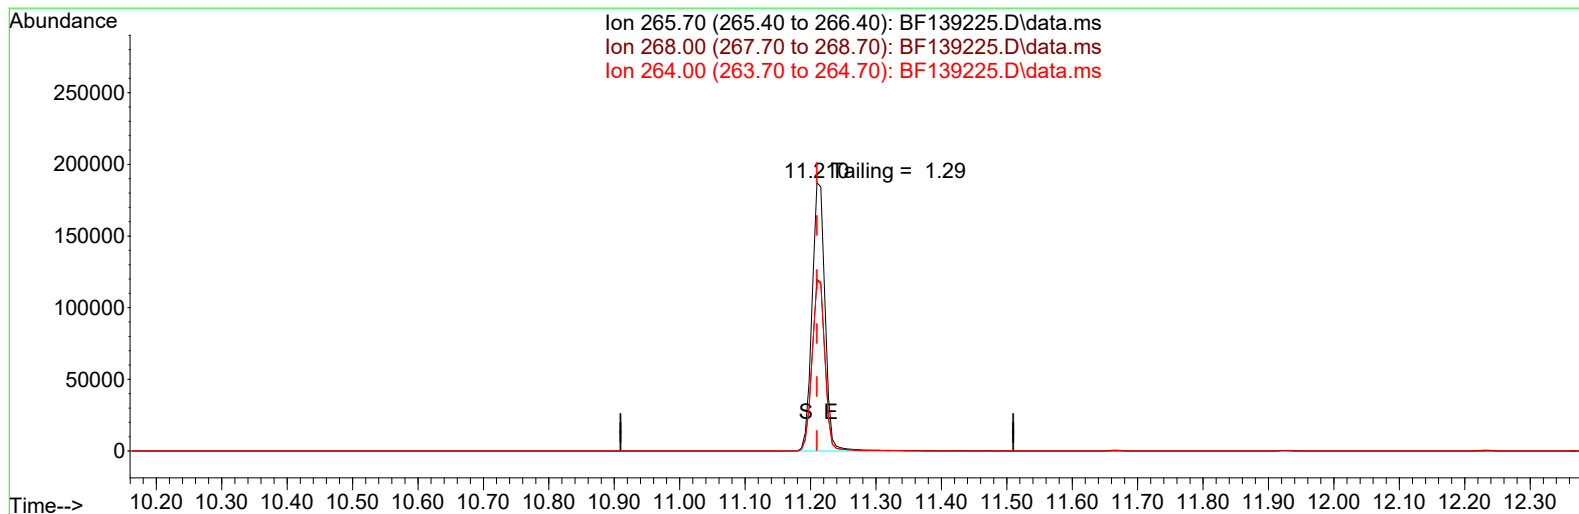

TIC: BF139225.D\data.ms

(70) Pentachlorophenol (C)




11.210min (-0.000) 27791.44 ng

response 257322

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	63.85
264.00	62.80	63.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090324\
Data File : BF139225.D
Acq On : 03 Sep 2024 09:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 03 11:15:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 29 15:46:29 2024
Response via : Initial Calibration

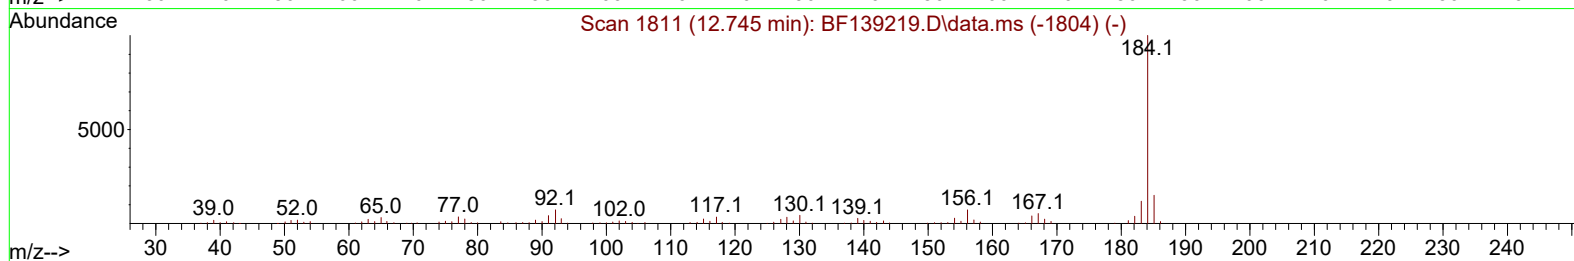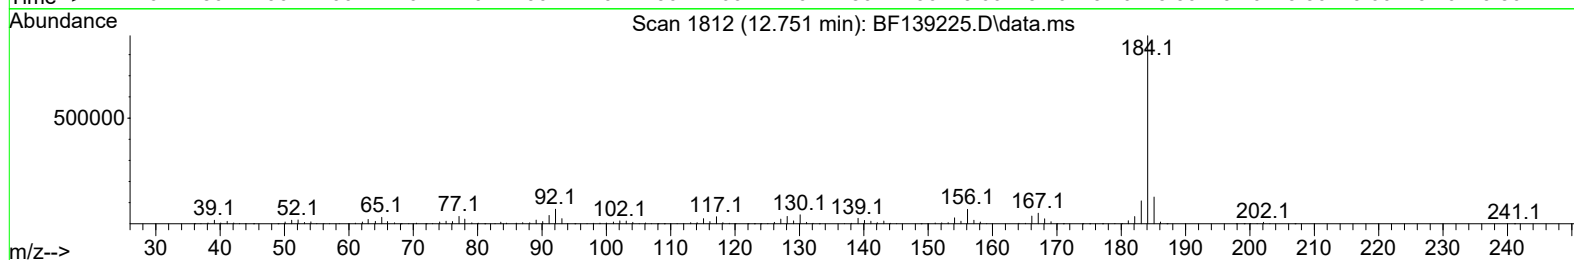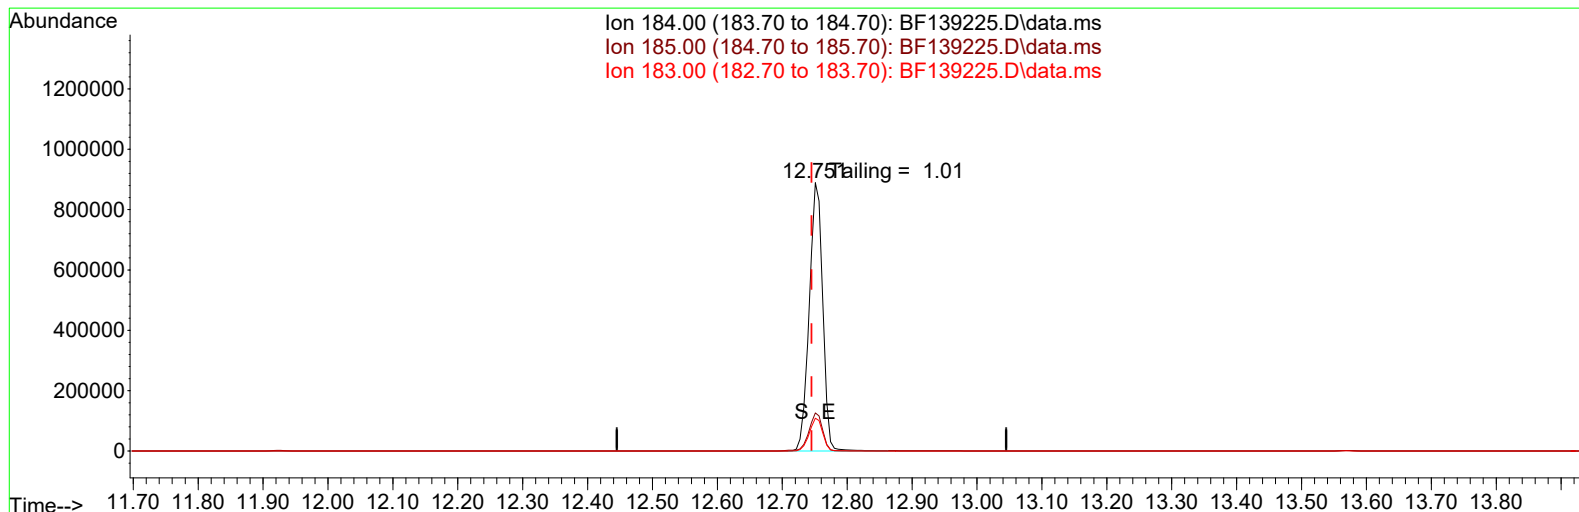

TIC: BF139225.D\data.ms

(77) Benzidine

12.751min (+ 0.006) 0.00 ng

response 1292313

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.21
183.00	11.90	12.23
0.00	0.00	0.00