
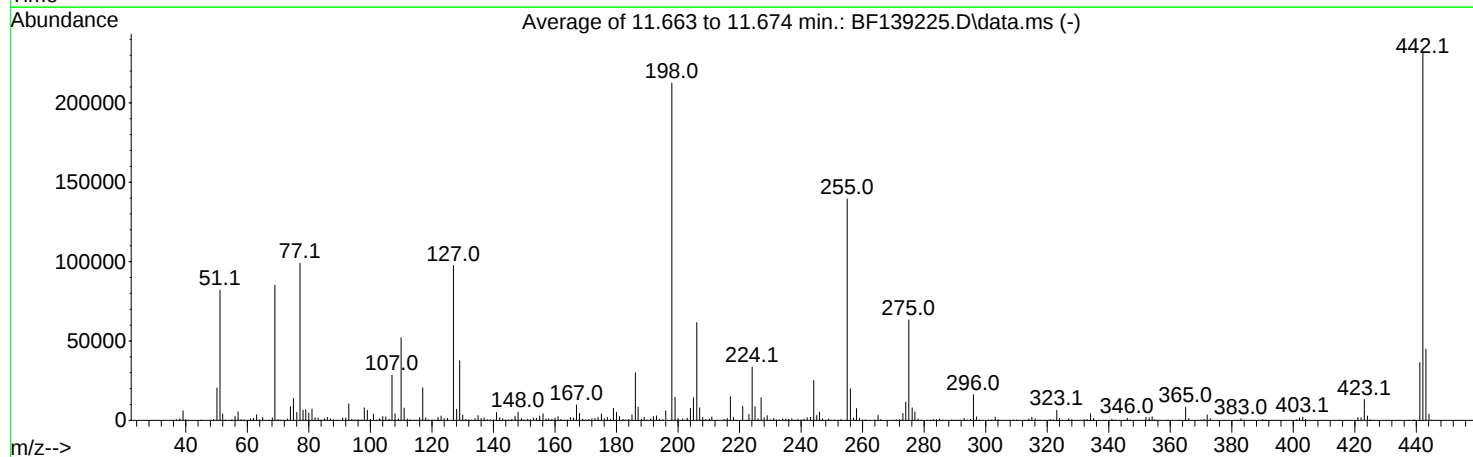


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090324\
Data File : BF139225.D
Acq On : 03 Sep 2024 09:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Aug 29 15:46:29 2024

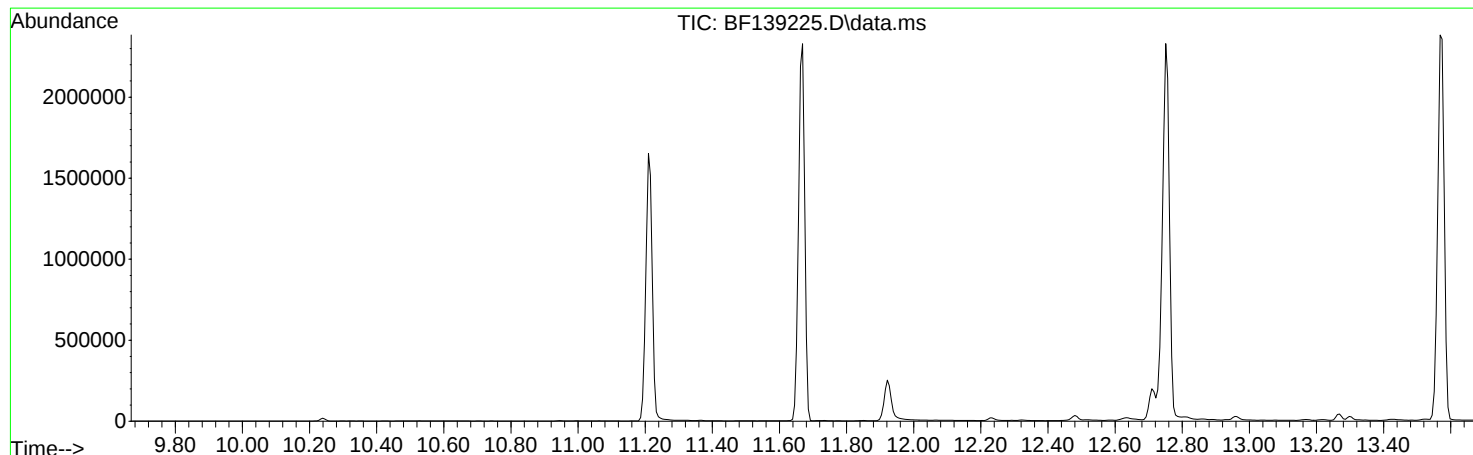




AutoFind: Scans 1627, 1628, 1629; Background Corrected with Scan 1620

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.6	82003	PASS
68	69	0.00	2	2.0	1659	PASS
69	198	0.00	100	40.0	85051	PASS
70	69	0.00	2	0.7	559	PASS
127	198	10	80	45.9	97549	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	212416	PASS
199	198	5	9	6.8	14506	PASS
275	198	10	60	29.8	63283	PASS
365	198	1	100	3.9	8267	PASS
441	198	0.01	100	17.1	36424	PASS
442	442	50	100	100.0	231723	PASS
443	442	15	24	19.4	44885	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090324\
Data File : BF139225.D
Acq On : 03 Sep 2024 09:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 03 11:15:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 29 15:46:29 2024
Response via : Initial Calibration

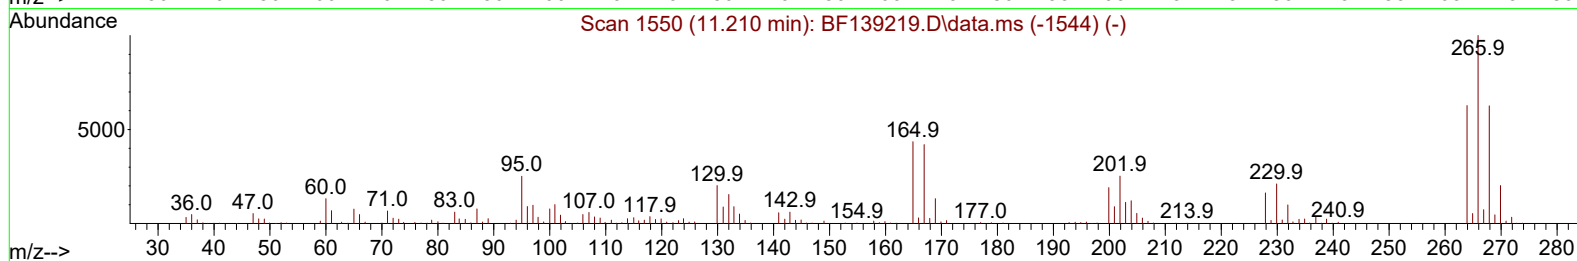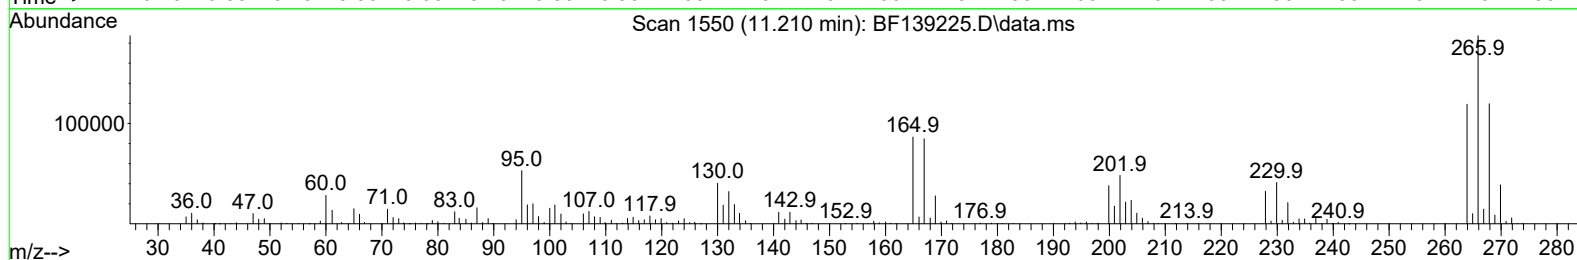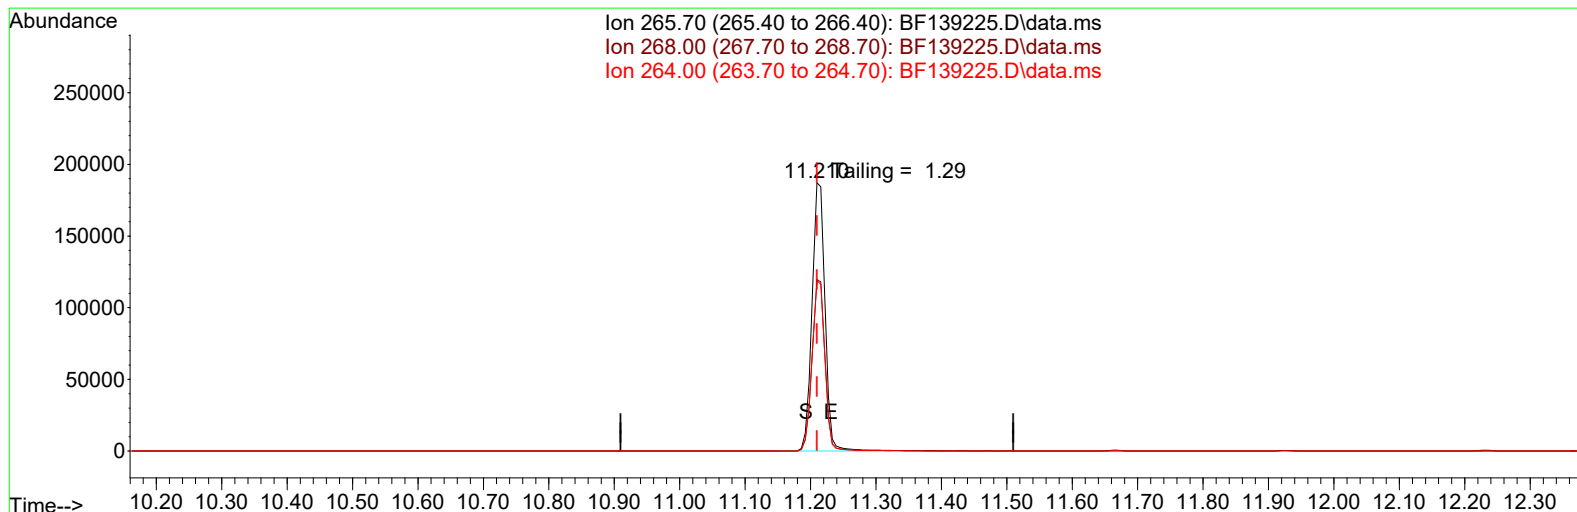

TIC: BF139225.D\data.ms

(70) Pentachlorophenol (C)

11.210min (-0.000) 27791.44 ng




response 257322

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	63.85
264.00	62.80	63.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090324\
Data File : BF139225.D
Acq On : 03 Sep 2024 09:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 03 11:15:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 29 15:46:29 2024
Response via : Initial Calibration

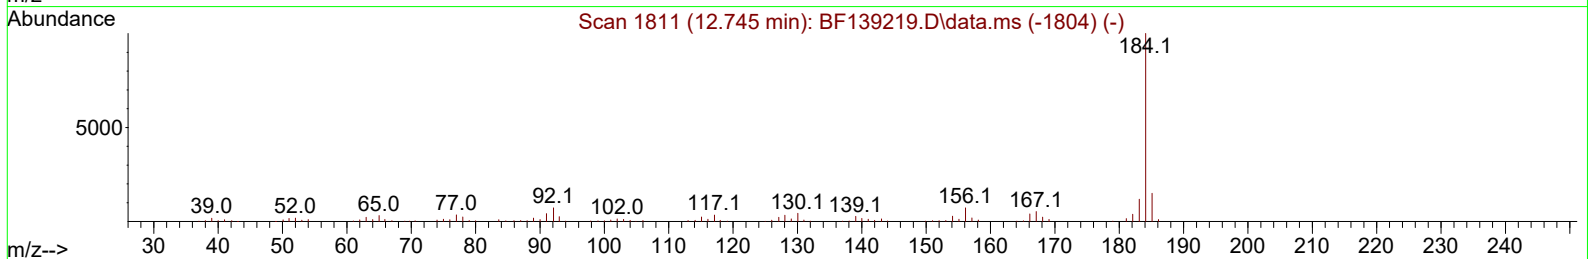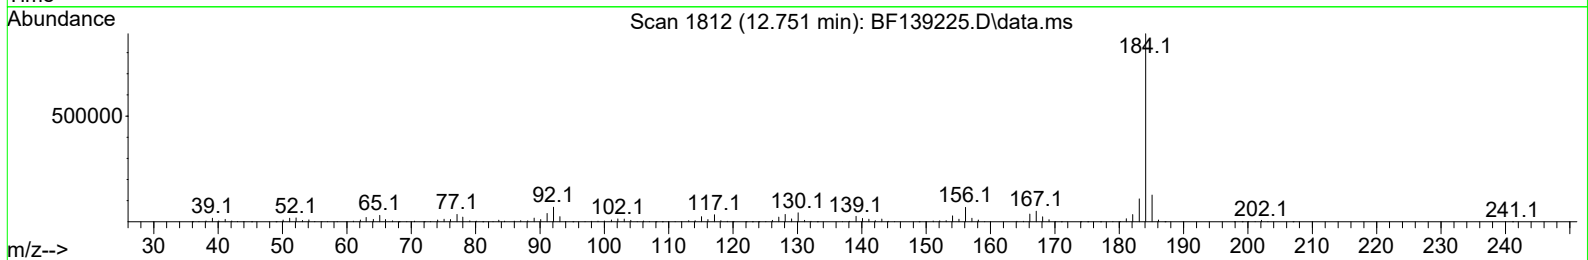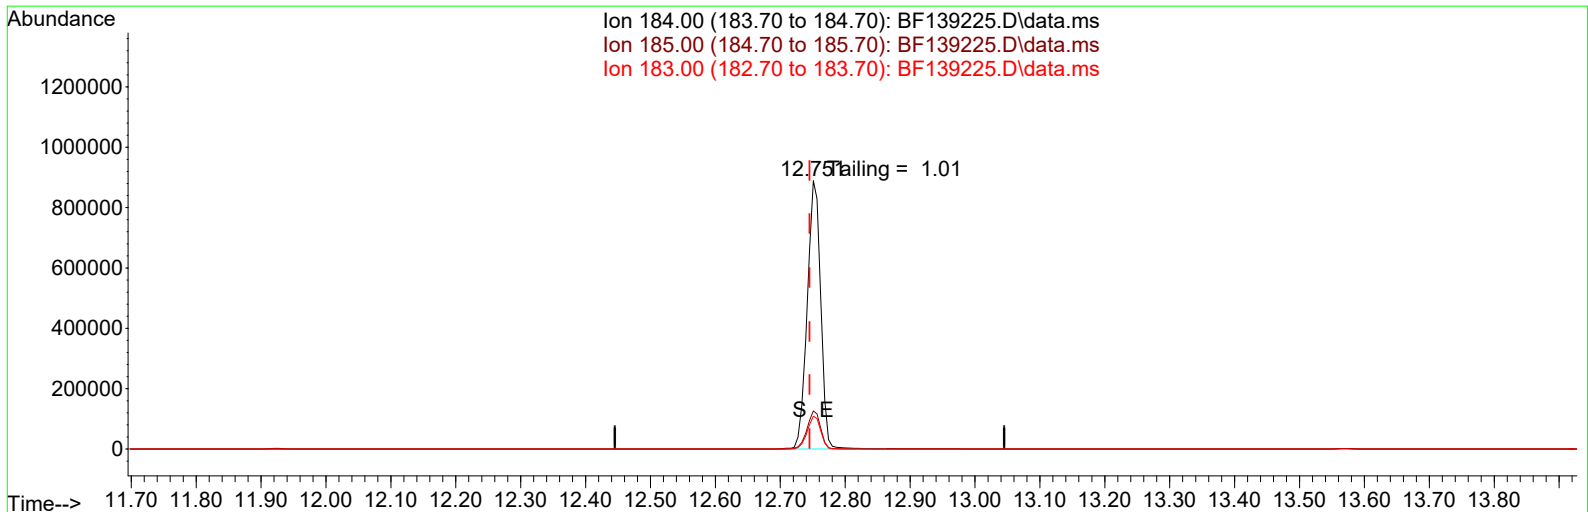

TIC: BF139225.D\data.ms

(77) Benzidine

12.751min (+ 0.006) 0.00 ng

response 1292313

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.21
183.00	11.90	12.23
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/3/2024	BNA_F	<u>BF139225.D</u>
Compound Name	Response	Retention Time
DDT	596959	13.574
DDD	14540	13.268
DDE	59	12.233
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14599	611558	2.39

Instrument :
BNA_F
ClientSampleId :
DFTPP