
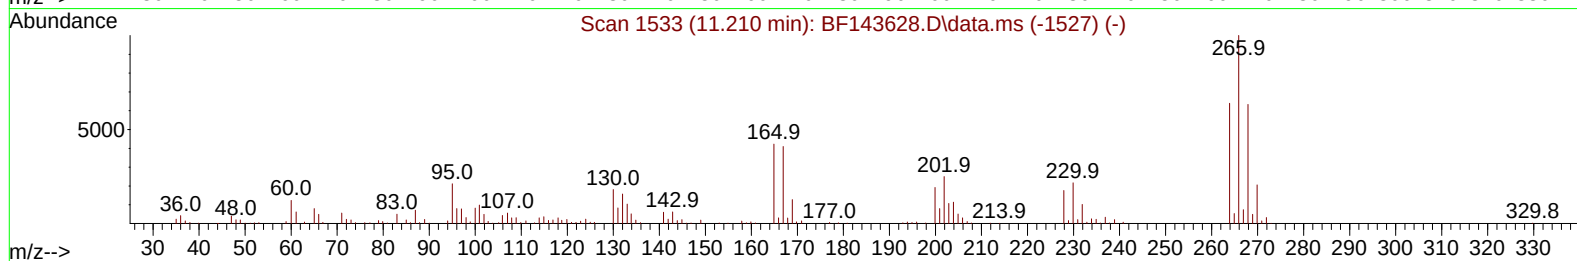
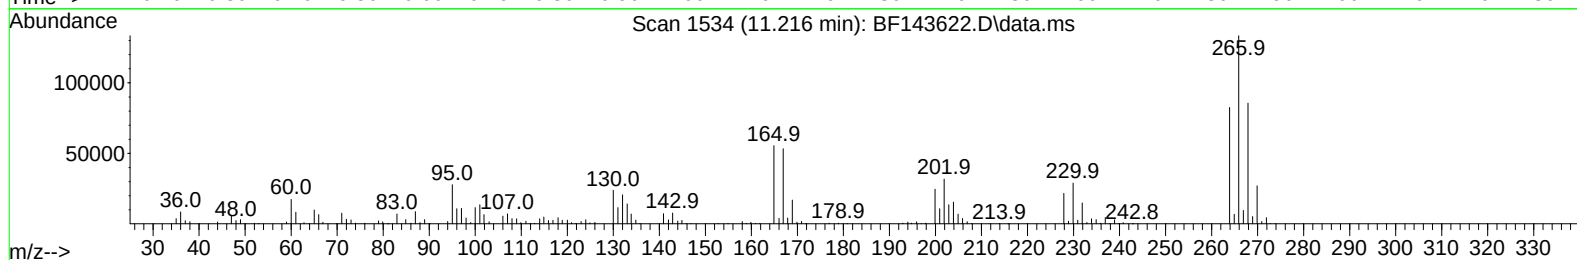


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090325\
Data File : BF143622.D
Acq On : 03 Sep 2025 12:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 03 18:25:23 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF090325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 03 18:14:10 2025
Response via : Initial Calibration

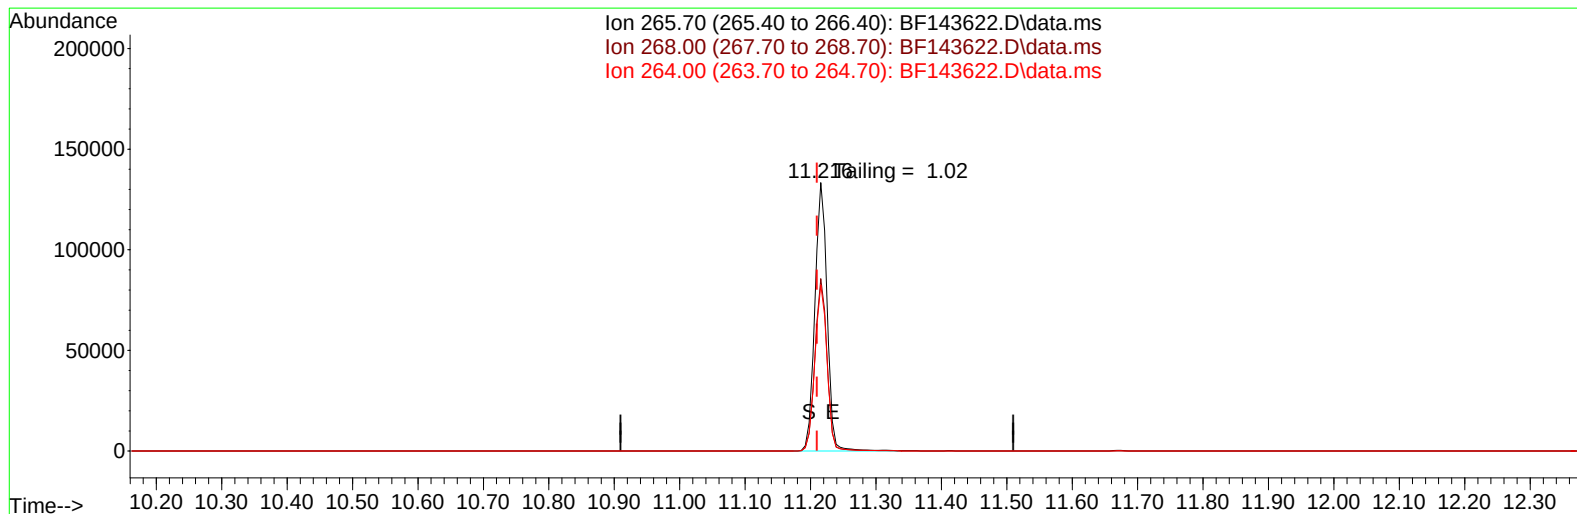

TIC: BF143622.D\data.ms

(70) Pentachlorophenol (C)




11.216min (+ 0.006) 22435.82 ng

response 173037

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	64.19
264.00	64.00	61.89
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090325\
Data File : BF143622.D
Acq On : 03 Sep 2025 12:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 03 18:25:23 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF090325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 03 18:14:10 2025
Response via : Initial Calibration

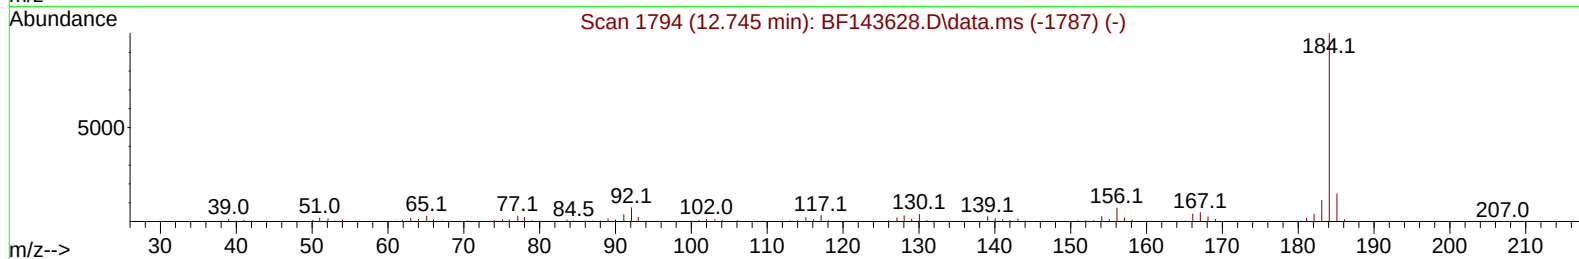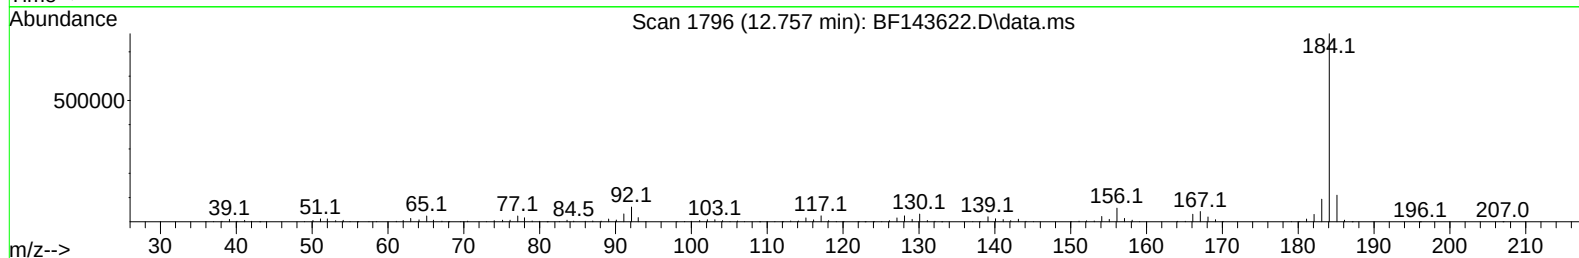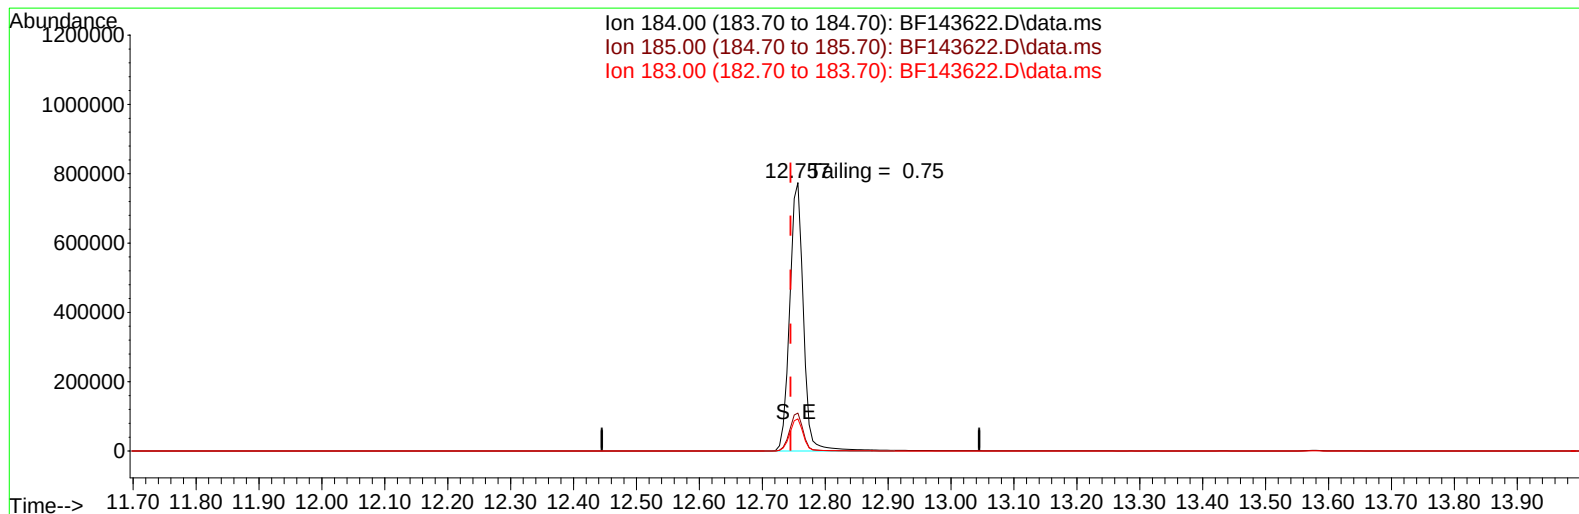

TIC: BF143622.D\data.ms

(77) Benzidine

12.757min (+ 0.012) 0.00 ng

response 1181043

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.15
183.00	11.30	12.00
0.00	0.00	0.00