

Data Path : Z:\HPCHEM1\BNA F\DATA\BF090415\
 Data File : BF081460.D
 Acq On : 5 Sep 2015 12:44
 Operator : UM/IZ
 Sample : G3511-09
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-07(0-0.16)

Quant Time: Sep 07 02:49:19 2015
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF090115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 07 02:47:26 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.35	152	54703	20.00	ng	-0.01
21) Naphthalene-d8	7.64	136	216205	20.00	ng	-0.01
38) Acenaphthene-d10	9.38	164	96822	20.00	ng	-0.01
63) Phenanthrene-d10	10.84	188	185757	20.00	ng	-0.01
75) Chrysene-d12	13.45	240	137377	20.00	ng	-0.01
86) Perylene-d12	14.77	264	105183	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	4.91	112	531337	150.70	ng	0.02
7) Phenol-d6	6.03	99	747244	160.11	ng	0.00
23) Nitrobenzene-d5	6.94	82	443694	99.01	ng	-0.01
41) 2,4,6-Tribromophenol	10.17	330	128937	149.56	ng	-0.01
44) 2-Fluorobiphenyl	8.73	172	737737	97.64	ng	0.00
78) Terphenyl-d14	12.43	244	615683	104.33	ng	0.00
Target Compounds						
15) Benzyl Alcohol	6.51	79	7694	2.01	ng	# 31
19) n-Nitroso-di-n-propylamine	6.94	70	62093	19.55	ng	# 62
25) Isophorone	6.94	82	323013	38.75	ng	# 58
49) Dimethylphthalate	9.13	163	163848	21.78	ng	# 97
56) 2,4-Dinitrotoluene	9.38	165	12197	5.61	ng	# 31
66) 4-Bromophenyl-phenylether	10.17	248	10317	5.49	ng	# 1
74) Fluoranthene	12.05	202	26332	2.36	ng	87
77) Pyrene	12.05	202	26332	2.59	ng	98
80) Benzo(a)anthracene	13.45	228	18121	2.07	ng	98
82) Chrysene	13.45	228	18121	2.31	ng	98
87) Benzo(b)fluoranthene	14.43	252	34754	4.63	ng	# 86
88) Benzo(k)fluoranthene	14.43	252	34754	5.58	ng	# 87
89) Benzo(a)pyrene	14.72	252	13905	2.19	ng	# 83
91) Benzo(a,h,i)perylene	16.15	276	10830	2.31	ng	# 74

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF090415\
Data File : BF081460.D
Acq On : 5 Sep 2015 12:44
Operator : UM/IZ
Sample : G3511-09
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-07(0-0.16)

Quant Time: Sep 07 02:49:19 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF090115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 07 02:47:26 2015
Response via : Initial Calibration

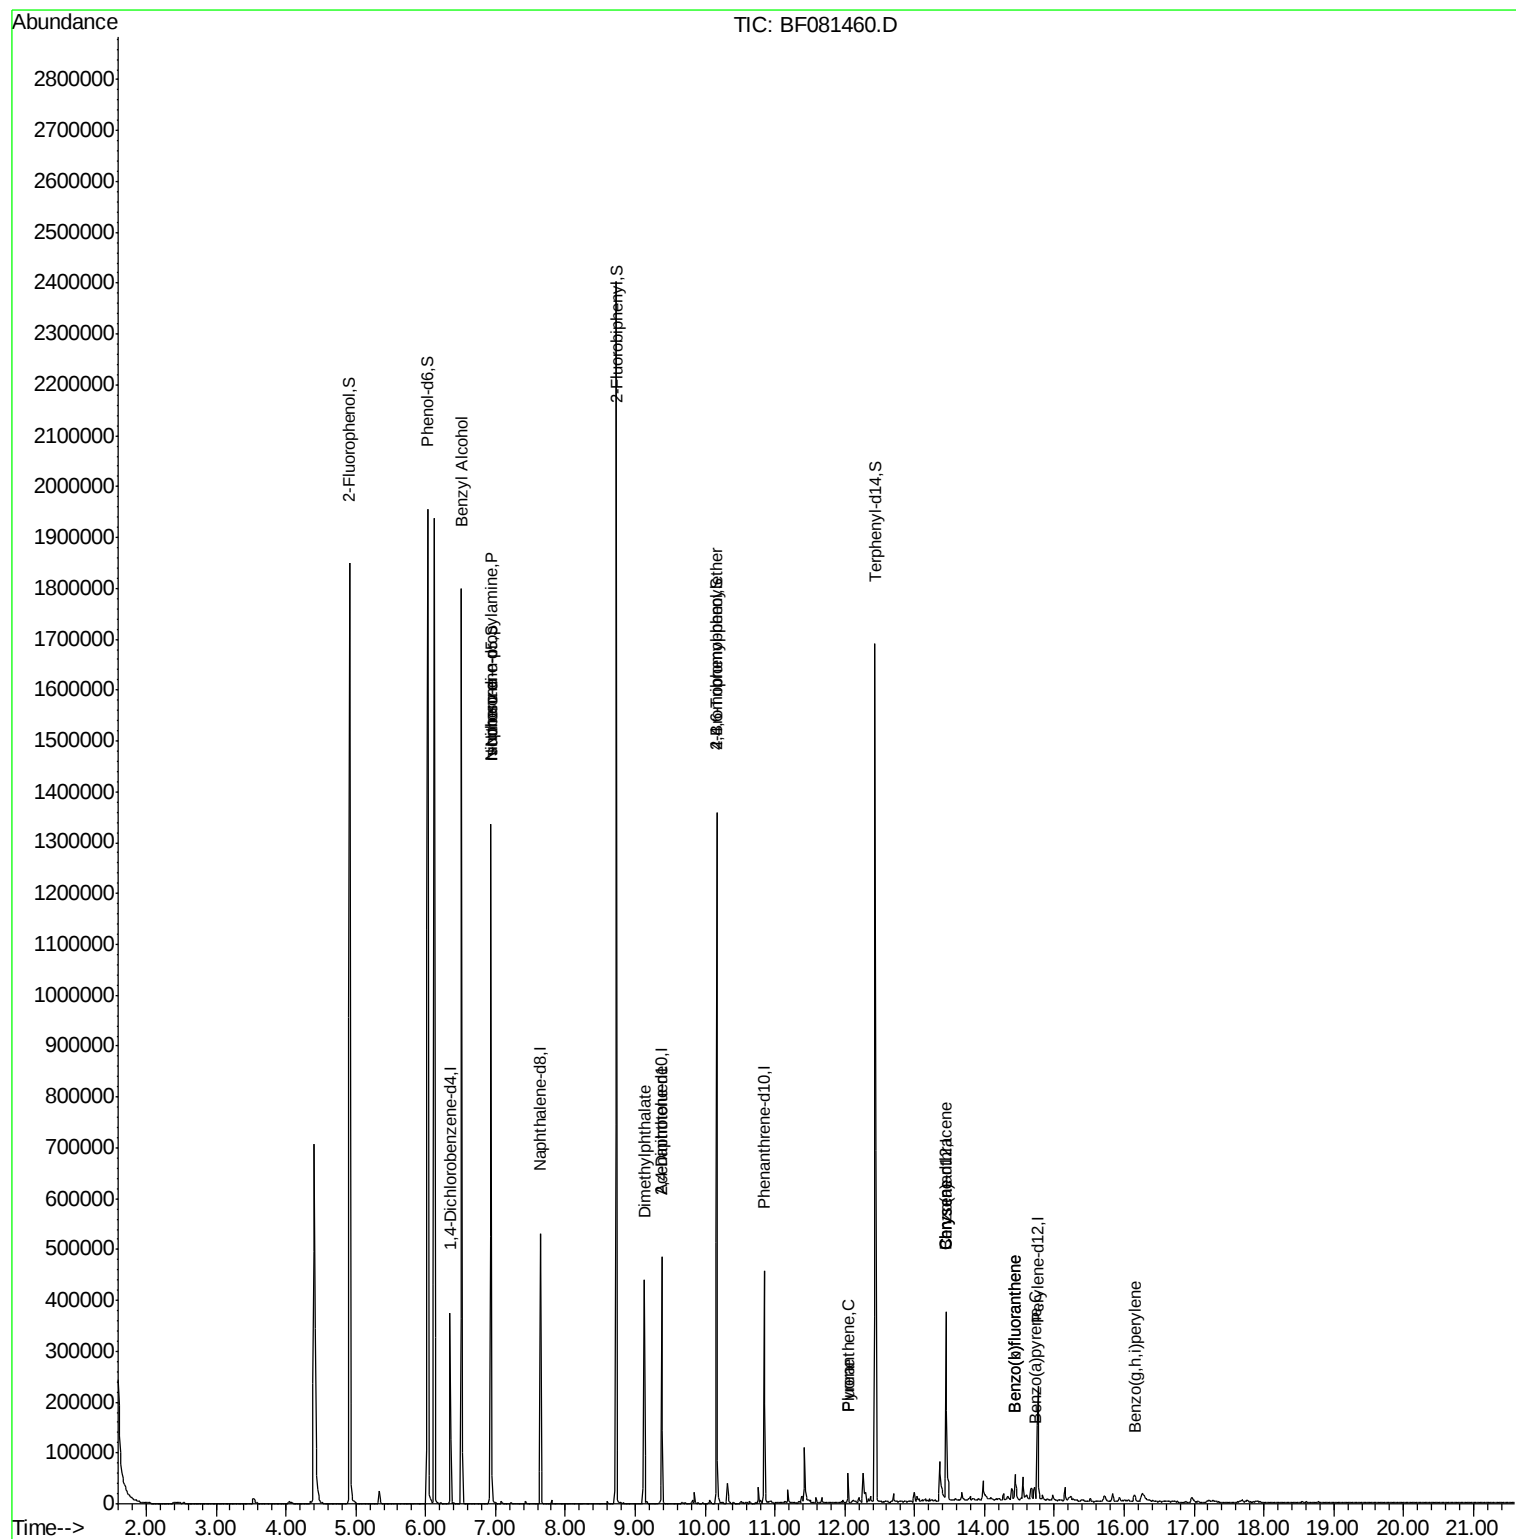




#1



1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.35 min Scan# 417
Delta R.T. -0.01 min
Lab File: BF081460.D
Acq: 5 Sep 2015 12:44

Instrument :
BNA_F
ClientSampleId :
SB-07(0-0.16)

Tot Ion:152 Resp: 54703
Ion Ratio Lower Upper
152 100
150 161.0 124.7 187.1
115 70.6 39.0 58.4#

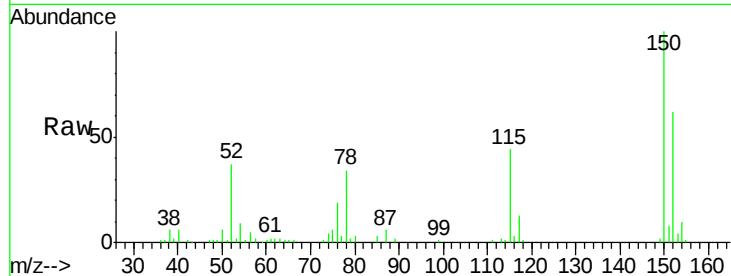


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

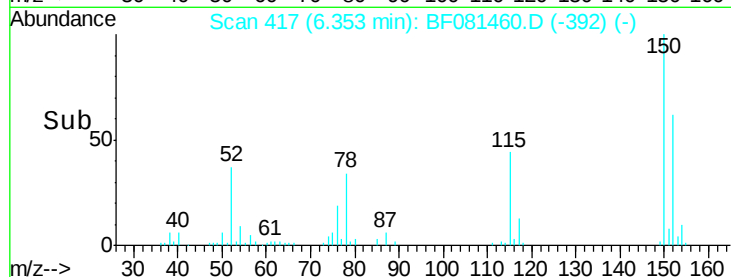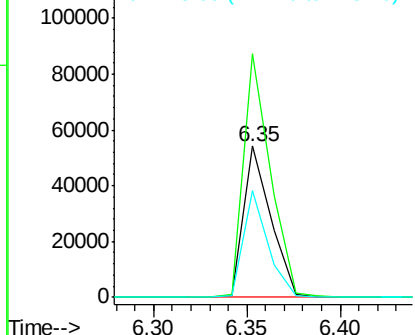



#5


2-Fluorophenol
Concen: 150.70 ng
RT: 4.91 min Scan# 291
Delta R.T. 0.02 min
Lab File: BF081460.D
Acq: 5 Sep 2015 12:44

Tgt Ion:112 Resp: 531337
Ion Ratio Lower Upper
112 100
64 72.6 39.7 59.5#
63 38.9 17.4 26.0#



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

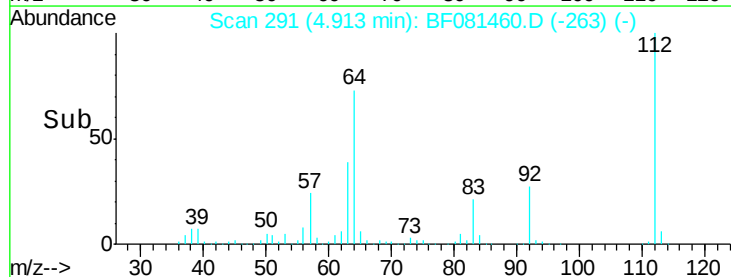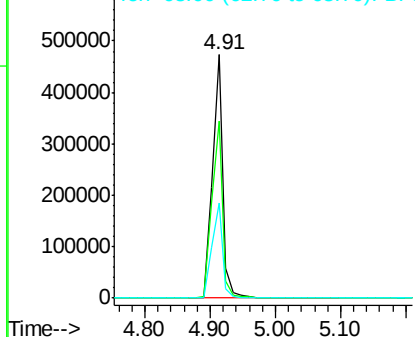

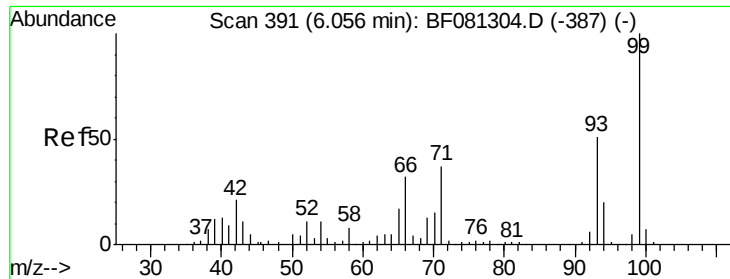

#7

Phenol-d6

Concen: 160.11 ng

RT: 6.03 min Scan# 389

Delta R.T. 0.00 min

Lab File: BF081460.D

Acq: 5 Sep 2015 12:44

Instrument :

BNA_F

ClientSampleId :

SB-07(0-0.16)


Tot Ion: 99 Resp: 747244

Ion Ratio Lower Upper

99 100

42 21.1 13.7 20.5#




71 37.8 14.2 21.2#



Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

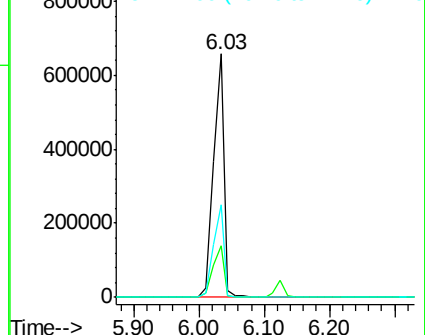

#15

Benzyl Alcohol

Concen: 2.01 ng

RT: 6.51 min Scan# 431

Delta R.T. -0.01 min

Lab File: BF081460.D

Acq: 5 Sep 2015 12:44


Tgt Ion: 79 Resp: 7694

Ion Ratio Lower Upper

79 100

108 25.7 88.6 132.8#



77 94.3 47.0 70.4#

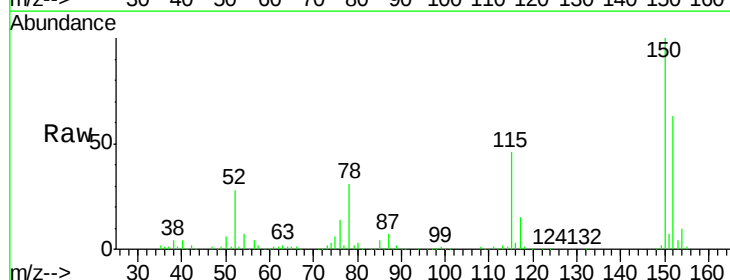


Abundance Ion 79.00 (78.70 to 79.70): BF0

Ion 108.00 (107.70 to 108.70): BF0

Ion 77.00 (76.70 to 77.70): BF0



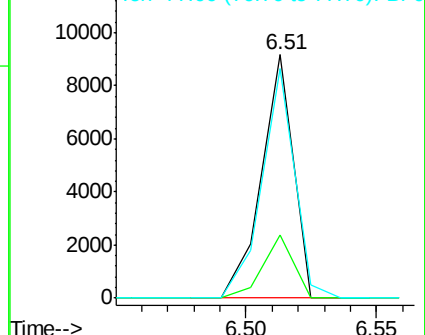





#19
n-Nitroso-di-n-propylamine
Concen: 19.55 ng
RT: 6.94 min Scan# 468
Delta R.T. 0.13 min
Lab File: BF081460.D
Acq: 5 Sep 2015 12:44




Instrument :
BNA_F
ClientSampleId :
SB-07(0-0.16)

Tot Ion: 70 Resp: 62093
Ion Ratio Lower Upper
70 100
42 51.5 63.8 95.6#
101 0.0 9.2 13.8#
130 1.9 27.3 40.9#

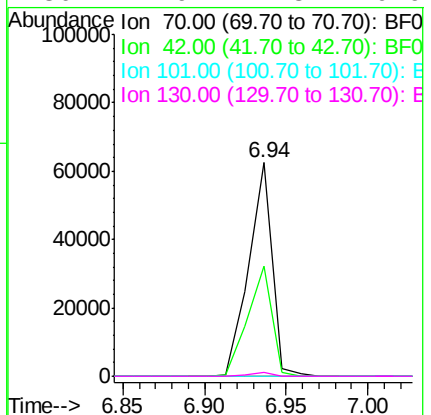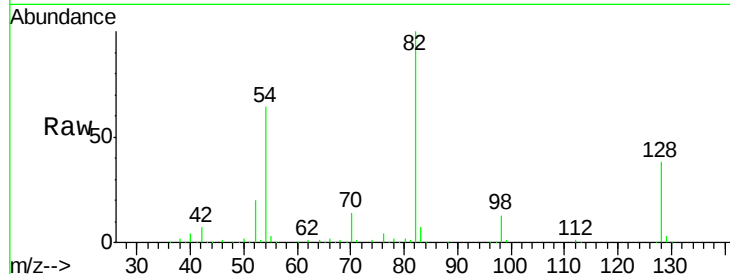

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 7.64 min Scan# 530
Delta R.T. -0.01 min
Lab File: BF081460.D
Acq: 5 Sep 2015 12:44

Tgt Ion: 136 Resp: 216205
Ion Ratio Lower Upper
136 100
137 11.0 9.0 13.6
54 11.6 8.2 12.2
68 5.1 5.8 8.6#


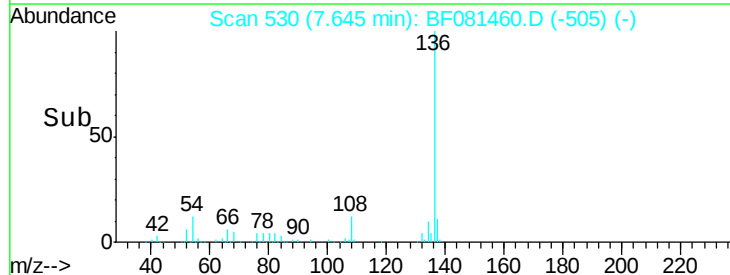
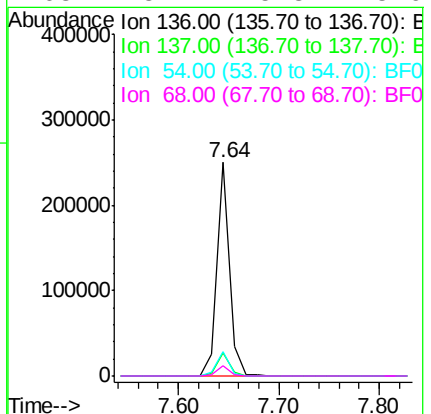





#23
 Nitrobenzene-d5
 Concen: 99.01 ng
 RT: 6.94 min Scan# 468
 Delta R.T. -0.01 min
 Lab File: BF081460.D
 Acq: 5 Sep 2015 12:44




Instrument :
 BNA_F
 ClientSampleId :
 SB-07(0-0.16)


Tot Ion: 82 Resp: 443694
 Ion Ratio Lower Upper
 82 100
 128 37.5 51.0 76.6#
 54 63.9 47.5 71.3

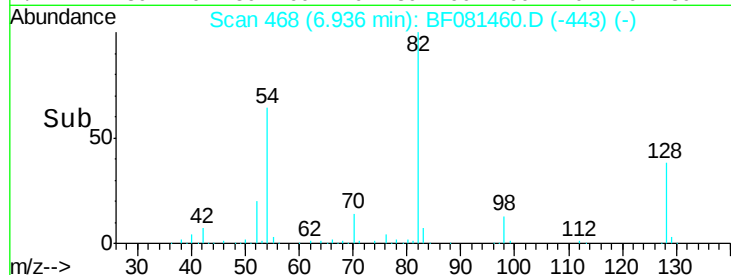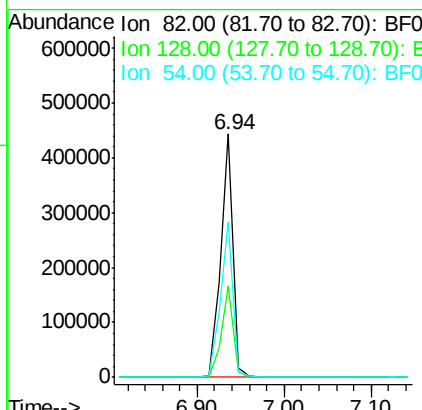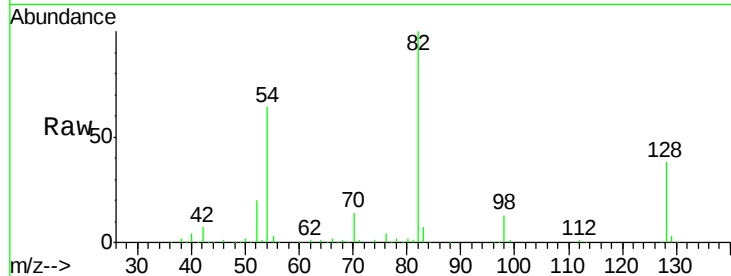

#25
 Isophorone
 Concen: 38.75 ng
 RT: 6.94 min Scan# 468
 Delta R.T. -0.27 min
 Lab File: BF081460.D
 Acq: 5 Sep 2015 12:44

Tgt Ion: 82 Resp: 323013
 Ion Ratio Lower Upper
 82 100
 95 0.0 4.0 6.0#
 138 0.0 18.3 27.5#

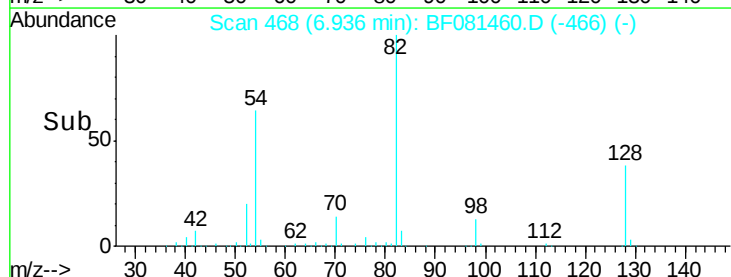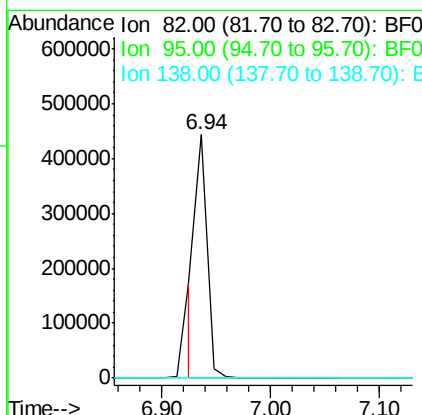

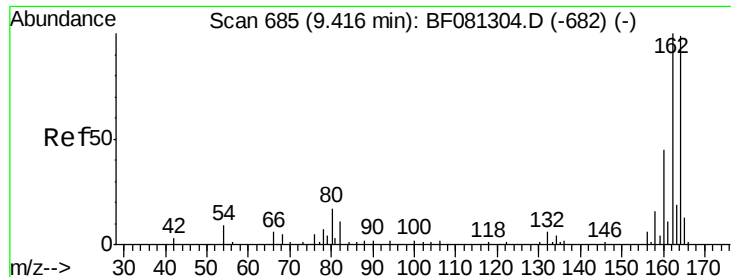

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.38 min Scan# 682

Delta R.T. -0.01 min

Lab File: BF081460.D

Acq: 5 Sep 2015 12:44

Instrument :

BNA_F

ClientSampleId :

SB-07(0-0.16)


Tot Ion:164 Resp: 96822

Ion Ratio Lower Upper

164 100

162 101.6 75.2 112.8




160 44.6 31.5 47.3



Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

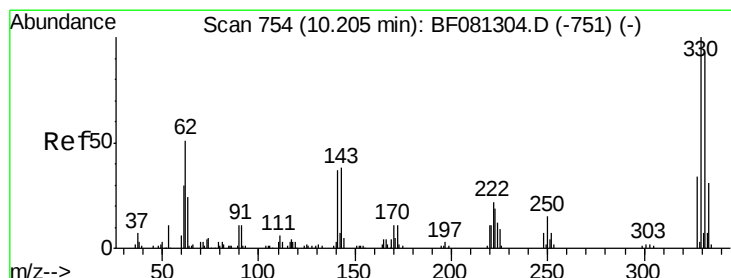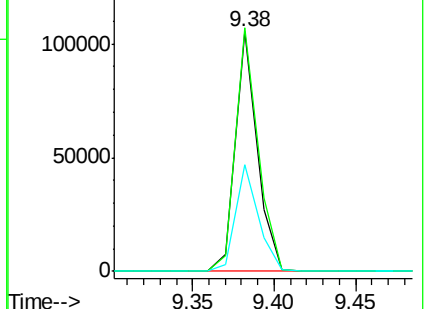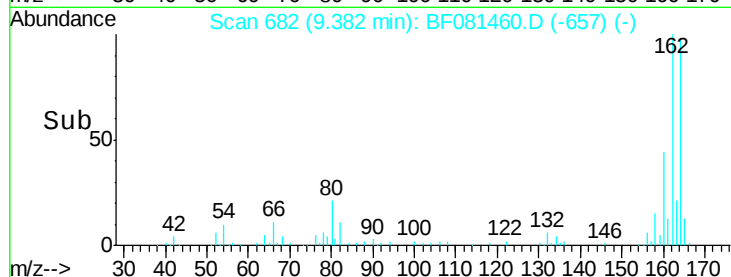

#41

2,4,6-Tribromophenol

Concen: 149.56 ng

RT: 10.17 min Scan# 751

Delta R.T. -0.01 min

Lab File: BF081460.D

Acq: 5 Sep 2015 12:44


Tgt Ion:330 Resp: 128937

Ion Ratio Lower Upper

330 100

332 94.4 76.6 114.8



141 54.1 29.7 44.5#




Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



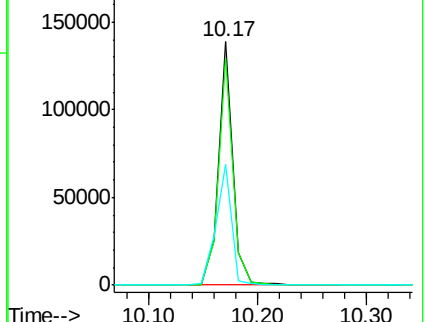
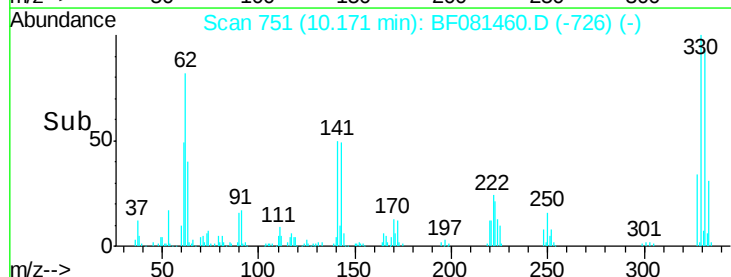


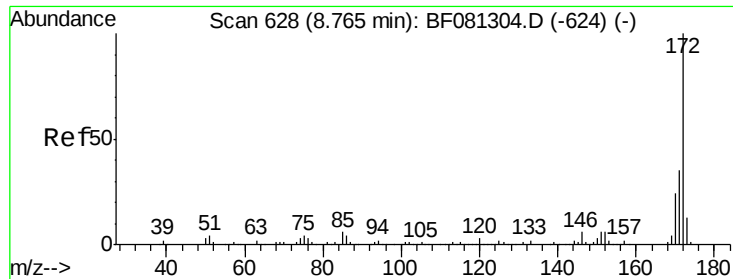

#44
 2-Fluorobiphenyl
 Concen: 97.64 ng
 RT: 8.73 min Scan# 625
 Delta R.T. 0.00 min
 Lab File: BF081460.D
 Acq: 5 Sep 2015 12:44




Instrument :
 BNA_F
 ClientSampleId :
 SB-07(0-0.16)


Tot Ion:172 Resp: 737737
 Ion Ratio Lower Upper
 172 100
 171 35.9 26.1 39.1
 170 24.3 17.4 26.2

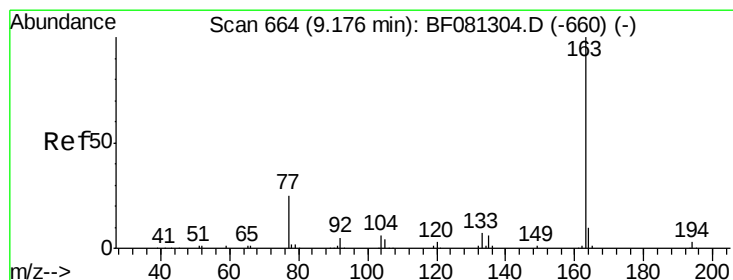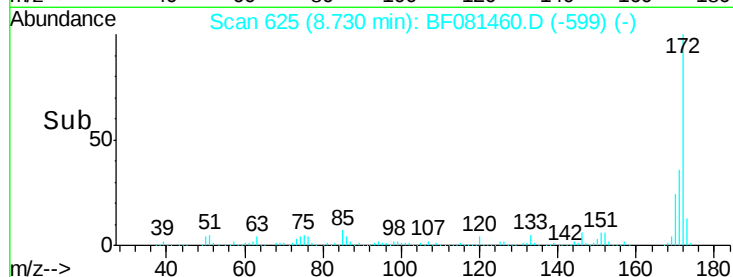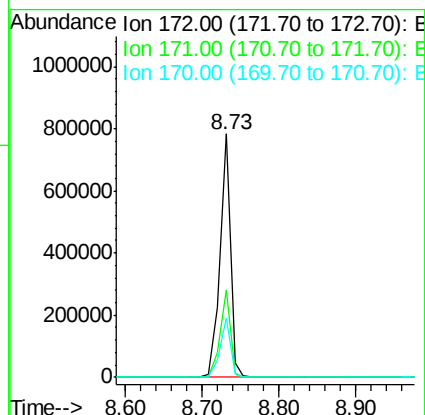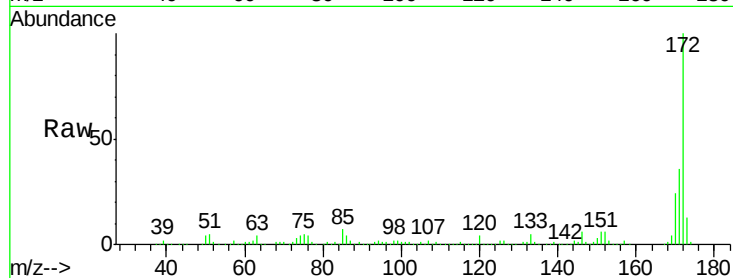

#49
 Dimethylphthalate
 Concen: 21.78 ng
 RT: 9.13 min Scan# 660
 Delta R.T. -0.02 min
 Lab File: BF081460.D
 Acq: 5 Sep 2015 12:44

Tgt Ion:163 Resp: 163848
 Ion Ratio Lower Upper
 163 100
 194 2.9 4.4 6.6#
 164 10.0 8.3 12.5

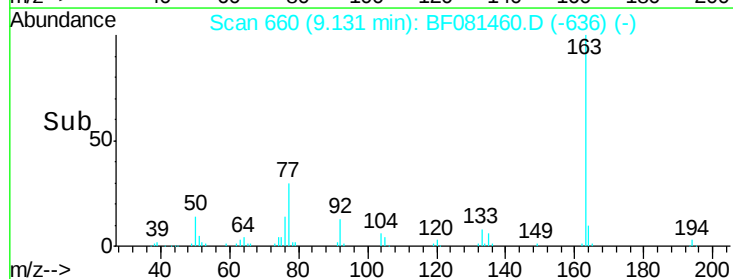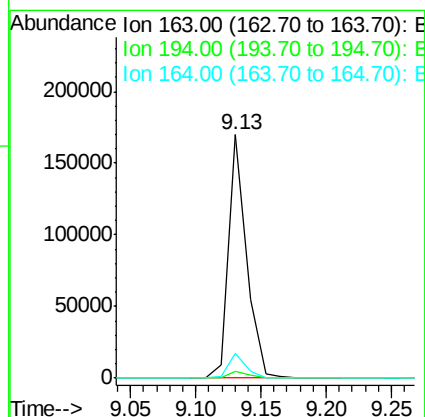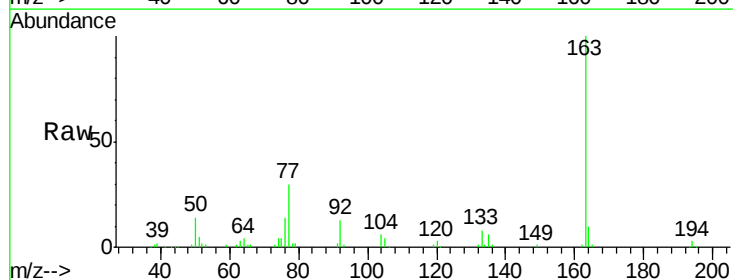


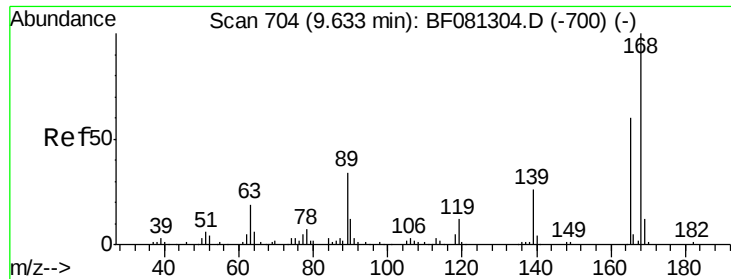

#56
 2,4-Dinitrotoluene
 Concen: 5.61 ng
 RT: 9.38 min Scan# 682
 Delta R.T. -0.22 min
 Lab File: BF081460.D
 Acq: 5 Sep 2015 12:44

Instrument :
 BNA_F
 ClientSampleId :
 SB-07(0-0.16)

Tot Ion:	165	Resp:	12197
Ion	Ratio	Lower	Upper
165	100		
63	0.0	29.8	44.6#
89	0.0	44.5	66.7#
182	0.0	3.0	4.4#






Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF0


Ion 89.00 (88.70 to 89.70): BF0

Ion 182.00 (181.70 to 182.70): E

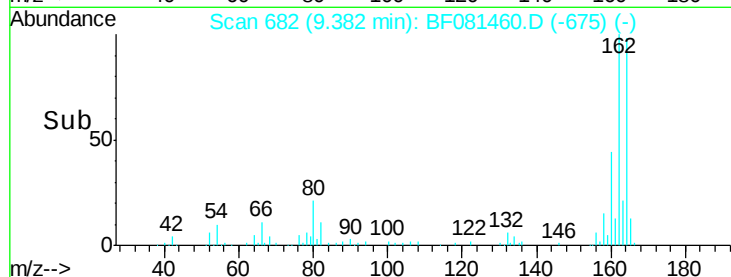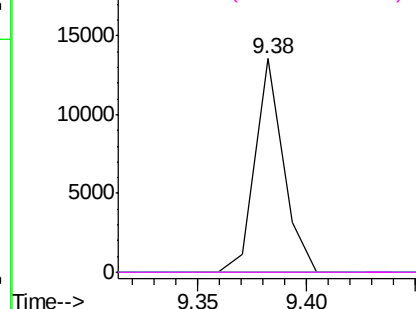

#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 10.84 min Scan# 810
 Delta R.T. -0.01 min
 Lab File: BF081460.D
 Acq: 5 Sep 2015 12:44



Tgt Ion:	188	Resp:	185757
Ion	Ratio	Lower	Upper
188	100		
94	10.2	11.1	16.7#
80	11.6	11.0	16.4




Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

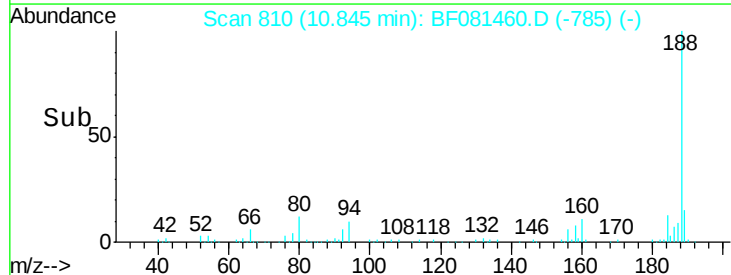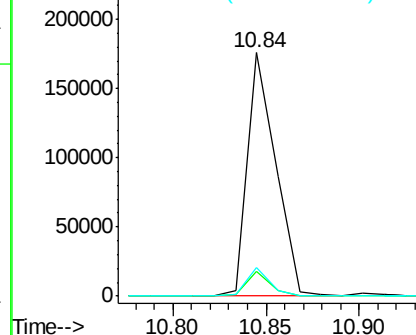


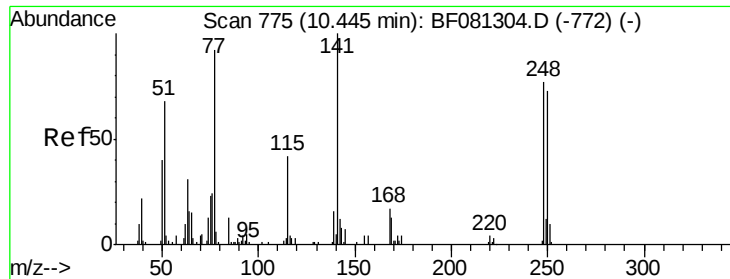




#66
4-Bromophenyl-phenylether
Concen: 5.49 ng
RT: 10.17 min Scan# 751
Delta R.T. -0.25 min
Lab File: BF081460.D
Acq: 5 Sep 2015 12:44

Instrument :
BNA_F
ClientSampleId :
SB-07(0-0.16)

Tot Ion:248 Resp: 10317
Ion Ratio Lower Upper
248 100
250 188.5 78.5 117.7#
141 600.8 59.0 88.6#

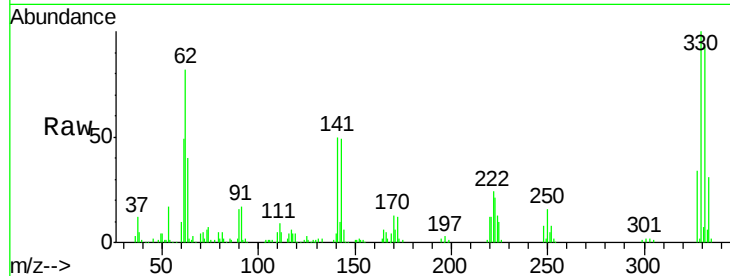


Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E


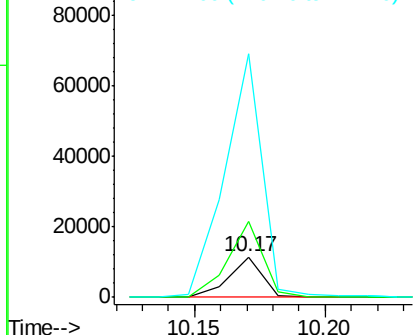



#74
Fluoranthene
Concen: 2.36 ng
RT: 12.05 min Scan# 915
Delta R.T. 0.00 min
Lab File: BF081460.D
Acq: 5 Sep 2015 12:44

Tgt Ion:202 Resp: 26332
Ion Ratio Lower Upper
202 100
101 8.4 0.0 38.3
203 16.1 0.0 37.3



Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 203.00 (202.70 to 203.70): E

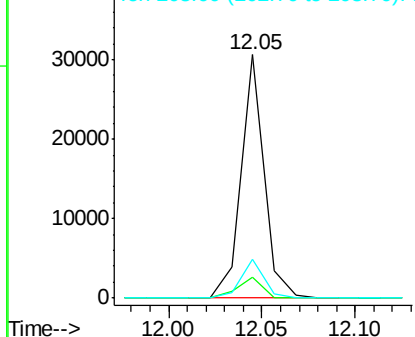

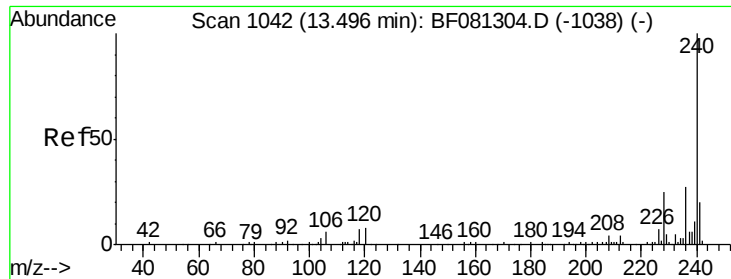

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.45 min Scan# 1038

Delta R.T. -0.01 min

Lab File: BF081460.D

Acq: 5 Sep 2015 12:44

Instrument :

BNA_F

ClientSampleId :

SB-07(0-0.16)


Tot Ion:240 Resp: 137377

Ion Ratio Lower Upper

240 100

120 12.5 16.2 24.2#




236 25.9 18.4 27.6

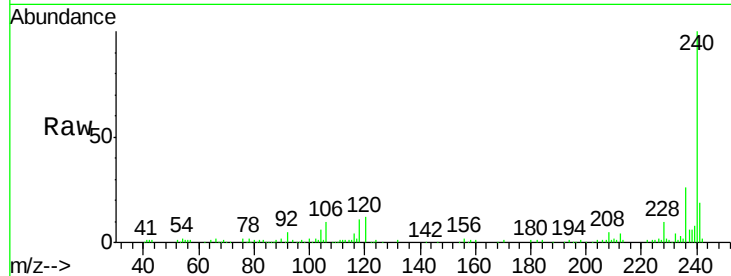

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

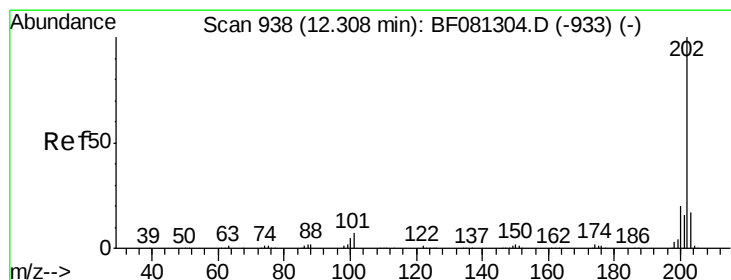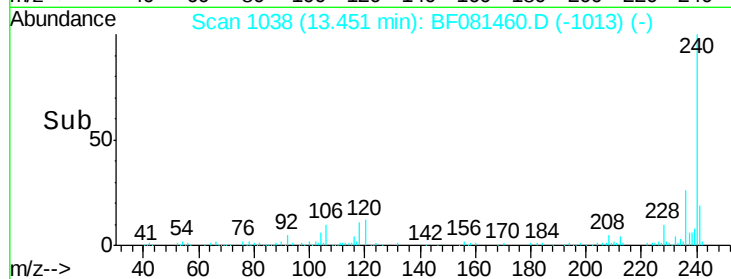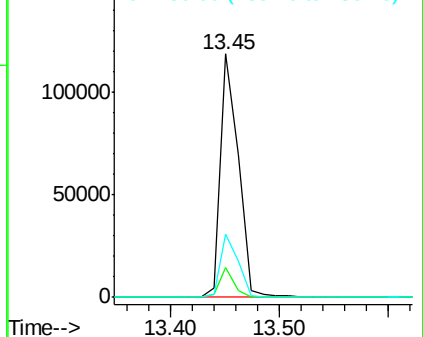

#77

Pyrene

Concen: 2.59 ng

RT: 12.05 min Scan# 915

Delta R.T. -0.23 min

Lab File: BF081460.D

Acq: 5 Sep 2015 12:44


Tgt Ion:202 Resp: 26332

Ion Ratio Lower Upper

202 100

200 18.2 15.0 22.4



203 16.1 14.1 21.1




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E



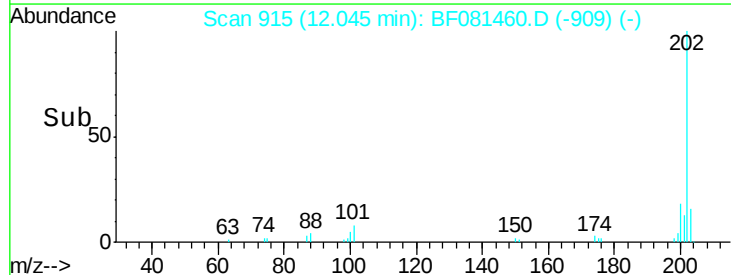
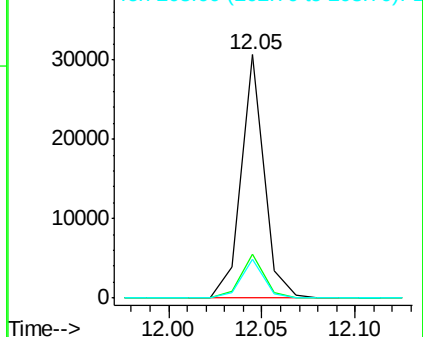


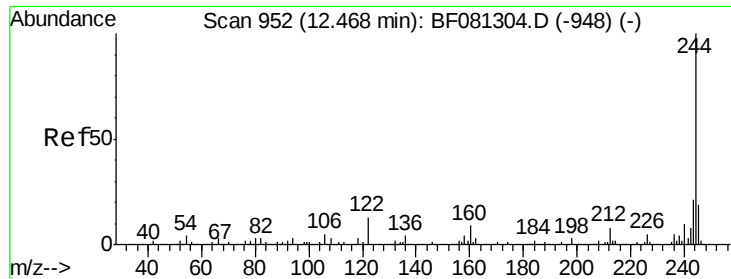

#78
 Terphenyl-d14
 Concen: 104.33 ng
 RT: 12.43 min Scan# 949
 Delta R.T. 0.00 min
 Lab File: BF081460.D
 Acq: 5 Sep 2015 12:44




Instrument :
 BNA_F
 ClientSampleId :
 SB-07(0-0.16)


Tot Ion:244 Resp: 615683
 Ion Ratio Lower Upper
 244 100
 212 8.3 4.3 6.5#
 122 14.1 17.4 26.2#

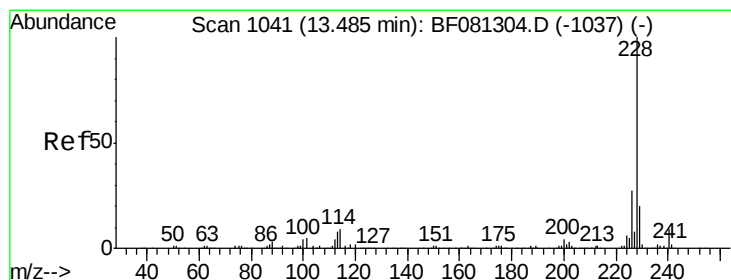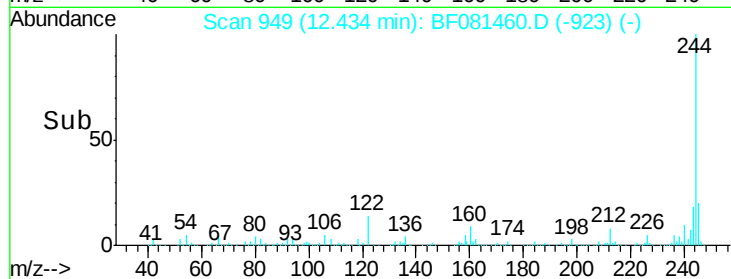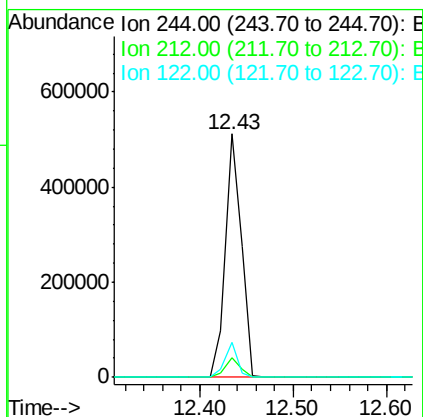

#80
 Benzo(a)anthracene
 Concen: 2.07 ng
 RT: 13.45 min Scan# 1038
 Delta R.T. 0.00 min
 Lab File: BF081460.D
 Acq: 5 Sep 2015 12:44

Tgt Ion:228 Resp: 18121
 Ion Ratio Lower Upper
 228 100
 226 25.8 20.0 30.0
 229 20.8 15.4 23.2

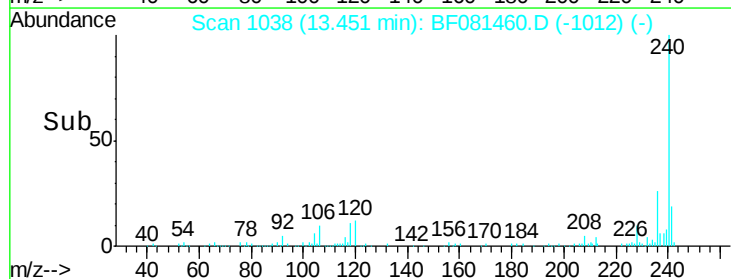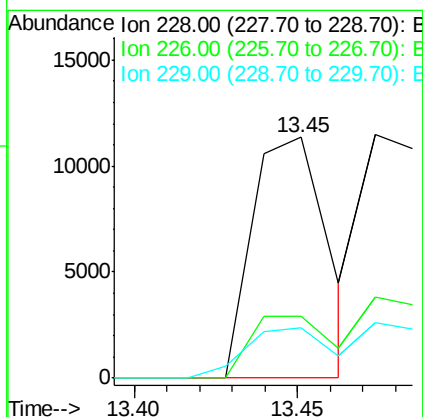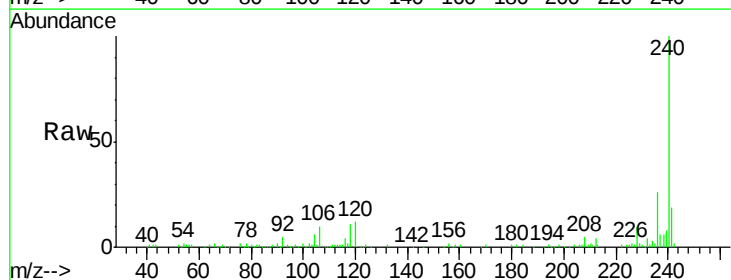



#82

Chrysene

Concen: 2.31 ng

RT: 13.45 min Scan# 1038

Delta R.T. -0.03 min

Lab File: BF081460.D

Acq: 5 Sep 2015 12:44

Instrument :

BNA_F

ClientSampleId :

SB-07(0-0.16)


Tot Ion:228 Resp: 18121

Ion Ratio Lower Upper

228 100

226 25.8 21.0 31.4




229 20.8 15.6 23.4



Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

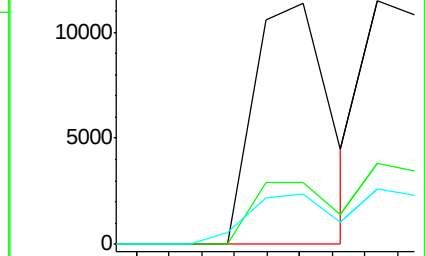

#86

Perylene-d12

Concen: 20.00 ng

RT: 14.77 min Scan# 1153

Delta R.T. 0.00 min

Lab File: BF081460.D

Acq: 5 Sep 2015 12:44


Tgt Ion:264 Resp: 105183

Ion Ratio Lower Upper

264 100

260 24.3 16.7 25.1



265 21.6 17.2 25.8




Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

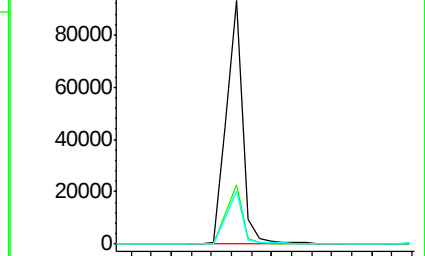



#87

Benzo(b)fluoranthene

Concen: 4.63 ng

RT: 14.43 min Scan# 1124

Delta R.T. -0.01 min

Lab File: BF081460.D

Acq: 5 Sep 2015 12:44

Instrument :

BNA_F

ClientSampleId :

SB-07(0-0.16)


Tot Ion:252 Resp: 34754

Ion Ratio Lower Upper

252 100

253 23.7 17.5 26.3




125 10.3 17.1 25.7#



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

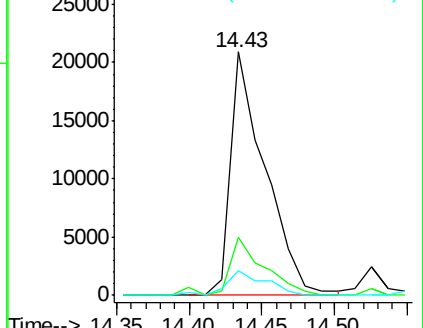

#88

Benzo(k)fluoranthene

Concen: 5.58 ng

RT: 14.43 min Scan# 1124

Delta R.T. -0.03 min

Lab File: BF081460.D

Acq: 5 Sep 2015 12:44


Tgt Ion:252 Resp: 34754

Ion Ratio Lower Upper

252 100

253 23.7 17.0 25.4



125 10.3 16.0 24.0#




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

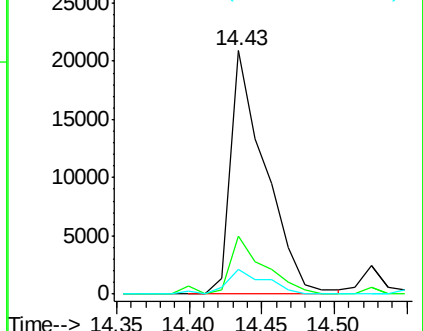

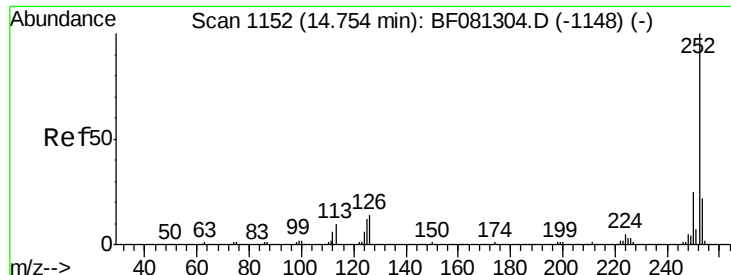

#89

Benzo(a)pyrene

Concen: 2.19 ng

RT: 14.72 min Scan# 1149

Delta R.T. 0.00 min

Lab File: BF081460.D

Acq: 5 Sep 2015 12:44

Instrument :

BNA_F

ClientSampleId :

SB-07(0-0.16)


Tot Ion:252 Resp: 13905

Ion Ratio Lower Upper

252 100

253 23.3 17.2 25.8




125 7.9 18.0 27.0#

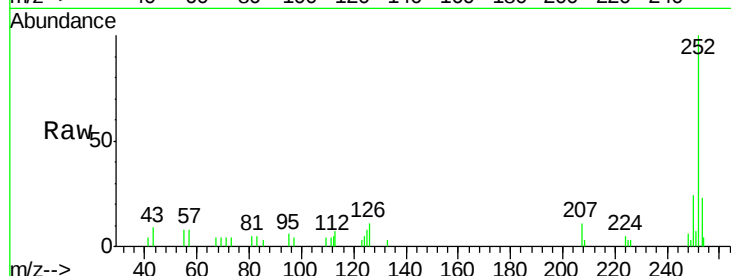

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

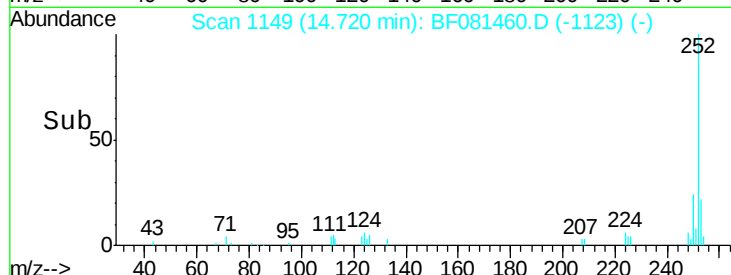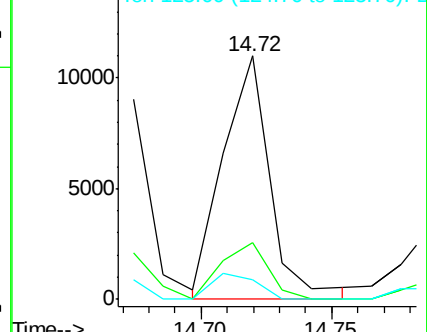

#91

Benzo(g,h,i)perylene

Concen: 2.31 ng

RT: 16.15 min Scan# 1274

Delta R.T. -0.01 min

Lab File: BF081460.D

Acq: 5 Sep 2015 12:44


Tgt Ion:276 Resp: 10830

Ion Ratio Lower Upper

276 100

277 27.4 17.8 26.6#

138 21.1 34.6 51.8#



Abundance Ion 276.00 (275.70 to 276.70): E

Ion 277.00 (276.70 to 277.70): E

Ion 138.00 (137.70 to 138.70): E

