

Data Path : Z:\HPCHEM1\BNA F\DATA\BF090415\
 Data File : BF081468.D
 Acq On : 5 Sep 2015 16:50
 Operator : UM/IZ
 Sample : G3559-02
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MGP226BR-40-42

Quant Time: Sep 07 02:51:01 2015
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF090115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 07 02:47:26 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.35	152	53846	20.00	ng	-0.01
21) Naphthalene-d8	7.64	136	209844	20.00	ng	-0.01
38) Acenaphthene-d10	9.38	164	95174	20.00	ng	-0.01
63) Phenanthrene-d10	10.85	188	181767	20.00	ng	-0.01
75) Chrysene-d12	13.45	240	140478	20.00	ng	-0.01
86) Perylene-d12	14.77	264	105740	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	4.90	112	291312	83.94	ng	0.01
7) Phenol-d6	6.02	99	367232	79.94	ng	-0.01
23) Nitrobenzene-d5	6.94	82	257422	59.19	ng	-0.01
41) 2,4,6-Tribromophenol	10.17	330	79877	94.26	ng	-0.01
44) 2-Fluorobiphenyl	8.73	172	409890	55.19	ng	0.00
78) Terphenyl-d14	12.43	244	336694	55.79	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propylamine	6.94	70	33578	10.74	ng	# 60
49) Dimethylphthalate	9.13	163	89420	12.09	ng	# 97
56) 2,4-Dinitrotoluene	9.38	165	12017	5.62	ng	# 31
66) 4-Bromophenyl-phenylether	10.17	248	5634	3.07	ng	# 1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF090415\
Data File : BF081468.D
Acq On : 5 Sep 2015 16:50
Operator : UM/IZ
Sample : G3559-02
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MGP226BR-40-42

Quant Time: Sep 07 02:51:01 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF090115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 07 02:47:26 2015
Response via : Initial Calibration

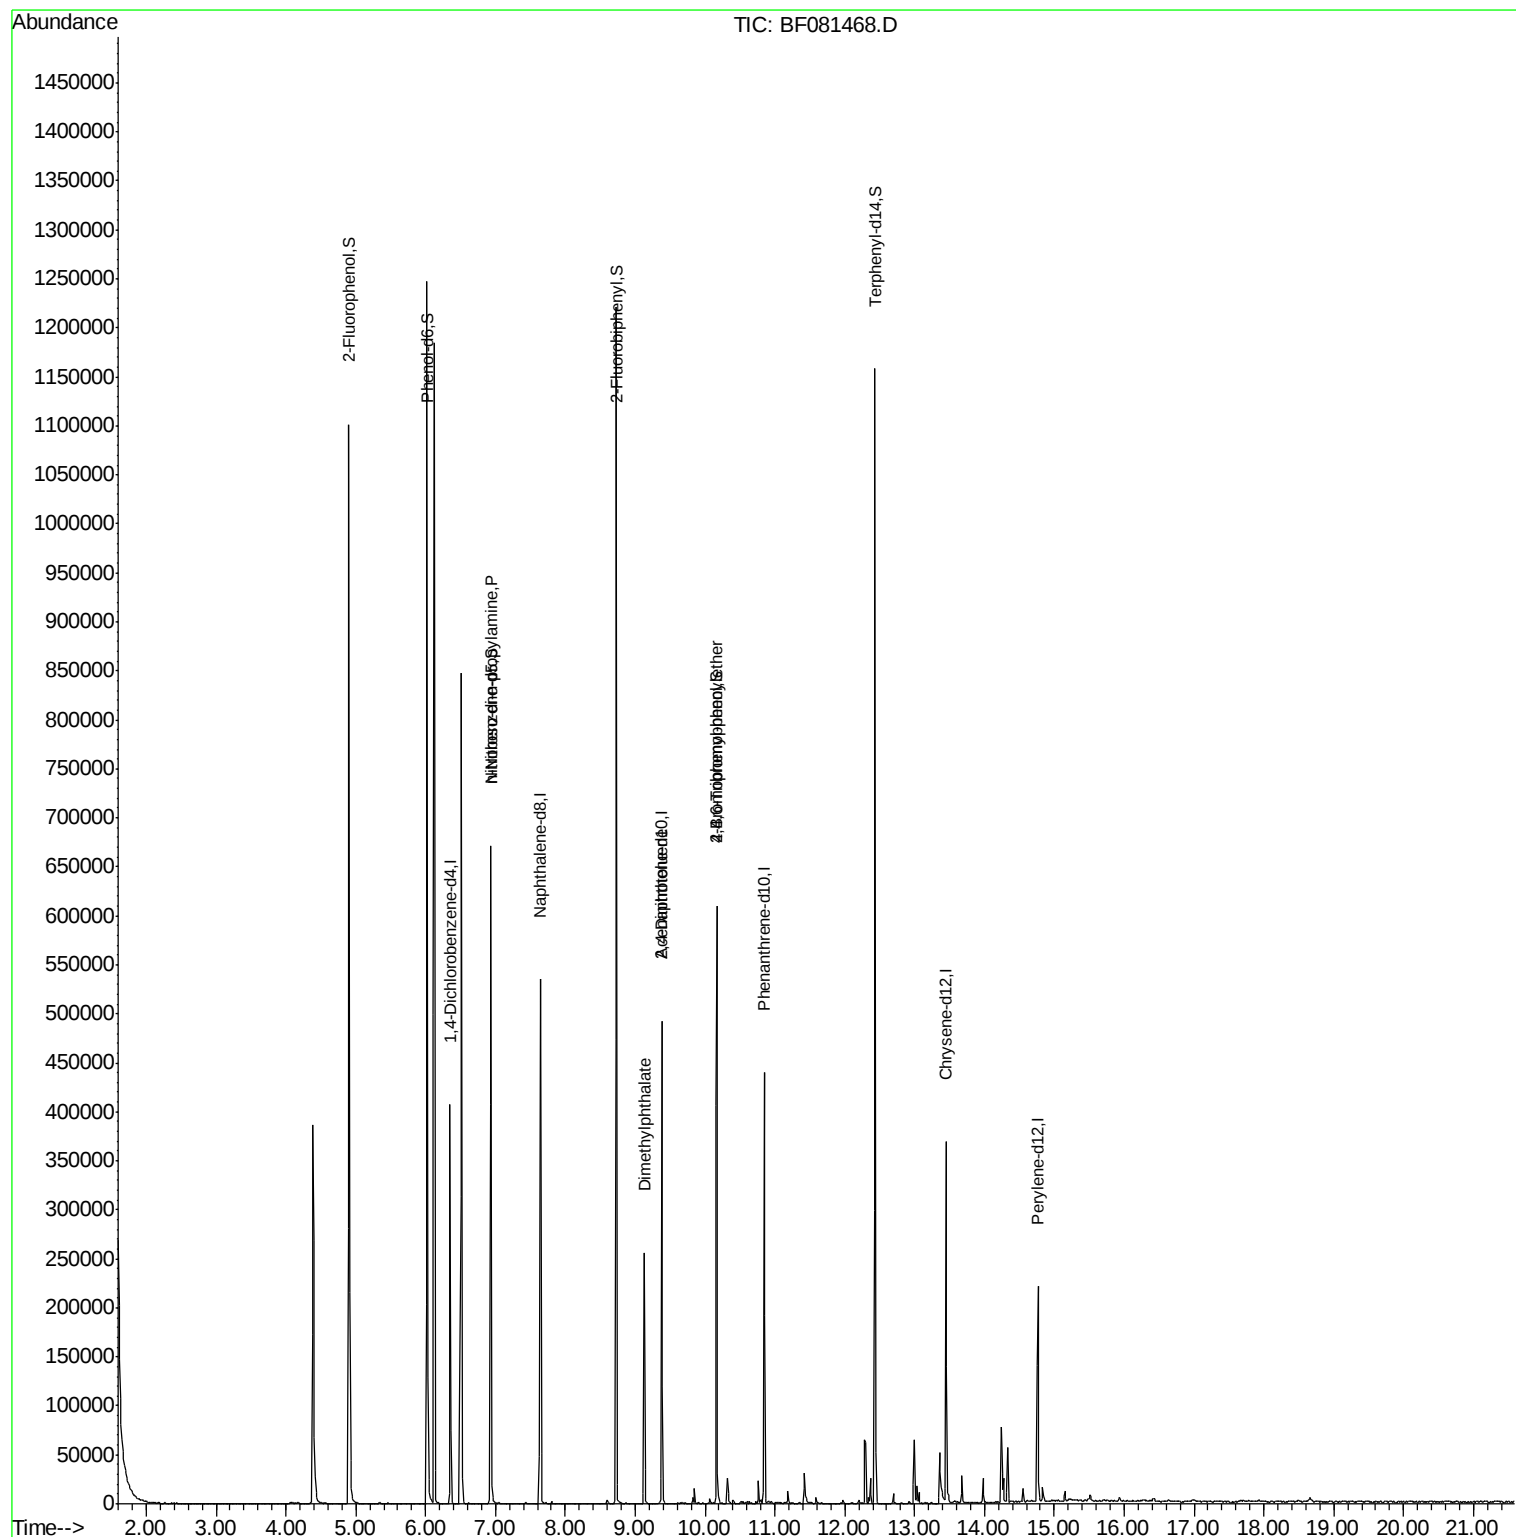



#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.35 min Scan# 417

Delta R.T. -0.01 min

Lab File: BF081468.D

Acq: 5 Sep 2015 16:50

Instrument :

BNA_F

ClientSampleId :

MGP226BR-40-42


Tot Ion:152 Resp: 53846

Ion Ratio Lower Upper

152 100

150 157.9 124.7 187.1




115 68.2 39.0 58.4#



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

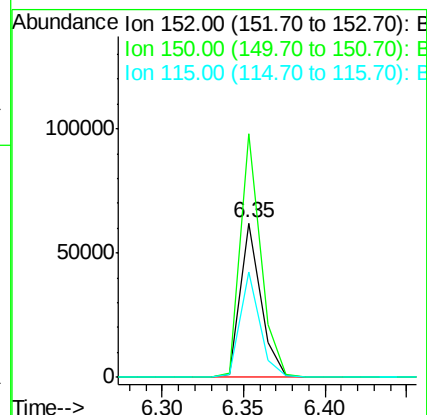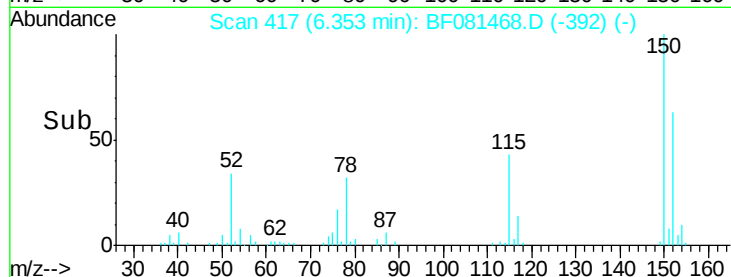

#5

2-Fluorophenol

Concen: 83.94 ng

RT: 4.90 min Scan# 290

Delta R.T. 0.01 min

Lab File: BF081468.D

Acq: 5 Sep 2015 16:50


Tgt Ion:112 Resp: 291312

Ion Ratio Lower Upper

112 100

64 72.0 39.7 59.5#



63 38.8 17.4 26.0#




Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

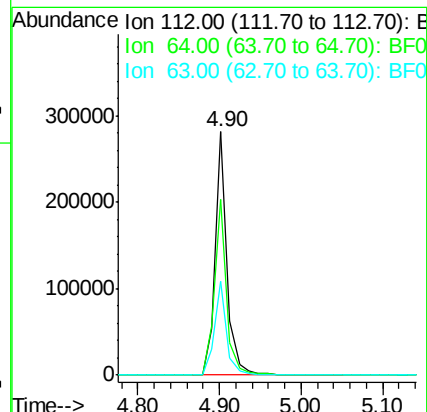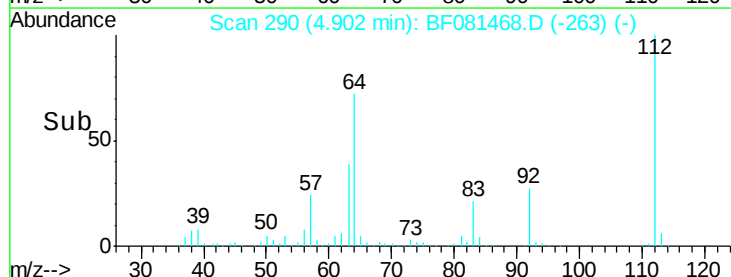

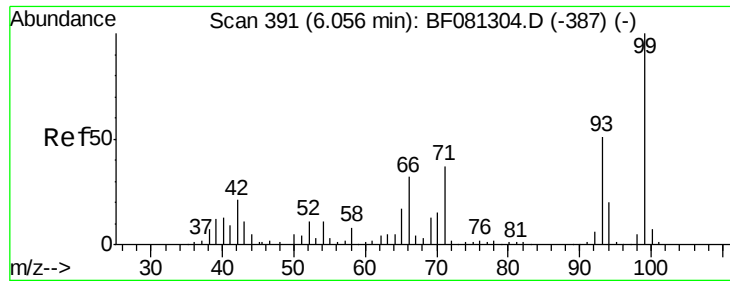

#7

Phenol-d6

Concen: 79.94 ng

RT: 6.02 min Scan# 388

Delta R.T. -0.01 min

Lab File: BF081468.D

Acq: 5 Sep 2015 16:50

Instrument :

BNA_F

ClientSampleId :

MGP226BR-40-42


Tot Ion: 99 Resp: 367232

Ion Ratio Lower Upper

99 100

42 23.0 13.7 20.5#




71 38.3 14.2 21.2#

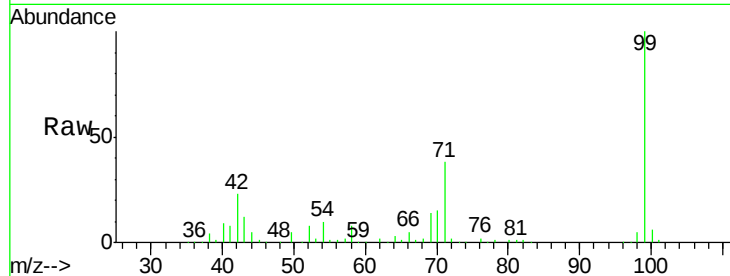

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

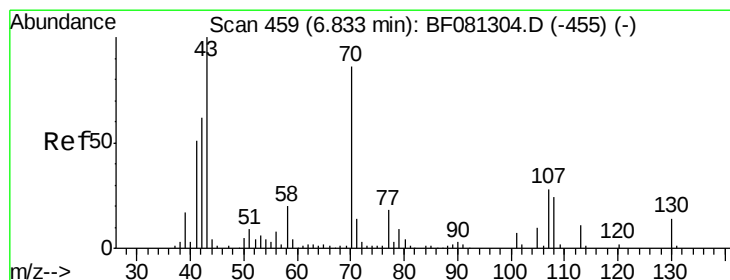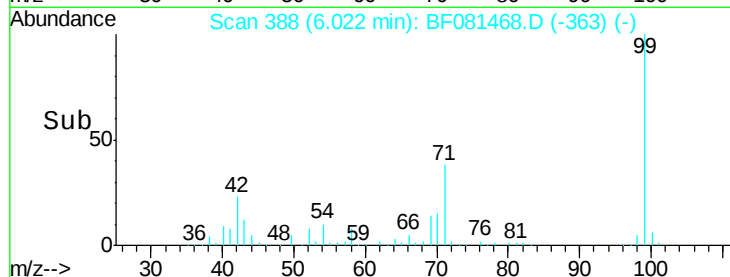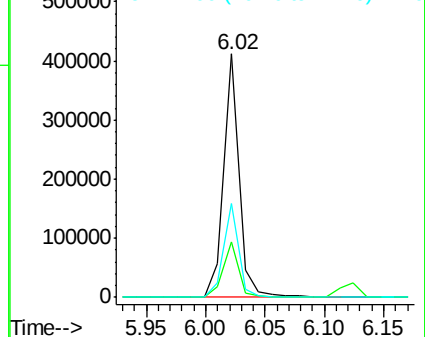

#19

n-Nitroso-di-n-propylamine

Concen: 10.74 ng

RT: 6.94 min Scan# 468

Delta R.T. 0.13 min

Lab File: BF081468.D

Acq: 5 Sep 2015 16:50

Tgt Ion: 70 Resp: 33578


Ion Ratio Lower Upper

70 100

42 49.5 63.8 95.6#

101 0.0 9.2 13.8#

130 2.2 27.3 40.9#


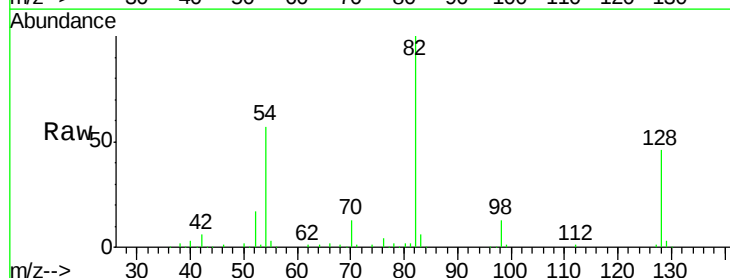



Abundance Ion 70.00 (69.70 to 70.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 101.00 (100.70 to 101.70): BF0

Ion 130.00 (129.70 to 130.70): BF0

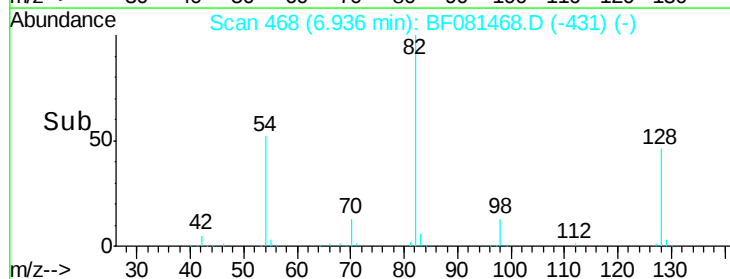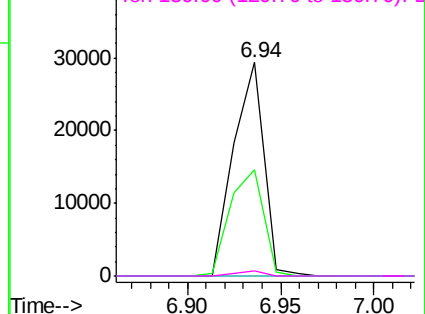

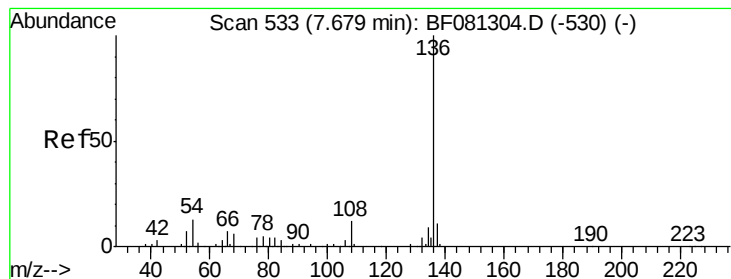

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.64 min Scan# 530

Delta R.T. -0.01 min

Lab File: BF081468.D

Acq: 5 Sep 2015 16:50

Instrument :

BNA_F

ClientSampleId :

MGP226BR-40-42

Tot Ion:136 Resp: 209844


Ion Ratio Lower Upper

136 100

137 11.2 9.0 13.6

54 11.4 8.2 12.2

68 5.0 5.8 8.6#






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

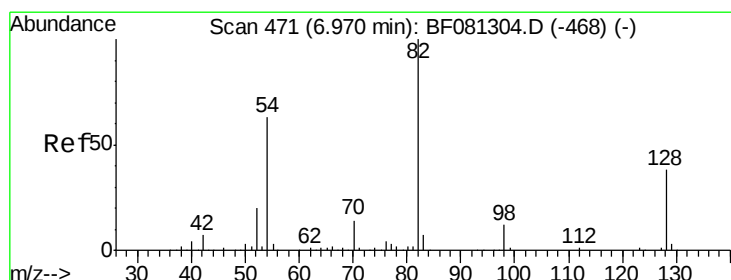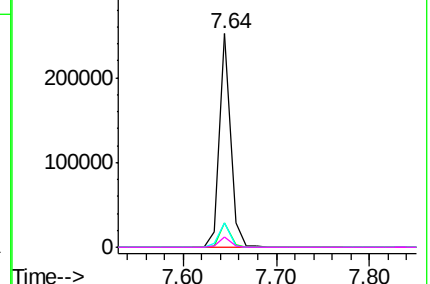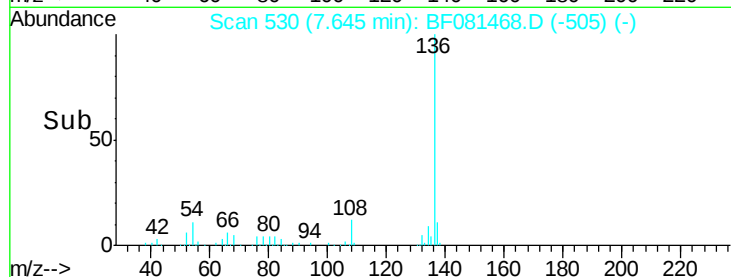

#23

Nitrobenzene-d5

Concen: 59.19 ng

RT: 6.94 min Scan# 468

Delta R.T. -0.01 min

Lab File: BF081468.D

Acq: 5 Sep 2015 16:50


Tgt Ion: 82 Resp: 257422

Ion Ratio Lower Upper

82 100

128 45.9 51.0 76.6#



54 57.1 47.5 71.3




Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF0

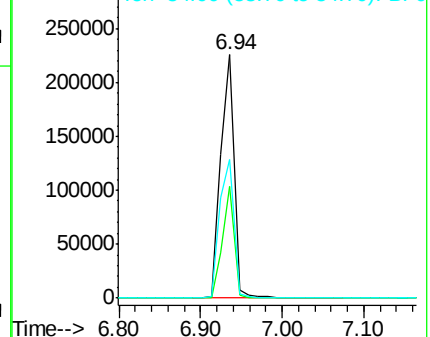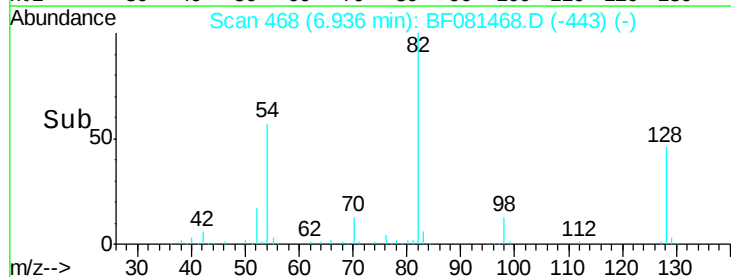


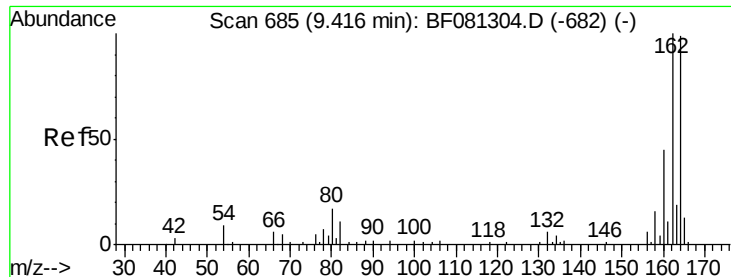




#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 9.38 min Scan# 682
Delta R.T. -0.01 min
Lab File: BF081468.D
Acq: 5 Sep 2015 16:50

Instrument :
BNA_F
ClientSampleId :
MGP226BR-40-42

Tot Ion:164 Resp: 95174
Ion Ratio Lower Upper
164 100
162 101.0 75.2 112.8
160 45.2 31.5 47.3

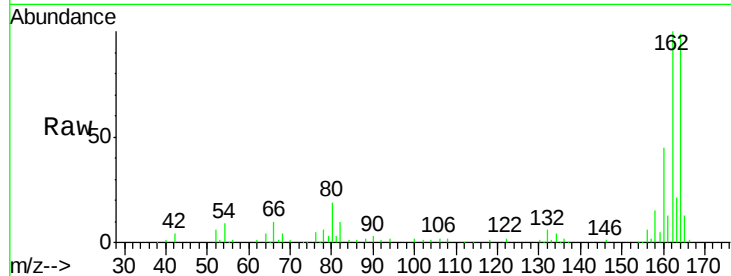


Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

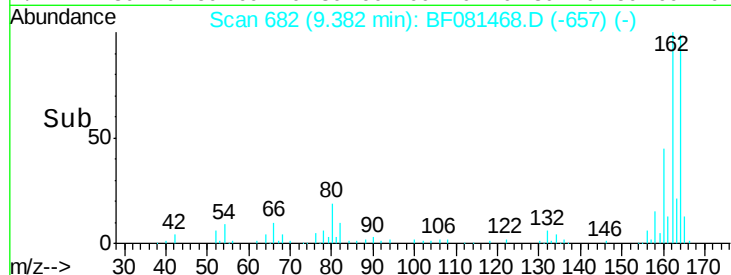
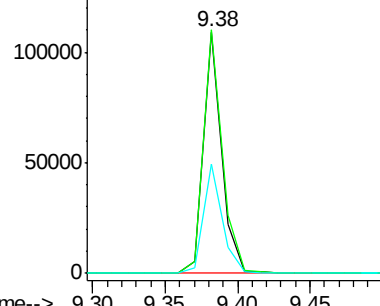


#41
2,4,6-Tribromophenol
Concen: 94.26 ng
RT: 10.17 min Scan# 751
Delta R.T. -0.01 min
Lab File: BF081468.D
Acq: 5 Sep 2015 16:50

Tgt Ion:330 Resp: 79877
Ion Ratio Lower Upper
330 100
332 94.3 76.6 114.8
141 44.3 29.7 44.5



Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

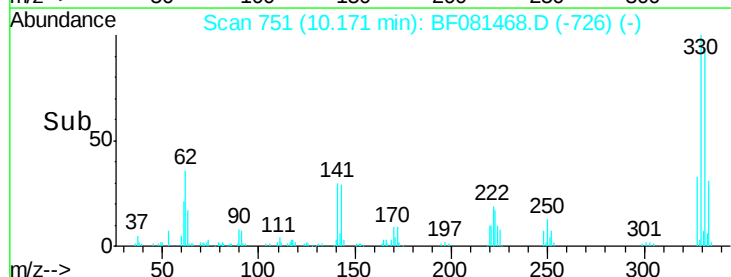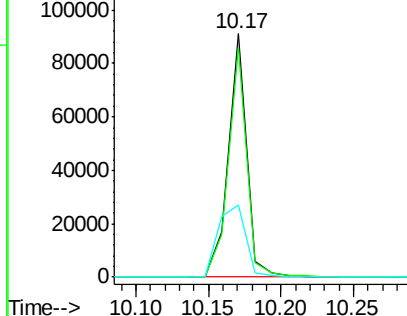







#44
2-Fluorobiphenyl
Concen: 55.19 ng
RT: 8.73 min Scan# 625
Delta R.T. 0.00 min
Lab File: BF081468.D
Acq: 5 Sep 2015 16:50

Instrument :
BNA_F
ClientSampleId :
MGP226BR-40-42

Tot Ion:172 Resp: 409890
Ion Ratio Lower Upper
172 100
171 34.8 26.1 39.1
170 23.3 17.4 26.2

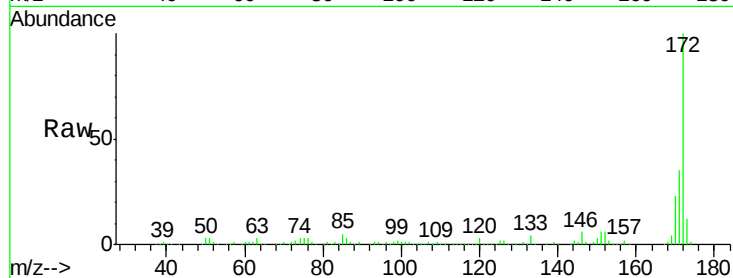


Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

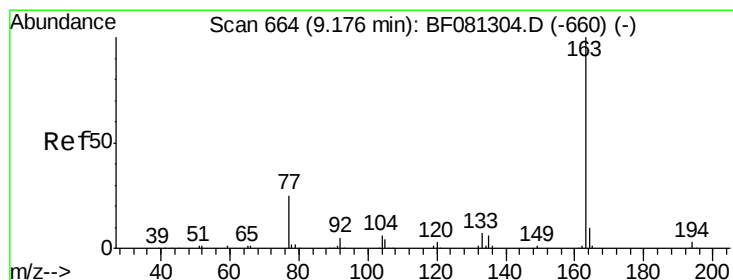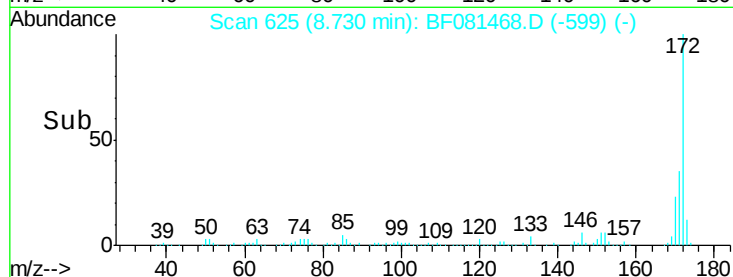
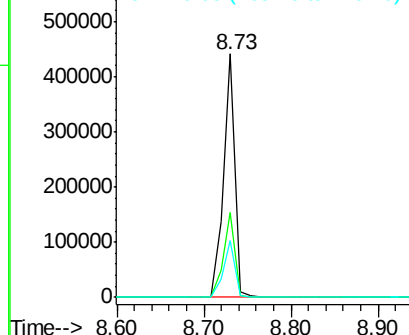


#49
Dimethylphthalate
Concen: 12.09 ng
RT: 9.13 min Scan# 660
Delta R.T. -0.02 min
Lab File: BF081468.D
Acq: 5 Sep 2015 16:50

Tgt Ion:163 Resp: 89420
Ion Ratio Lower Upper
163 100
194 3.3 4.4 6.6#
164 10.0 8.3 12.5

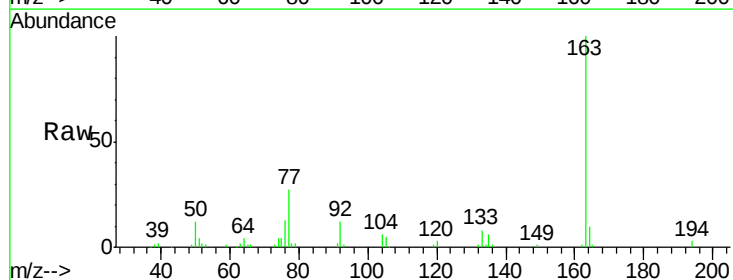

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

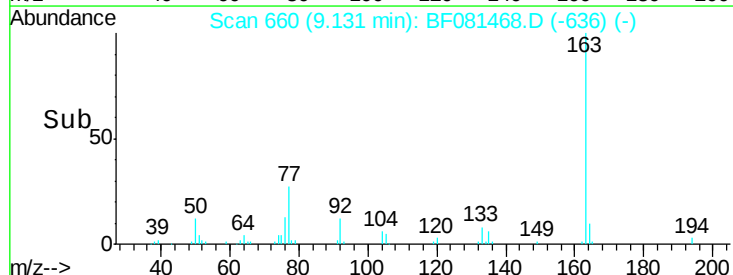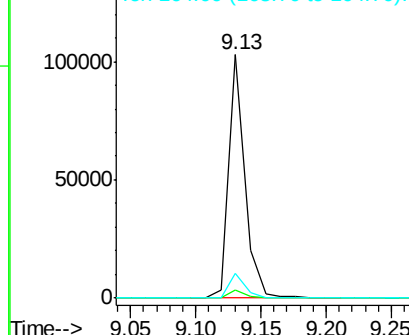




#56
 2,4-Dinitrotoluene
 Concen: 5.62 ng
 RT: 9.38 min Scan# 682
 Delta R.T. -0.22 min
 Lab File: BF081468.D
 Acq: 5 Sep 2015 16:50

Instrument :
 BNA_F
 ClientSampleId :
 MGP226BR-40-42

Tot Ion:165	Resp:	12017
Ion Ratio	Lower	Upper
165	100	
63	0.0	29.8 44.6#
89	0.0	44.5 66.7#
182	0.0	3.0 4.4#






Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF0


Ion 89.00 (88.70 to 89.70): BF0

Ion 182.00 (181.70 to 182.70): E

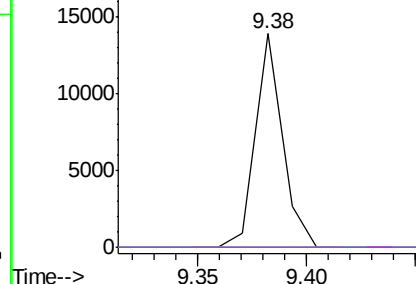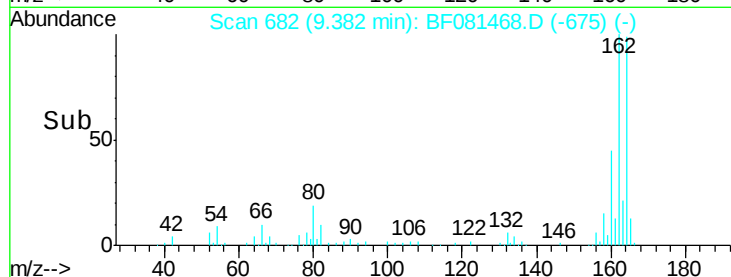

#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 10.85 min Scan# 810
 Delta R.T. -0.01 min
 Lab File: BF081468.D
 Acq: 5 Sep 2015 16:50



Tgt Ion:188	Resp:	181767
Ion Ratio	Lower	Upper
188	100	
94	10.3	11.1 16.7#
80	11.4	11.0 16.4




Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

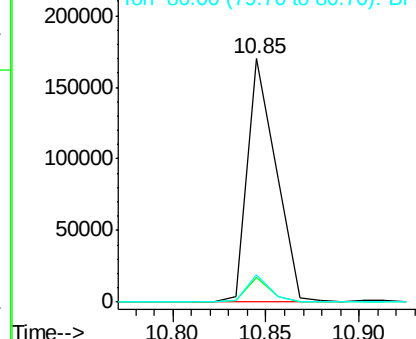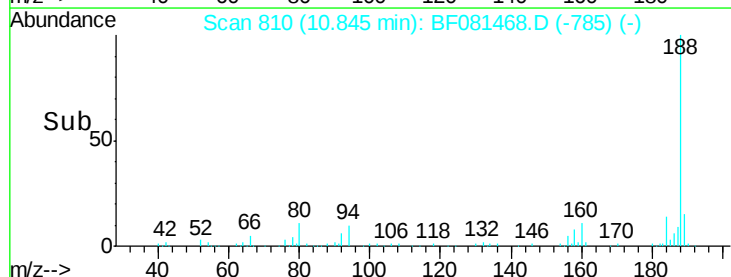


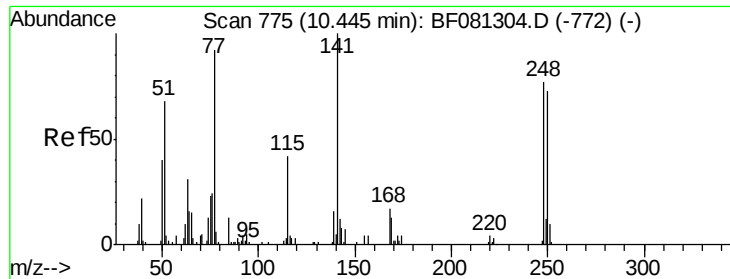




#66
 4-Bromophenyl-phenylether
 Concen: 3.07 ng
 RT: 10.17 min Scan# 751
 Delta R.T. -0.25 min
 Lab File: BF081468.D
 Acq: 5 Sep 2015 16:50

Instrument :
 BNA_F
 ClientSampleId :
 MGP226BR-40-42

Tot Ion:248 Resp: 5634
 Ion Ratio Lower Upper
 248 100
 250 198.5 78.5 117.7#
 141 448.3 59.0 88.6#

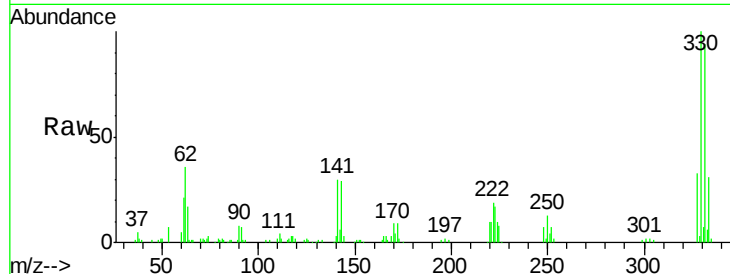


Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E

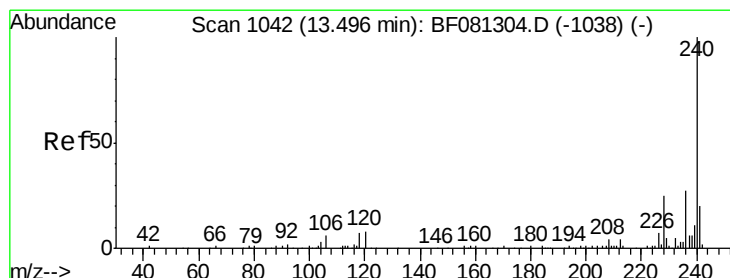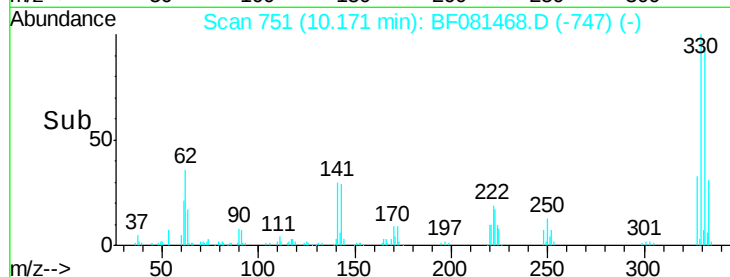
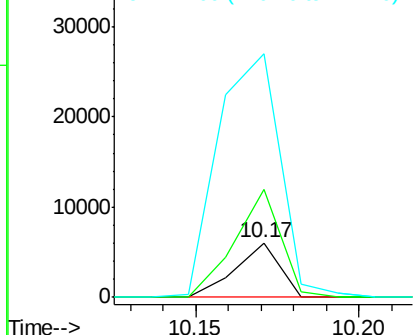


#75
 Chrysene-d12
 Concen: 20.00 ng
 RT: 13.45 min Scan# 1038
 Delta R.T. -0.01 min
 Lab File: BF081468.D
 Acq: 5 Sep 2015 16:50

Tgt Ion:240 Resp: 140478
 Ion Ratio Lower Upper
 240 100
 120 11.9 16.2 24.2#
 236 25.9 18.4 27.6

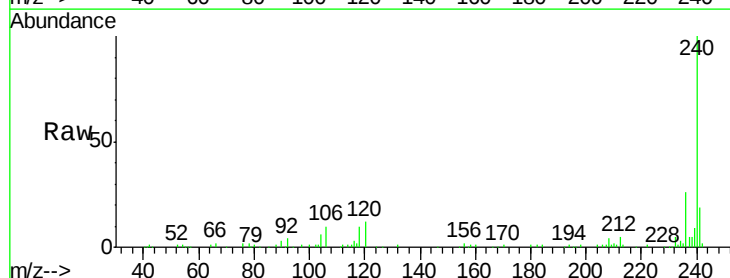

Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E



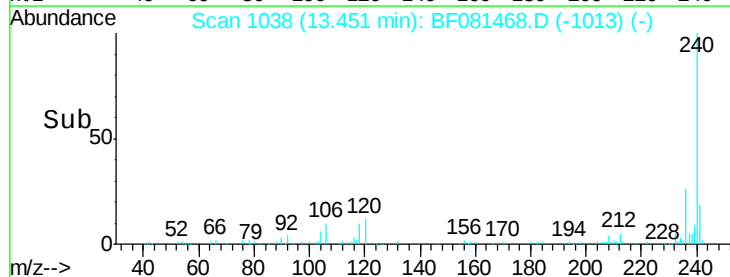
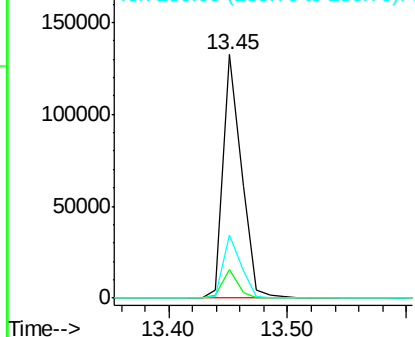




#78
 Terphenyl-d14
 Concen: 55.79 ng
 RT: 12.43 min Scan# 949
 Delta R.T. 0.00 min
 Lab File: BF081468.D
 Acq: 5 Sep 2015 16:50

Instrument :
 BNA_F
 ClientSampleId :
 MGP226BR-40-42

Tot Ion:244 Resp: 336694
 Ion Ratio Lower Upper
 244 100
 212 7.9 4.3 6.5#
 122 10.6 17.4 26.2#

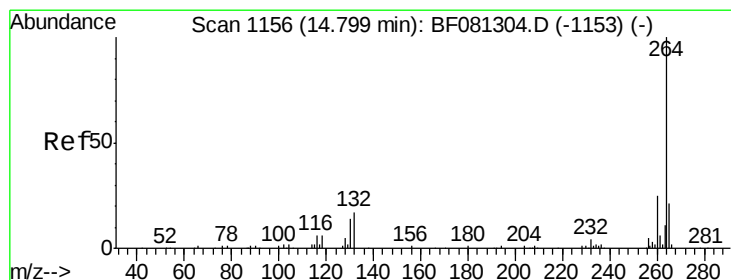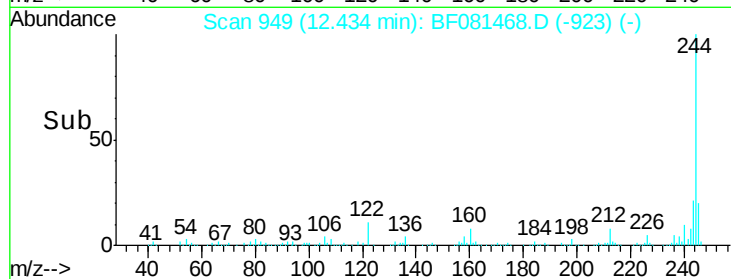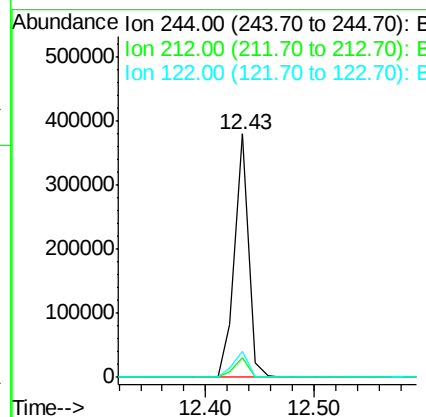

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 14.77 min Scan# 1153
 Delta R.T. 0.00 min
 Lab File: BF081468.D
 Acq: 5 Sep 2015 16:50

Tgt Ion:264 Resp: 105740
 Ion Ratio Lower Upper
 264 100
 260 23.0 16.7 25.1
 265 21.0 17.2 25.8

