
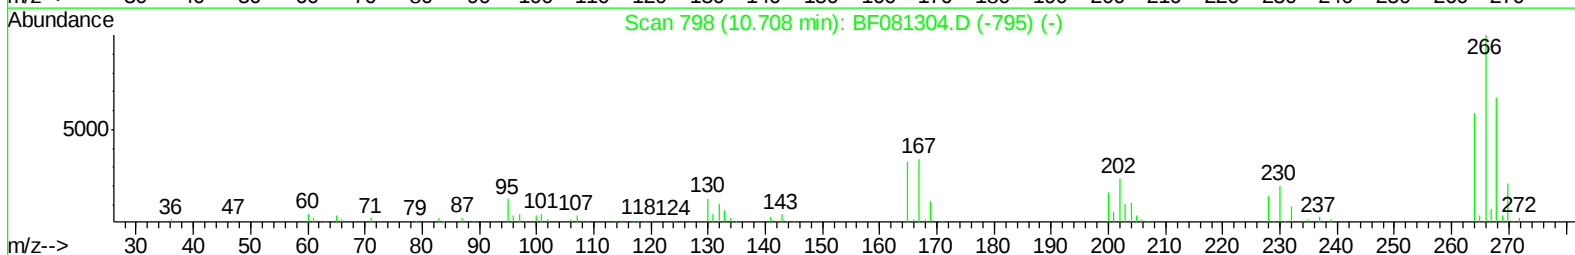
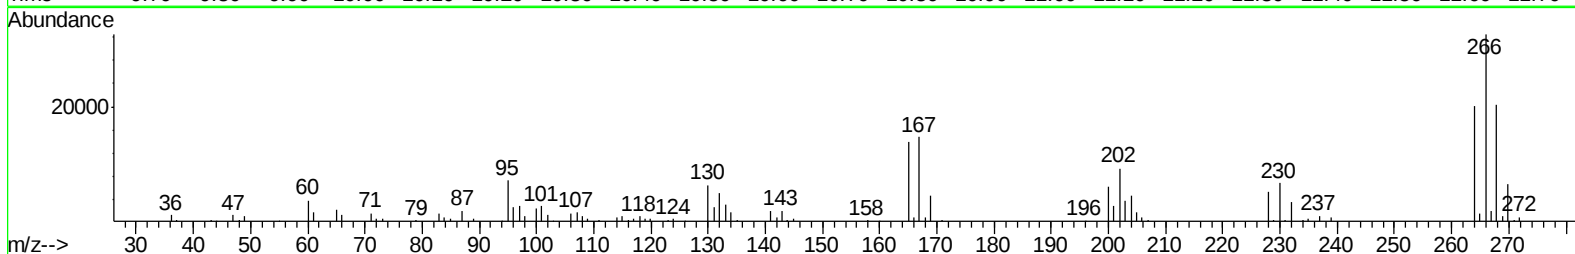


Data Path : Z:\HPCHEM1\BNA_F\Data\BF090415\
Data File : BF081418.D
Acq On : 4 Sep 2015 14:29
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 04 18:19:23 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF090115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 01 17:35:35 2015
Response via : Initial Calibration

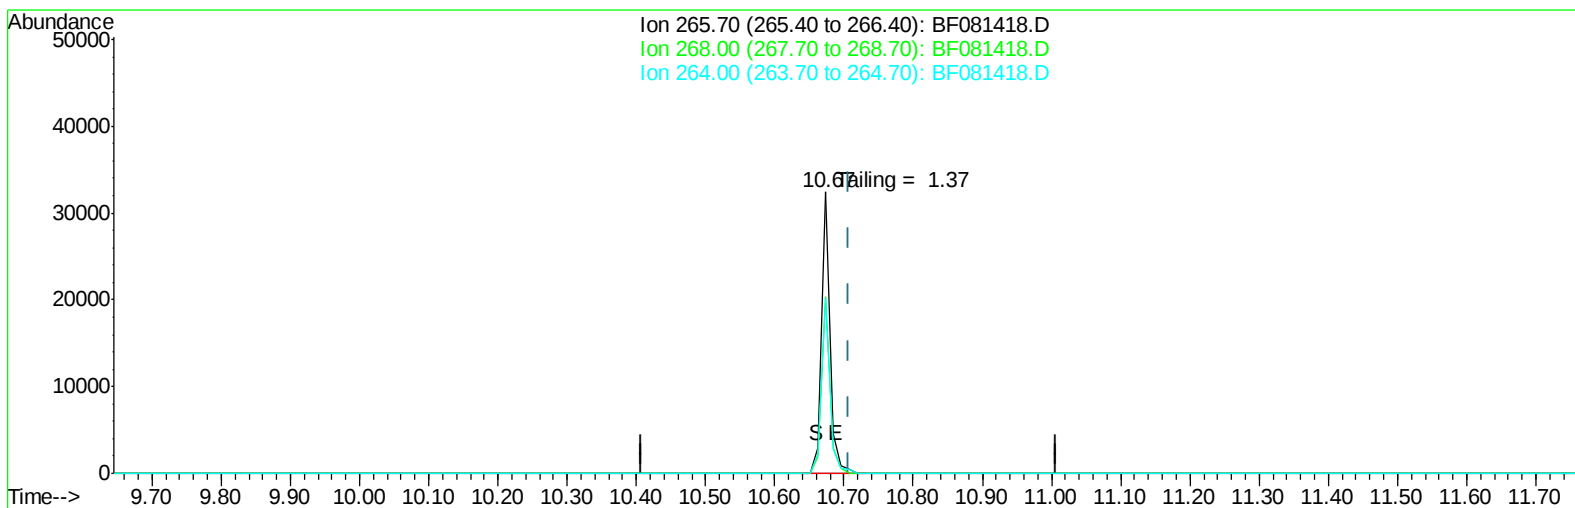

TIC: BF081418.D

(69) Pentachlorophenol (C)




10.673min (-0.034) 0.00ng

response 28306

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	62.61
264.00	62.70	62.07
0.00	0.00	0.00

```
Data Path : Z:\HPCHEM1\BNA_F\Data\BF090415\  
Data File : BF081418.D  
Acq On    : 4 Sep 2015 14:29  
Operator  : UM/IZ  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1 Sample Multiplier: 1
```

Quant Time: Sep 04 18:19:23 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF090115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 01 17:35:35 2015
Response via : Initial Calibration

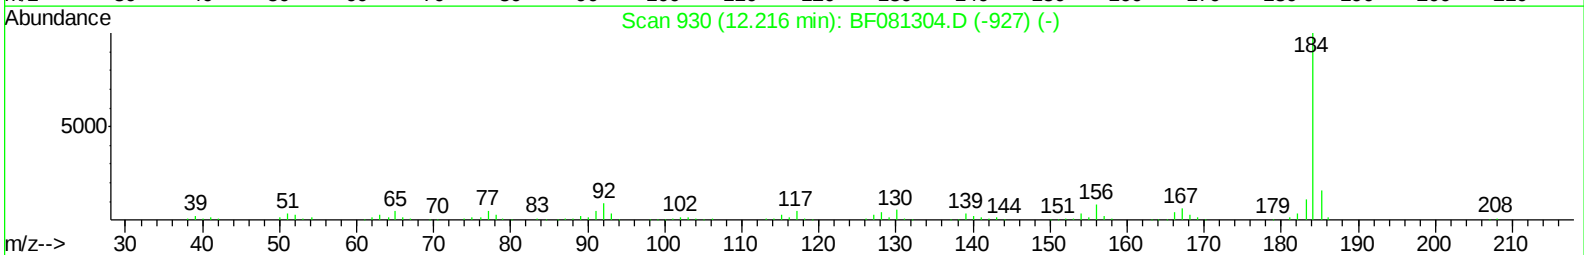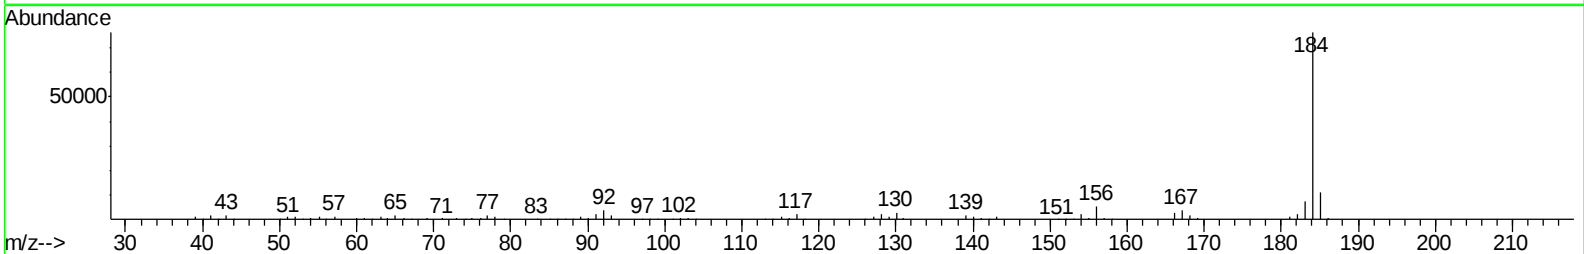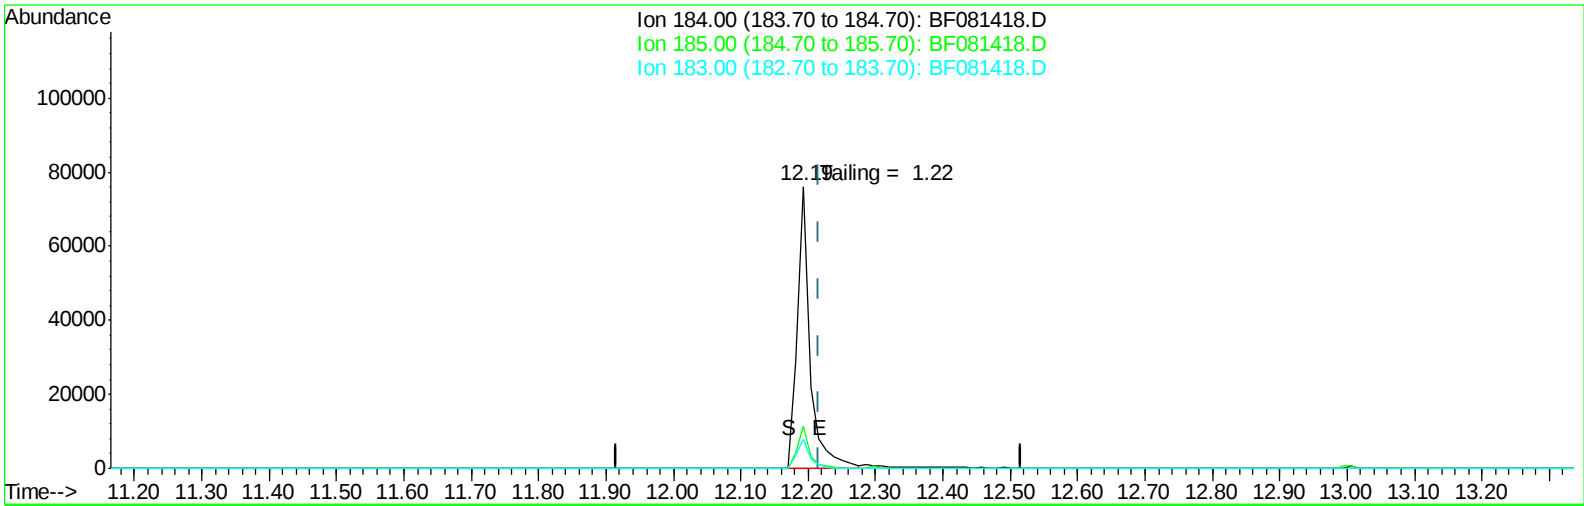

TIC: BF081418.D

(76) Benzidine

12.194min (-0.023) 1078.79ng

response 103135

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	14.90
183.00	9.50	10.30
0.00	0.00	0.00