
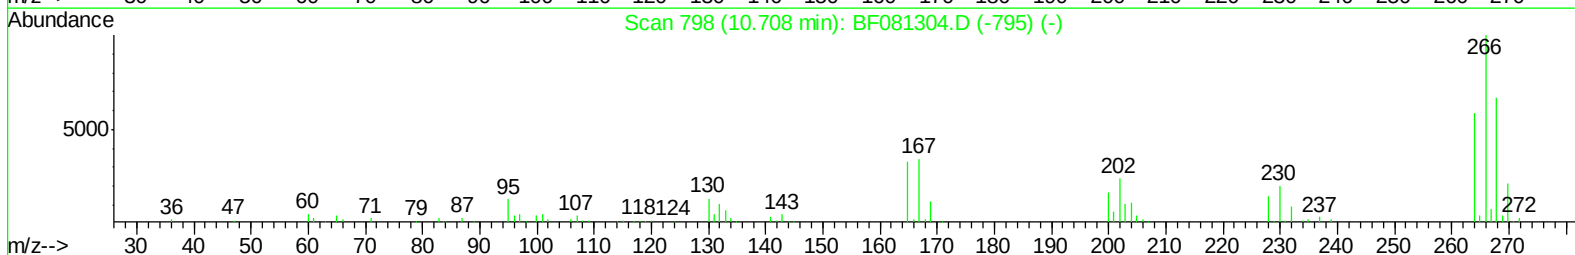
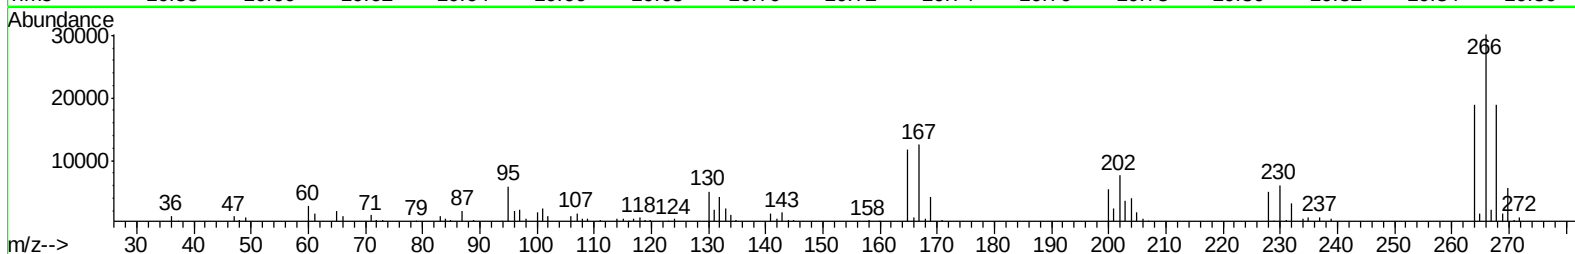


Data Path : Z:\HPCHEM1\BNA_F\Data\BF090415\
 Data File : BF081435.D
 Acq On : 4 Sep 2015 23:28
 Operator : UM/IZ
 Sample : DFTTP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 07 03:54:25 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF090115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 07 02:47:26 2015
 Response via : Initial Calibration

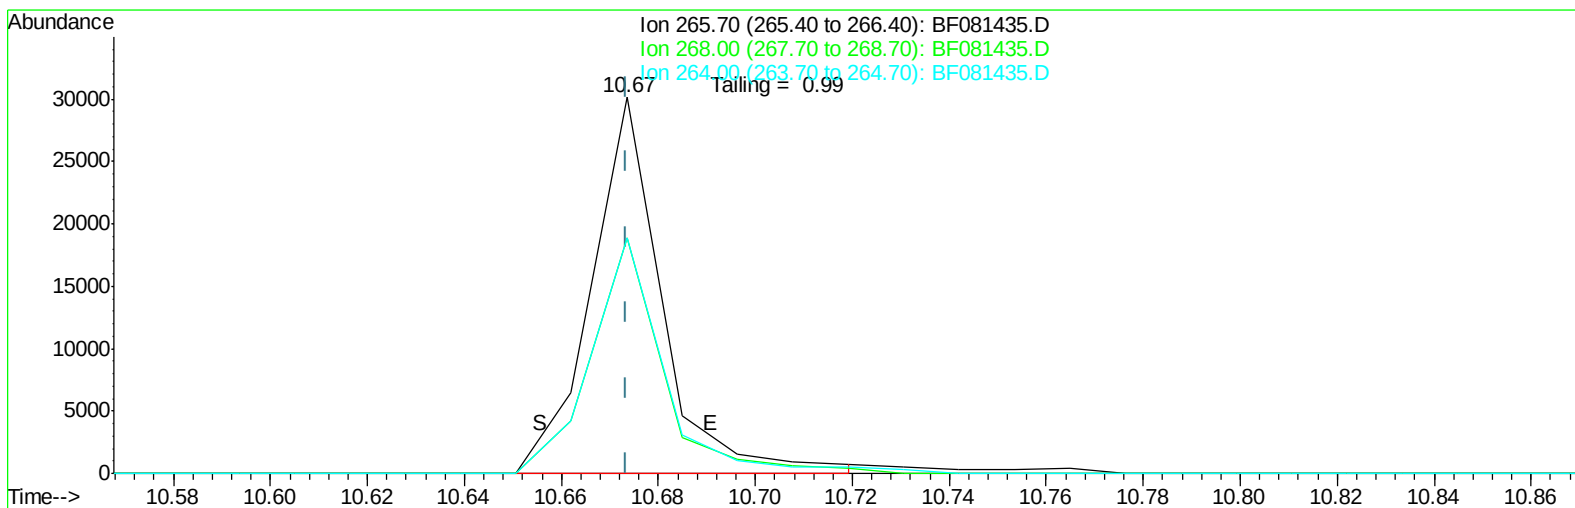

TIC: BF081435.D

(69) Pentachlorophenol (C)




10.673min (+0.000) 0.00ng

response 31506

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	62.62
264.00	62.70	62.67
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF090415\
Data File : BF081435.D
Acq On : 4 Sep 2015 23:28
Operator : UM/IZ
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 07 03:54:25 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF090115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 07 02:47:26 2015
Response via : Initial Calibration

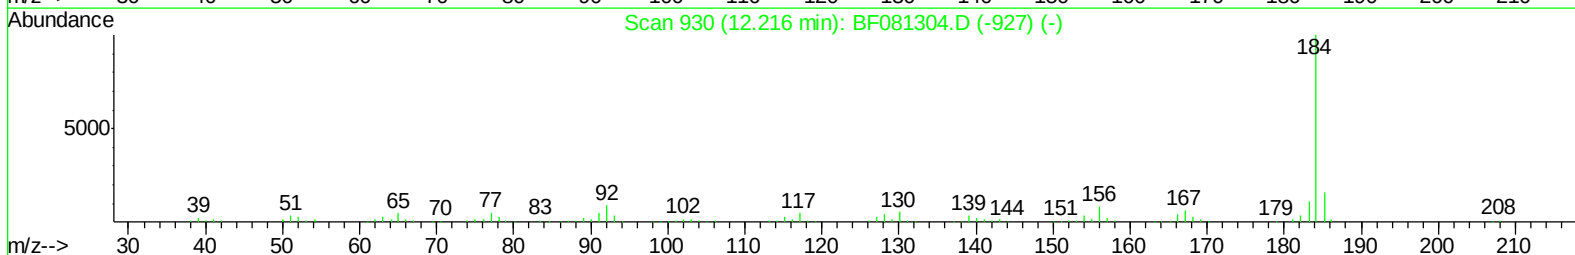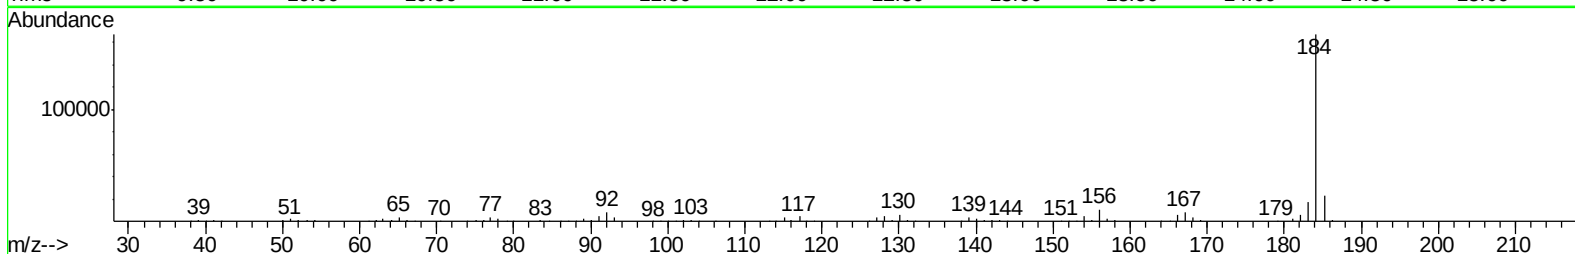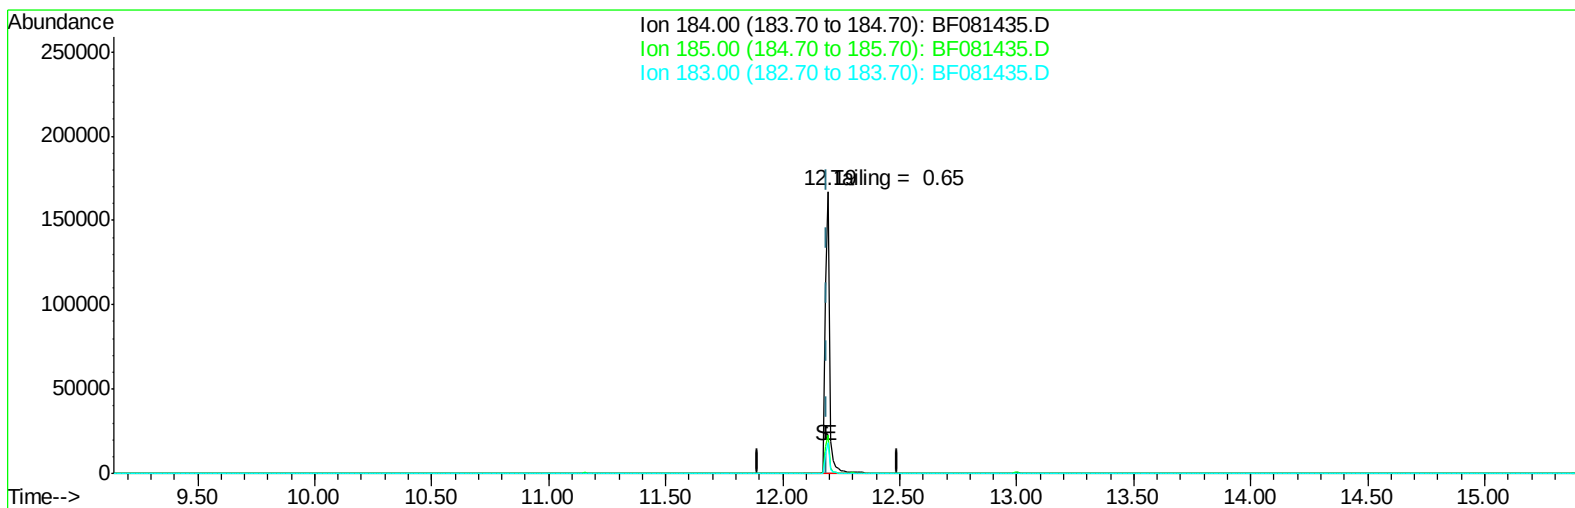

TIC: BF081435.D

(76) Benzidine

12.194min (+0.000) 20650.40ng m

response 215418

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	13.71
183.00	9.50	10.71
0.00	0.00	0.00