
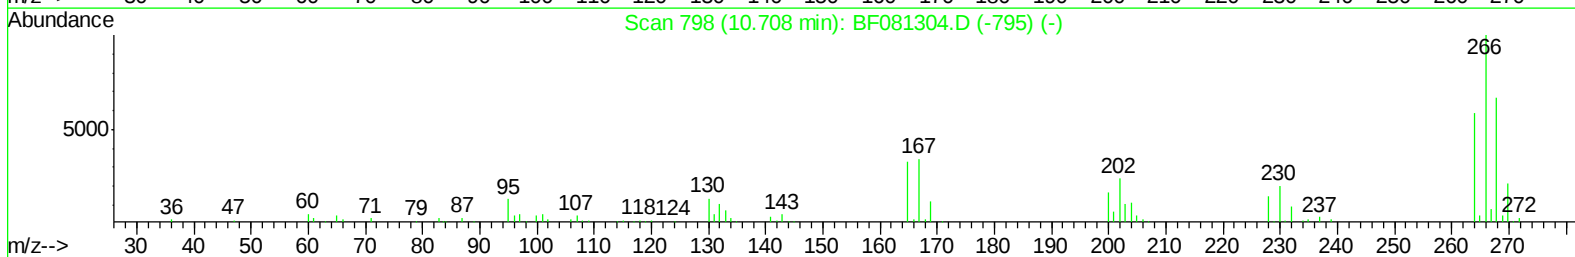
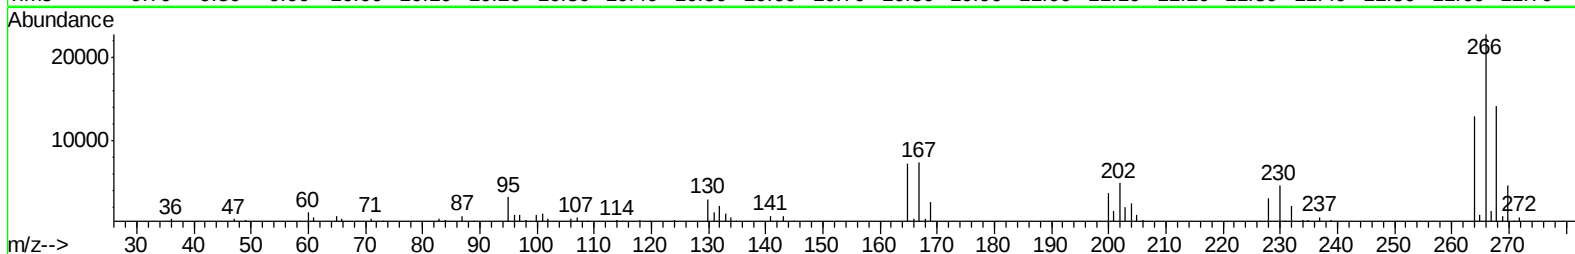


Data Path : Z:\HPCHEM1\BNA_F\Data\BF090415\
Data File : BF081455.D
Acq On : 5 Sep 2015 10:11
Operator : UM/IZ
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 08 15:38:17 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF090115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 01 17:35:35 2015
Response via : Initial Calibration

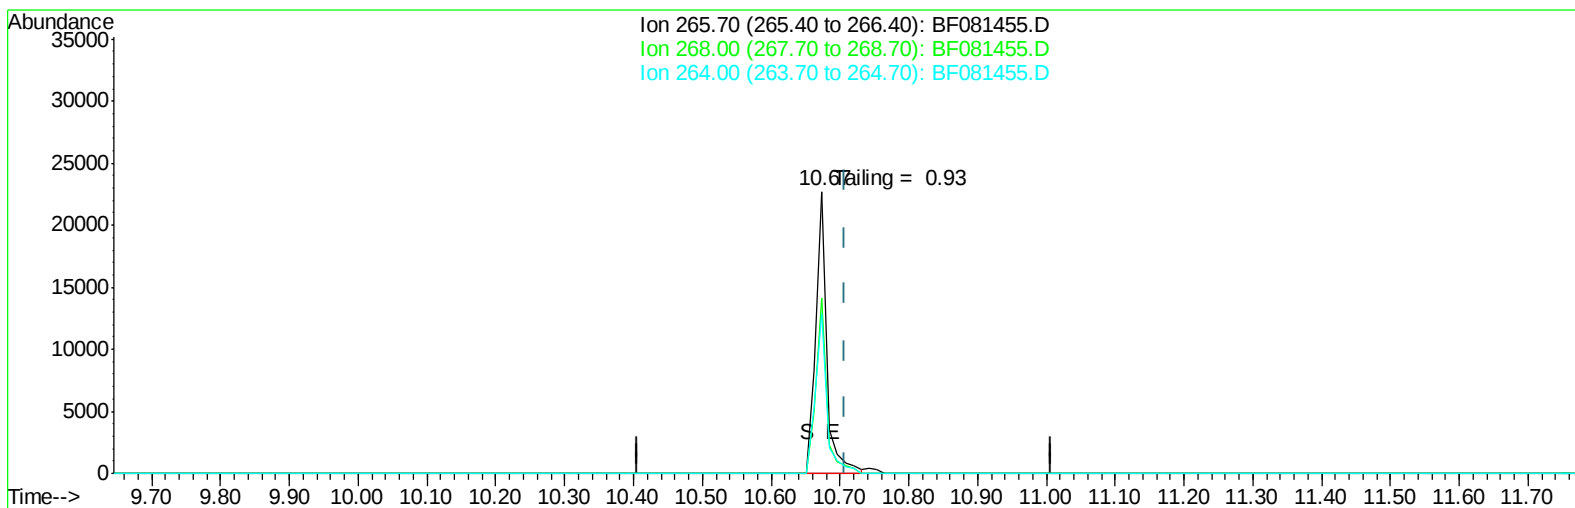

TIC: BF081455.D

(69) Pentachlorophenol (C)




10.674min (-0.033) 0.00ng

response 26309

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	62.29
264.00	62.70	56.86
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF090415\
 Data File : BF081455.D
 Acq On : 5 Sep 2015 10:11
 Operator : UM/IZ
 Sample : DFTTP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 08 15:38:17 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF090115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 01 17:35:35 2015
 Response via : Initial Calibration

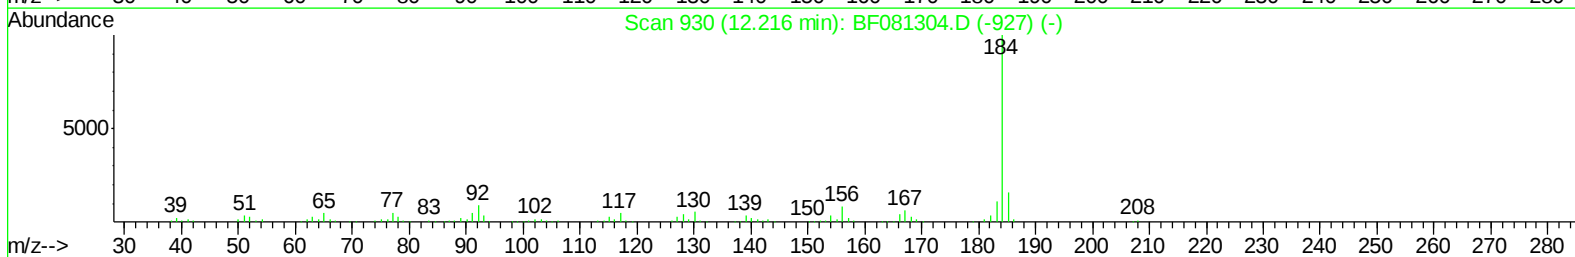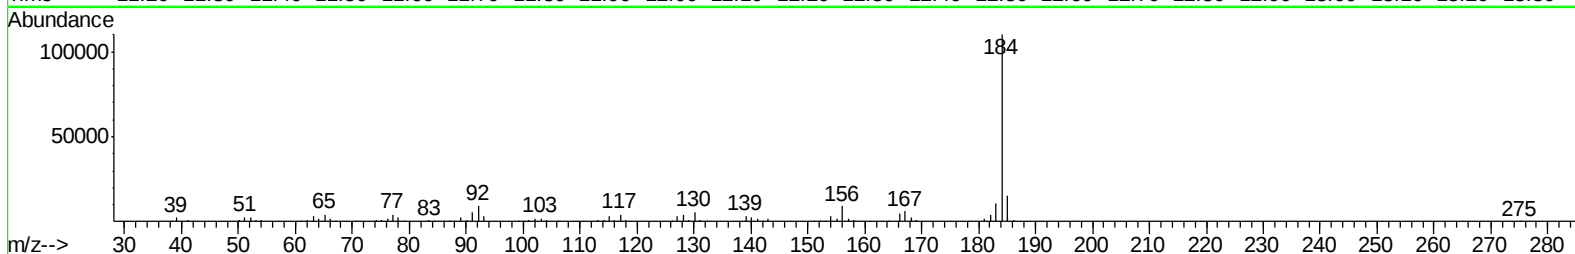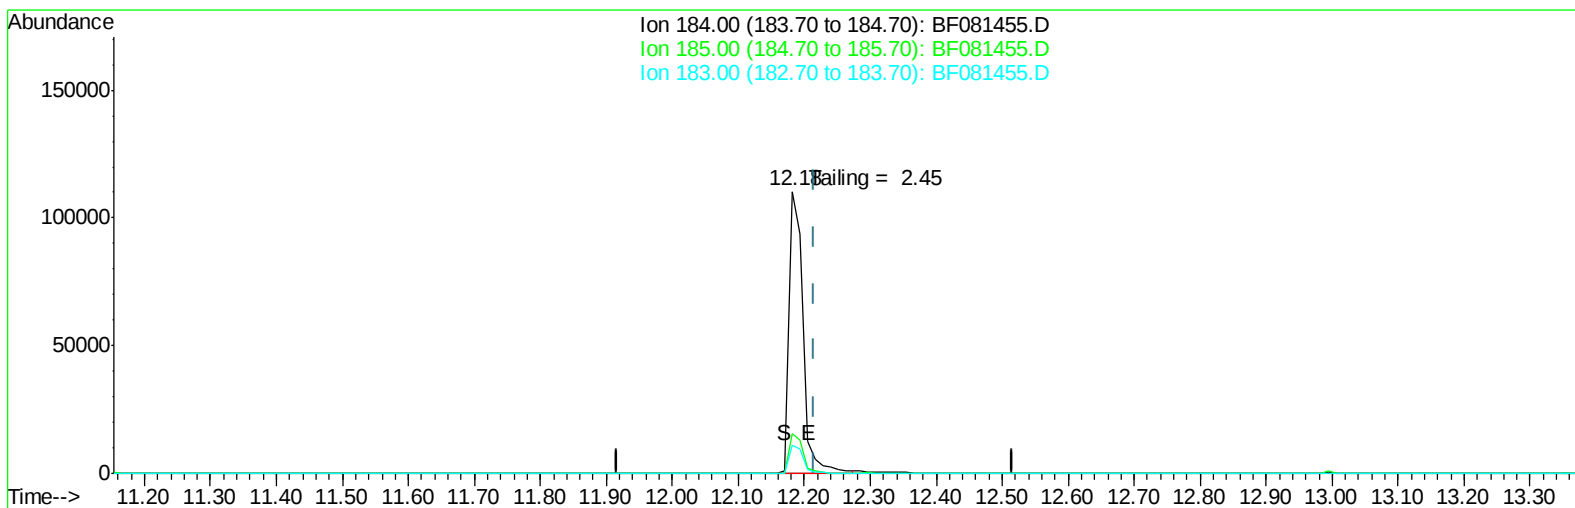

TIC: BF081455.D

(76) Benzidine

12.182min (-0.034) 15414.25ng

response 161458

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	13.93
183.00	9.50	10.00
0.00	0.00	0.00