


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF090415\
 Data File : BF081418.D
 Acq On : 4 Sep 2015 14:29
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampled :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF090115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 01 17:35:35 2015

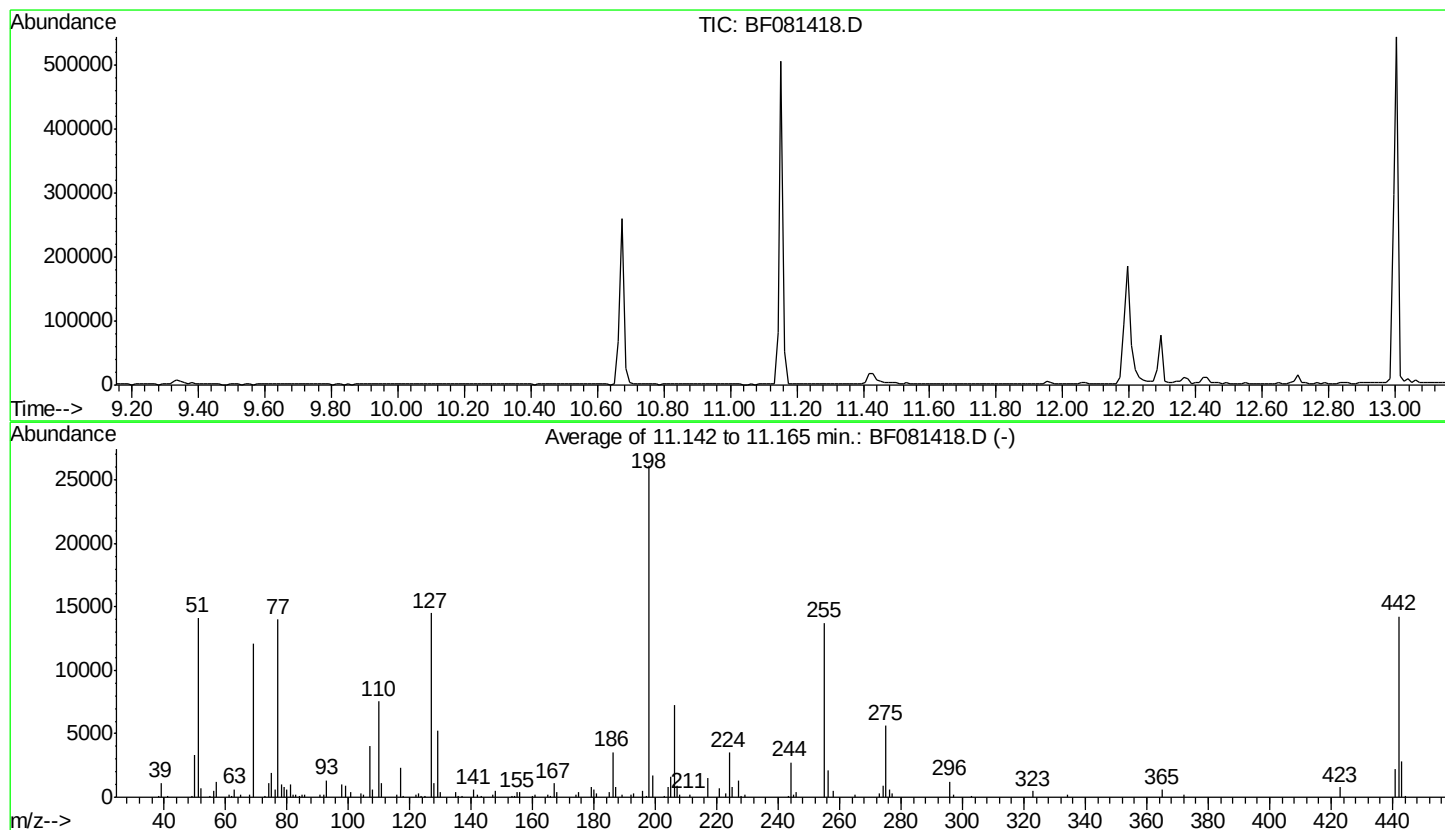

AutoFind: Scans 836, 837, 838; Background Corrected with Scan 833

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.1	14121	PASS
68	69	0.00	2	1.4	166	PASS
69	198	0.00	100	46.4	12123	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	55.6	14518	PASS
197	198	0.00	2	0.4	105	PASS
198	198	100	100	100.0	26123	PASS
199	198	5	9	6.5	1692	PASS
275	198	10	60	21.5	5624	PASS
365	198	1	100	2.3	593	PASS
441	442	0.01	24	15.8	2257	PASS
442	198	50	100	54.5	14240	PASS
443	442	15	24	19.9	2836	PASS