


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF090415\
 Data File : BF081455.D
 Acq On : 5 Sep 2015 10:11
 Operator : UM/IZ
 Sample : DFTTP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTTP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF090115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 01 17:35:35 2015

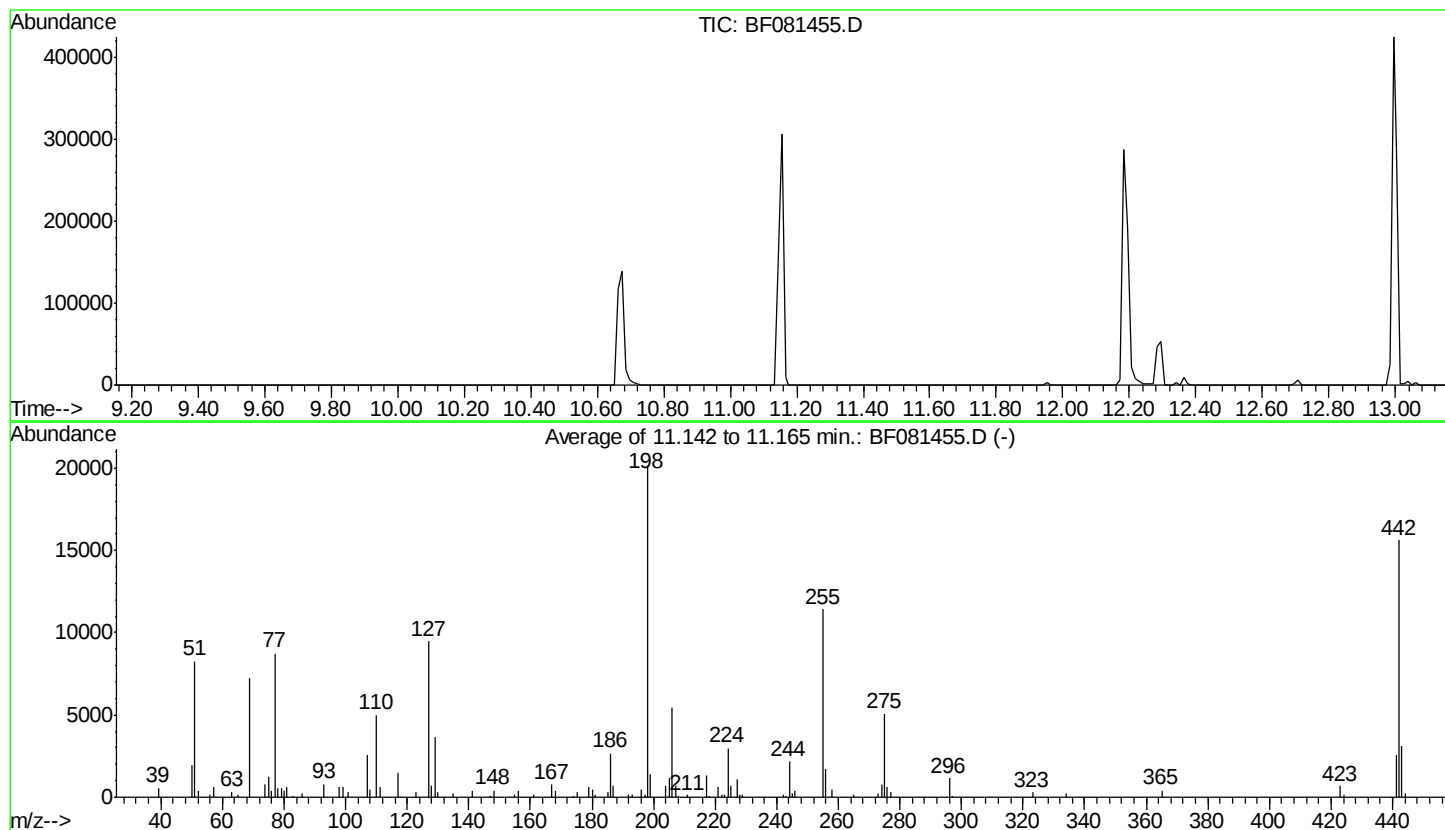

AutoFind: Scans 836, 837, 838; Background Corrected with Scan 833

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.0	8253	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	36.1	7266	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.0	9464	PASS
197	198	0.00	2	0.8	165	PASS
198	198	100	100	100.0	20152	PASS
199	198	5	9	6.8	1370	PASS
275	198	10	60	25.2	5071	PASS
365	198	1	100	2.0	411	PASS
441	442	0.01	24	16.3	2542	PASS
442	198	50	100	77.5	15627	PASS
443	442	15	24	19.8	3087	PASS