
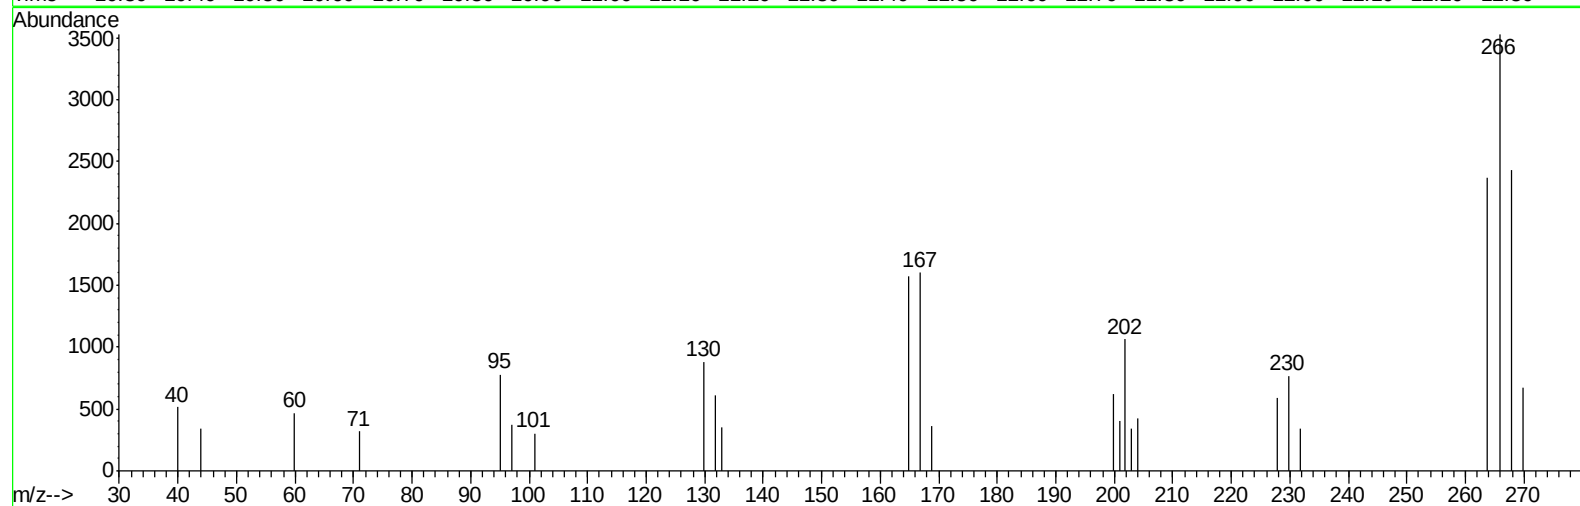


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF090418\
Data File : BF108759.D
Acq On : 5 Sep 2018 1:56
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 05 09:18:19 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 30 15:06:55 2018
Response via : Initial Calibration

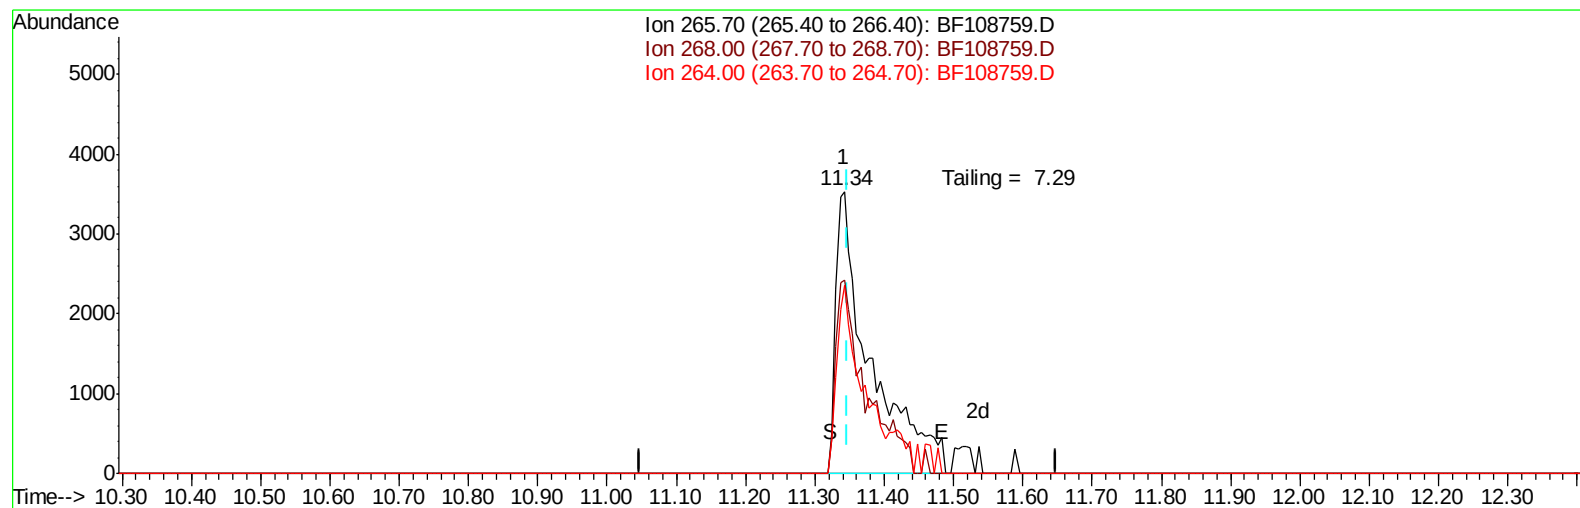

TIC: BF108759.D

(69) Pentachlorophenol (C)



11.342min (-0.006) 0.00ng

response 9317

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	68.82
264.00	61.90	67.04
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF090418\
Data File : BF108759.D
Acq On : 5 Sep 2018 1:56
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 05 09:18:19 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 30 15:06:55 2018
Response via : Initial Calibration

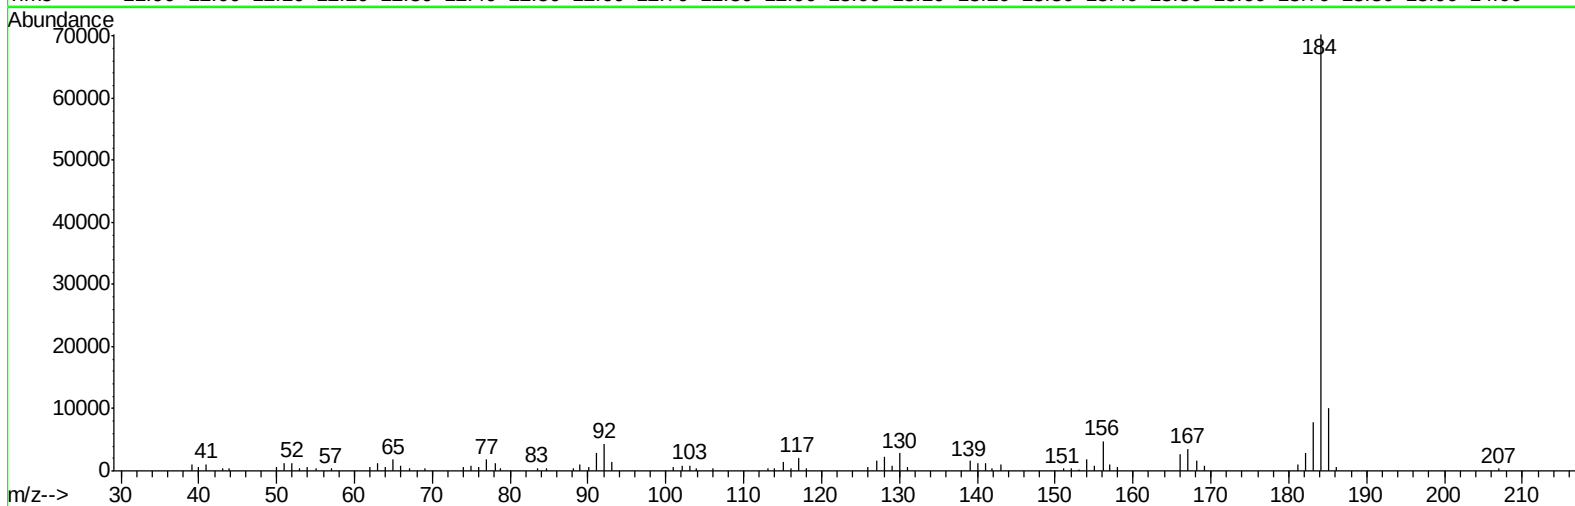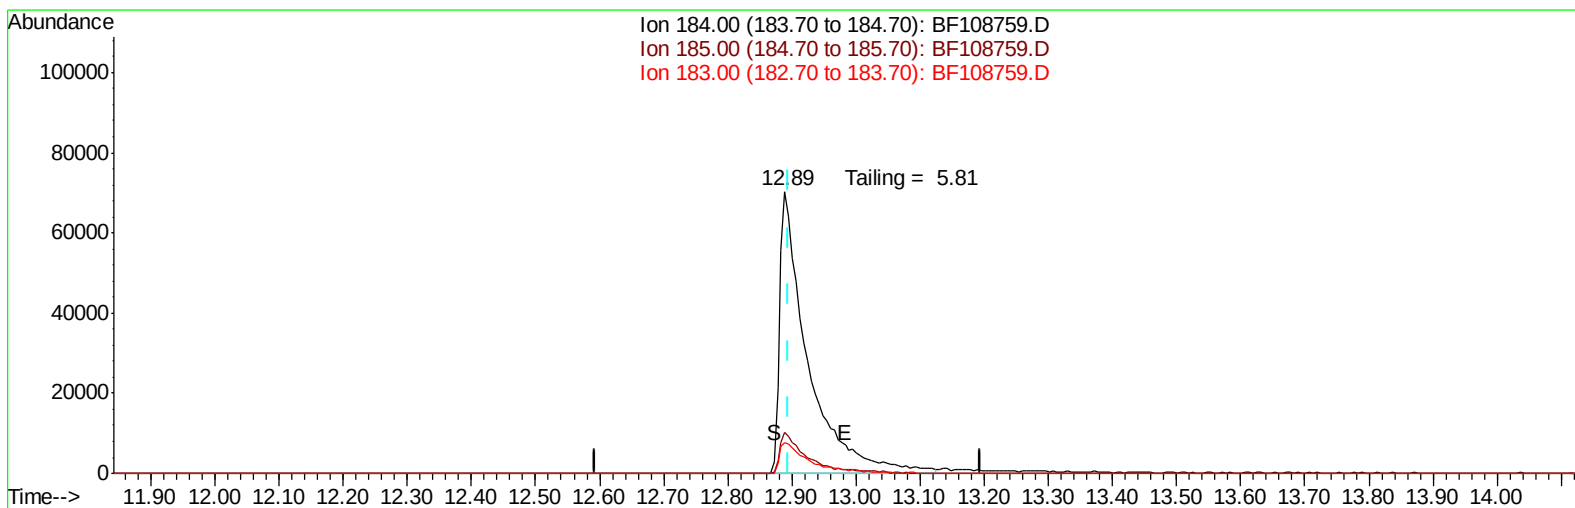

TIC: BF108759.D

(76) Benzidine

12.889min (-0.006) 0.00ng

response 215843

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.38
183.00	11.60	11.12
0.00	0.00	0.00