

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF090418\
 Data File : BF108743.D
 Acq On : 4 Sep 2018 16:19
 Operator : JU/SJ
 Sample : J4712-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-14

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF083018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.225	487	491	499	rBV	29621	41011	2.29%	0.318%
2	5.625	555	559	580	rBV	250097	739305	41.26%	5.730%
3	6.625	726	729	749	rBV	315480	969540	54.11%	7.514%
4	6.766	749	753	784	rVV	701345	1510085	84.27%	11.704%
5	6.995	788	792	814	rVV	177714	481043	26.85%	3.728%
6	7.142	814	817	848	rVB	663403	997560	55.67%	7.732%
7	7.560	884	888	922	rBV	213697	731051	40.80%	5.666%
8	8.272	1006	1009	1027	rBV	261021	464993	25.95%	3.604%
9	9.342	1187	1191	1214	rBV	1128244	1452191	81.04%	11.255%
10	9.736	1253	1258	1265	rBV	72432	82855	4.62%	0.642%
11	10.030	1304	1308	1330	rBV	468483	555150	30.98%	4.303%
12	10.830	1440	1444	1456	rBV	543556	866436	48.35%	6.715%
13	11.389	1536	1539	1544	rVB	23087	22612	1.26%	0.175%
14	11.530	1559	1563	1575	rBV	416830	697850	38.94%	5.409%
15	12.042	1646	1650	1651	rBV4	13372	19284	1.08%	0.149%
16	12.583	1739	1742	1744	rBV4	35865	36034	2.01%	0.279%
17	12.754	1768	1771	1777	rBV	130344	180521	10.07%	1.399%
18	12.960	1804	1806	1807	rBV	30065	22372	1.25%	0.173%
19	12.983	1808	1810	1816	rVB	81349	106677	5.95%	0.827%
20	13.112	1828	1832	1846	rBV	1552612	1791905	100.00%	13.888%
21	14.189	2011	2015	2025	rBV	463804	689383	38.47%	5.343%
22	15.748	2277	2280	2292	rVB	221105	444406	24.80%	3.444%


Sum of corrected areas: 12902264

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF090418\
Data File : BF108743.D
Acq On : 4 Sep 2018 16:19
Operator : JU/SJ
Sample : J4712-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-14

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

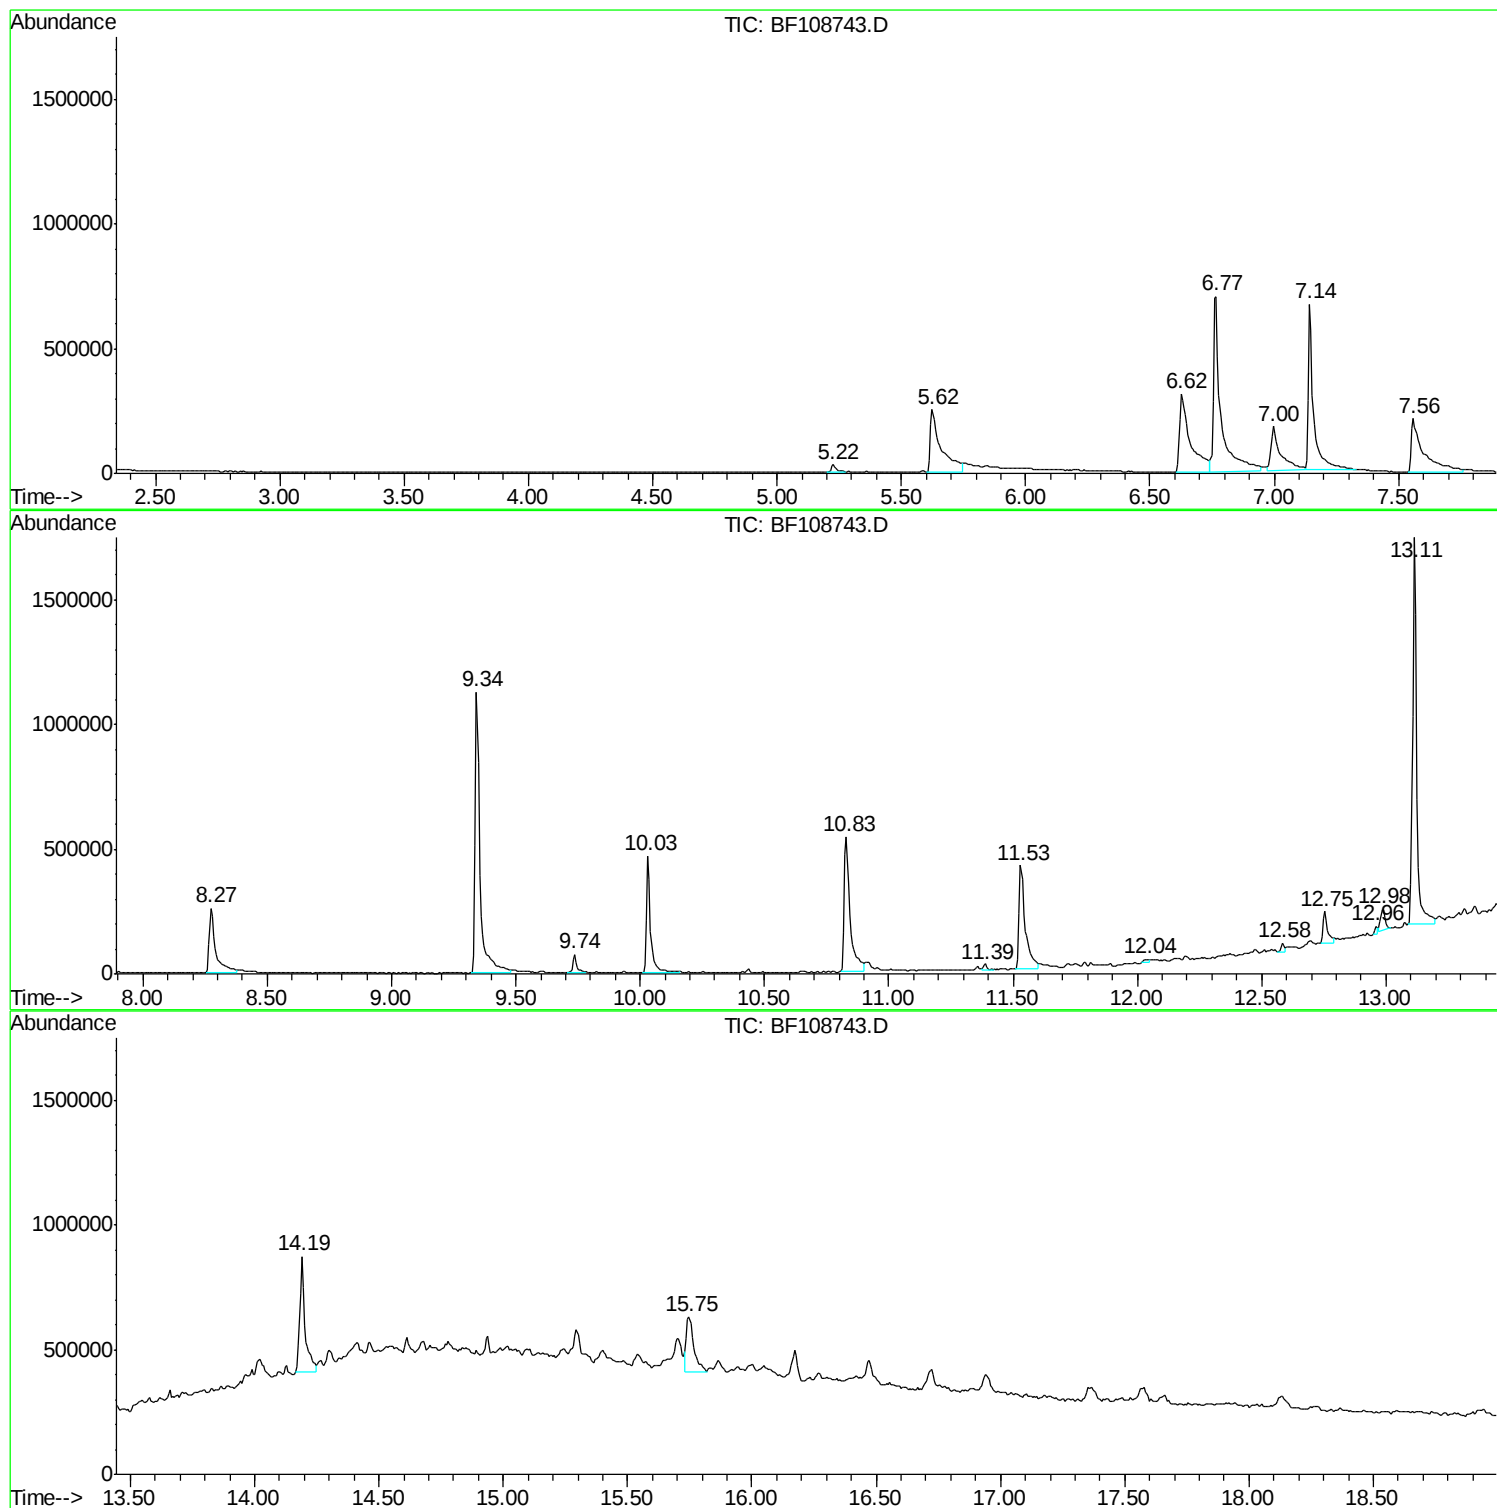

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF090418\
Data File : BF108743.D
Acq On : 4 Sep 2018 16:19
Operator : JU/SJ
Sample : J4712-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-14










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.77 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.77	62.78 ng	1510090	1,4-Dichlorobenzene-d4	7.00

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12
2		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10
3		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	9
4		1,3,5-Trifluorobenzene	132	C6H3F3	000372-38-3	9
5		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9

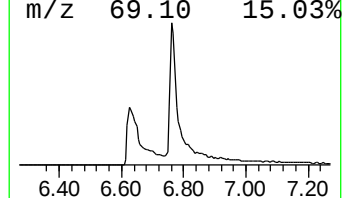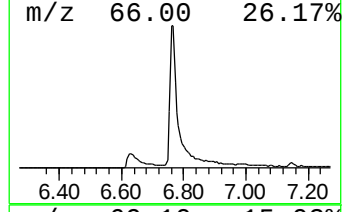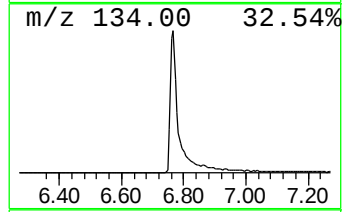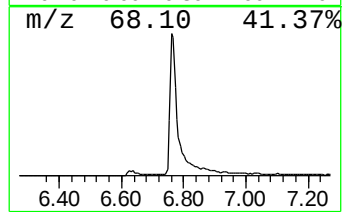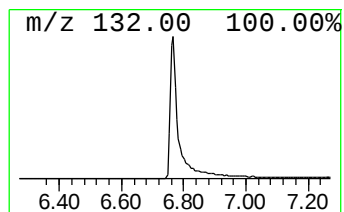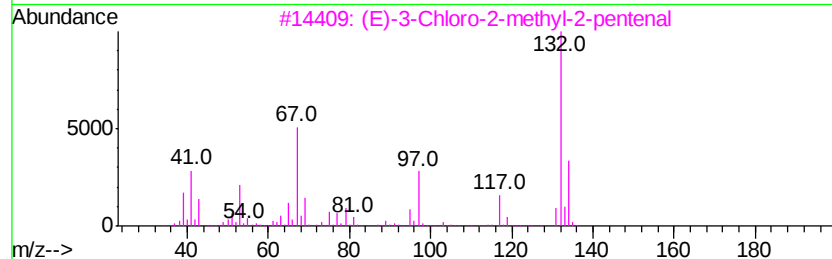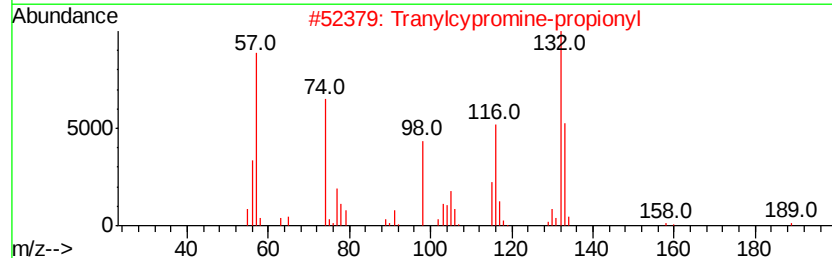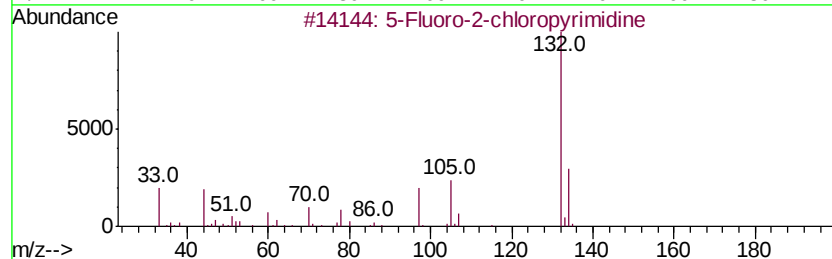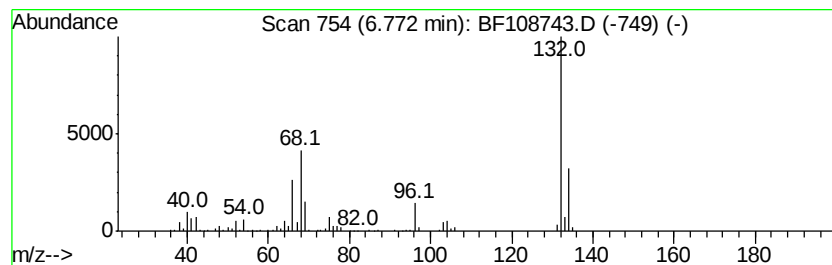

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF090418\
Data File : BF108743.D
Acq On : 4 Sep 2018 16:19
Operator : JU/SJ
Sample : J4712-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-14

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF083018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.77	6.77	62.8	ng	1510090	1	7.00	481043	20.0