

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF090418\
 Data File : BF108766.D
 Acq On : 5 Sep 2018 5:07
 Operator : JU/SJ
 Sample : J4741-03 10X
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 AOC2-03-C

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF083018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.995	789	792	806	rBV	75236	237933	36.51%	8.115%
2	7.154	815	819	828	rVB5	8288	18677	2.87%	0.637%
3	8.272	1006	1009	1033	rBV	214979	469200	72.00%	16.003%
4	9.348	1188	1192	1196	rBV2	4075	6793	1.04%	0.232%
5	10.031	1304	1308	1326	rBV	452342	562610	86.34%	19.189%
6	11.530	1559	1563	1592	rBV	359657	651624	100.00%	22.225%
7	12.754	1767	1771	1778	rBV	9105	16189	2.48%	0.552%
8	12.983	1803	1810	1818	rBV2	12579	23512	3.61%	0.802%
9	13.119	1829	1833	1841	rBV2	14286	25865	3.97%	0.882%
10	14.118	2001	2003	2007	rVB2	11907	12244	1.88%	0.418%
11	14.183	2010	2014	2030	rVV2	347962	551489	84.63%	18.810%
12	15.736	2273	2278	2288	rBV	179605	355780	54.60%	12.135%


Sum of corrected areas: 2931916

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF090418\
Data File : BF108766.D
Acq On : 5 Sep 2018 5:07
Operator : JU/SJ
Sample : J4741-03 10X
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
AOC2-03-C

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

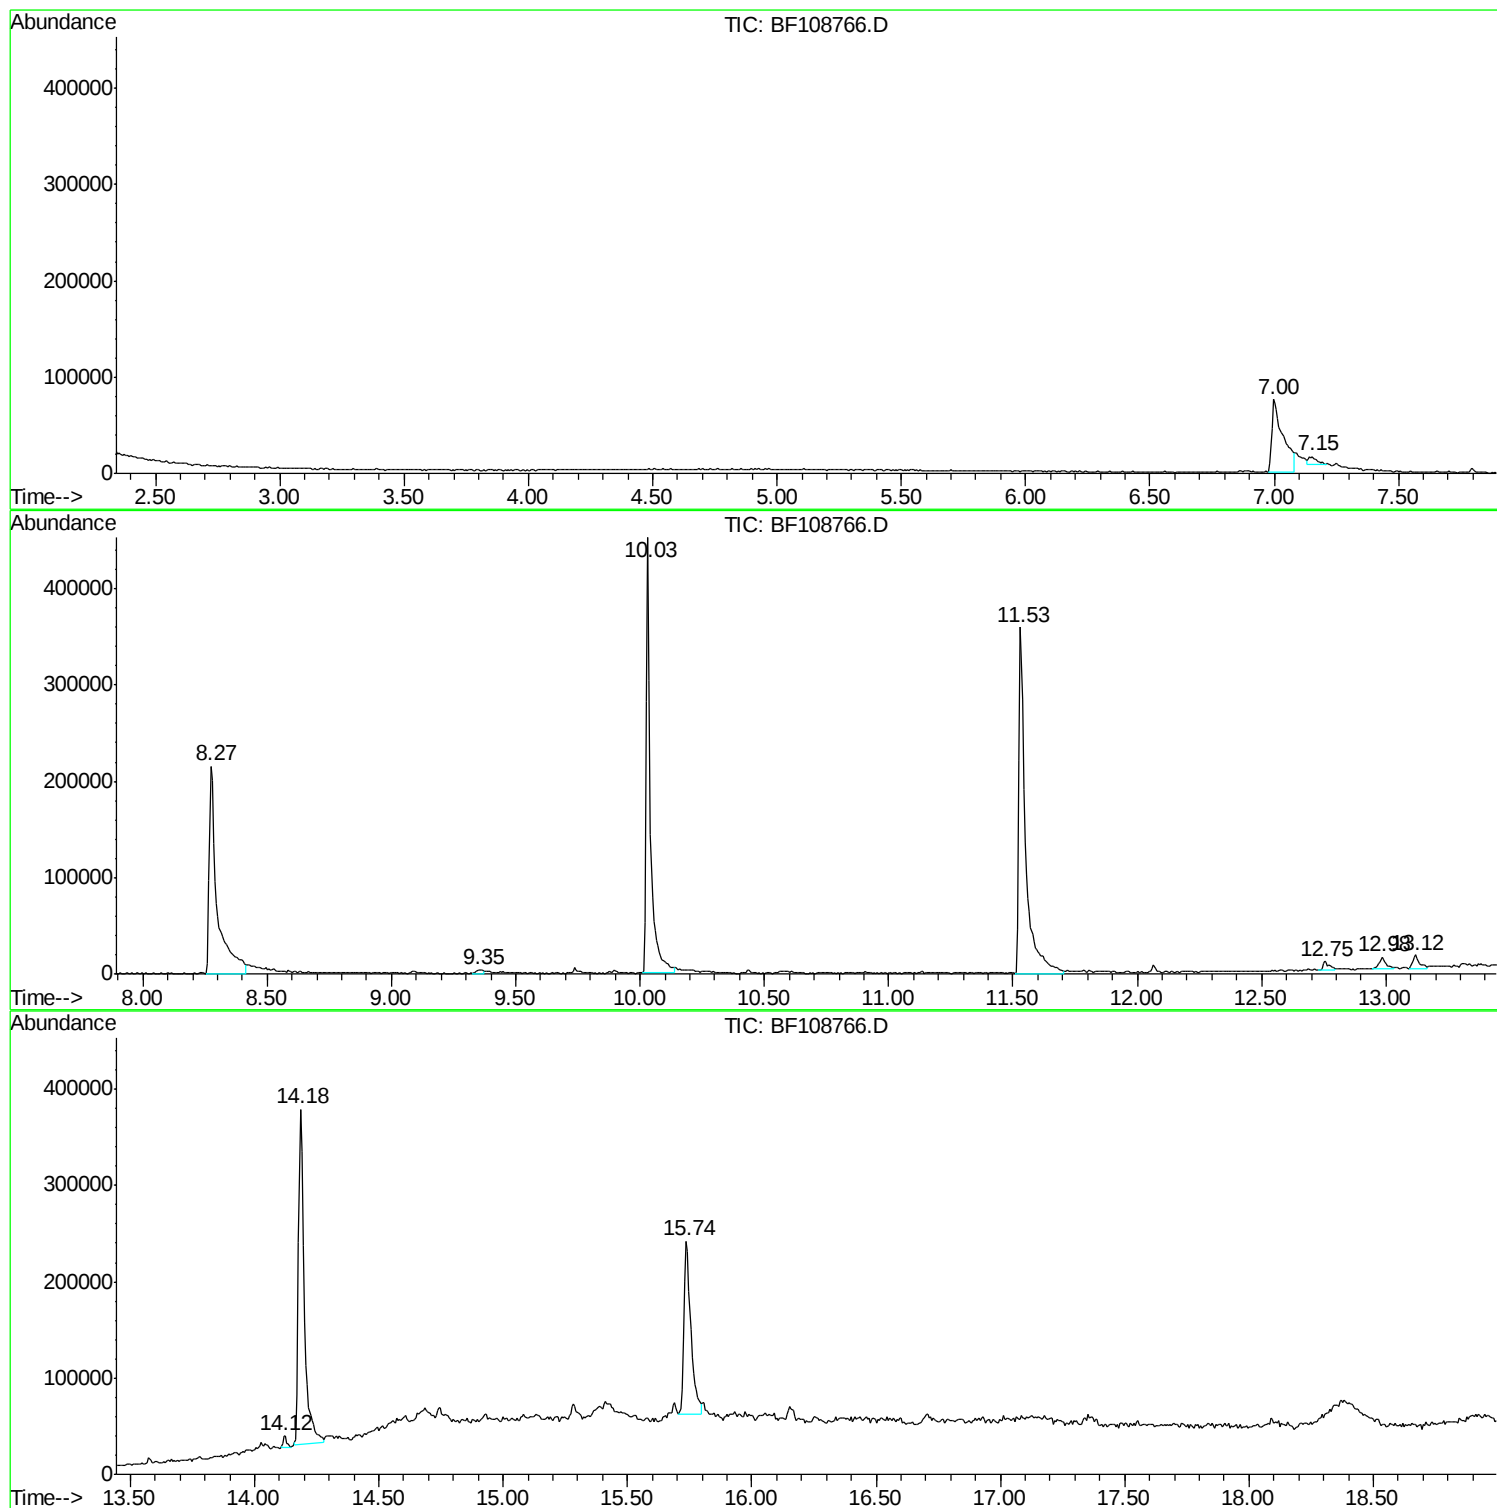

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF090418\
Data_File : BF108766.D
Acq_On : 5-Sep-2018 5:077
Operator : JU/SJJ
Sample : J4741-03-10XX
Misc :
ALS_Vial : 32 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
AOC2-03-C

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF083018.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
