

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF090418\
 Data File : BF108767.D
 Acq On : 5 Sep 2018 5:35
 Operator : JU/SJ
 Sample : J4741-04 10X
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 AOC2-03-D

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF083018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	7.001	788	793	816	rBV	74354	275671	46.88%	9.527%
2	7.148	816	818	831	rVB2	16427	42087	7.16%	1.454%
3	8.278	1006	1010	1034	rBV	176771	417055	70.93%	14.413%
4	9.348	1188	1192	1200	rBV	13548	30595	5.20%	1.057%
5	9.442	1205	1208	1213	rVB4	5626	8311	1.41%	0.287%
6	9.736	1254	1258	1265	rBV	5606	8676	1.48%	0.300%
7	10.030	1304	1308	1327	rBV	422015	515225	87.62%	17.805%
8	10.848	1442	1447	1450	rBV5	5952	11016	1.87%	0.381%
9	11.530	1559	1563	1585	rBV	320425	588019	100.00%	20.321%
10	12.754	1768	1771	1773	rBV3	5833	7451	1.27%	0.257%
11	12.989	1808	1811	1815	rVB4	8106	10772	1.83%	0.372%
12	13.113	1829	1832	1841	rBV	58539	90980	15.47%	3.144%
13	13.289	1860	1862	1863	rBV2	7198	6608	1.12%	0.228%
14	14.183	2011	2014	2029	rBV	345561	543391	92.41%	18.779%
15	15.742	2275	2279	2290	rVB2	175200	337801	57.45%	11.674%


Sum of corrected areas: 2893658

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF090418\
Data File : BF108767.D
Acq On : 5 Sep 2018 5:35
Operator : JU/SJ
Sample : J4741-04 10X
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
AOC2-03-D

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

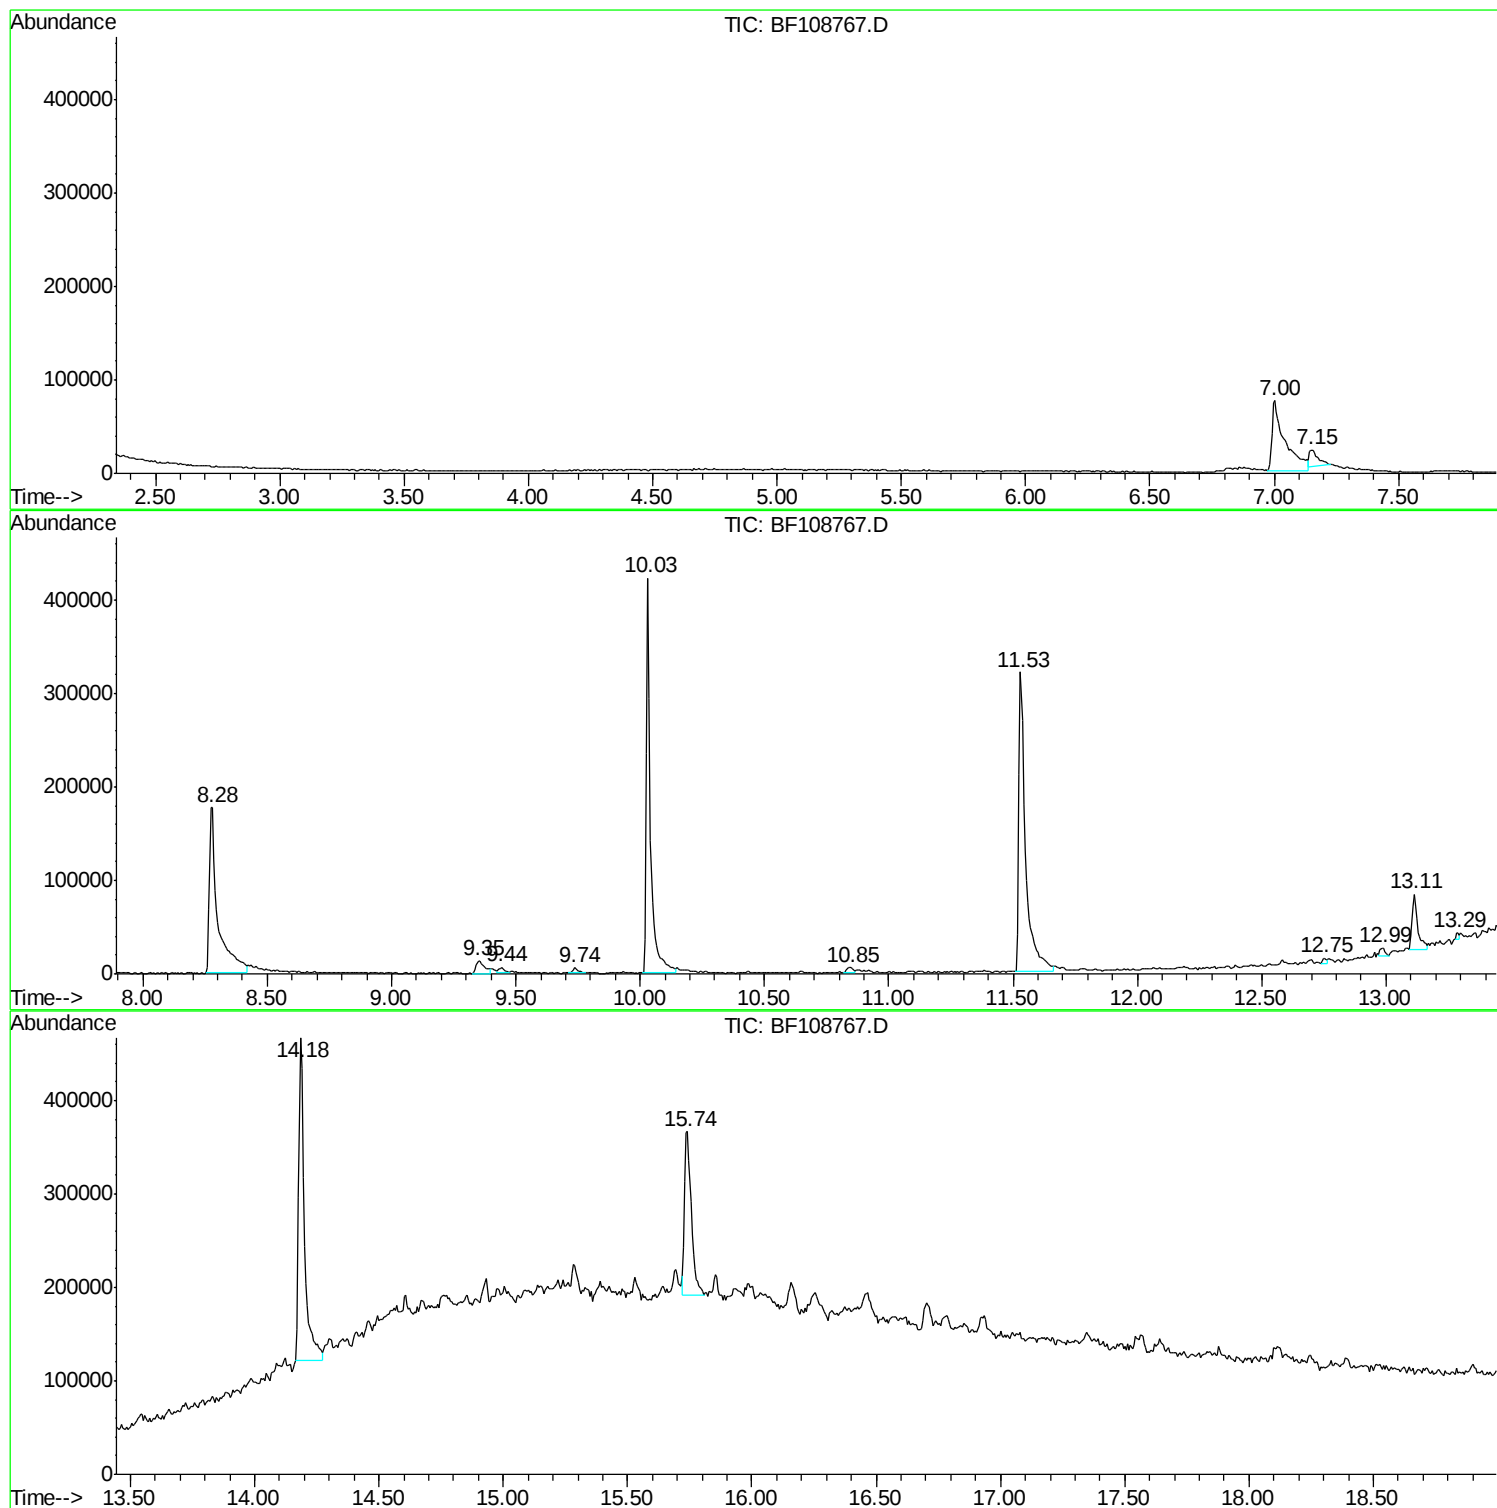

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF090418\
Data_File : BF108767.D
Acq_On : 5-Sep-2018 5:355
Operator : JU/SJJ
Sample : J4741-04 10XX
Misc :
ALS_Vial : 33 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
AOC2-03-D

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF083018.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
