

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF090418\
 Data File : BF108768.D
 Acq On : 5 Sep 2018 6:02
 Operator : JU/SJ
 Sample : J4741-14 10X
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 AOC10-01-B

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF083018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.795	752	758	761	rBV7	8884	19399	2.73%	0.495%
2	6.995	788	792	810	rBV	112618	316490	44.61%	8.084%
3	7.148	814	818	827	rVV	27741	57000	8.03%	1.456%
4	8.272	1006	1009	1040	rBV	226714	503675	70.99%	12.865%
5	9.348	1189	1192	1199	rBV	41325	73635	10.38%	1.881%
6	9.442	1205	1208	1213	rVB3	10711	11739	1.65%	0.300%
7	9.736	1253	1258	1262	rBV	13796	17659	2.49%	0.451%
8	10.030	1304	1308	1327	rBV	492161	587153	82.76%	14.997%
9	10.595	1395	1404	1409	rBV2	6890	15274	2.15%	0.390%
10	10.836	1441	1445	1455	rBV6	16511	42703	6.02%	1.091%
11	11.530	1559	1563	1575	rBV2	386737	709452	100.00%	18.121%
12	12.042	1645	1650	1651	rBV2	9659	13903	1.96%	0.355%
13	12.066	1651	1654	1658	rVB4	6693	11830	1.67%	0.302%
14	12.148	1664	1668	1671	rBV3	14064	19209	2.71%	0.491%
15	12.583	1739	1742	1746	rBV4	11091	17614	2.48%	0.450%
16	12.748	1766	1770	1778	rBV	90097	155515	21.92%	3.972%
17	12.901	1794	1796	1798	rBV3	6913	7534	1.06%	0.192%
18	12.983	1803	1810	1816	rBV	86155	159965	22.55%	4.086%
19	13.113	1828	1832	1842	rBV	113376	185076	26.09%	4.727%
20	13.289	1859	1862	1863	rBV3	13737	15046	2.12%	0.384%
21	13.313	1864	1866	1873	rVB	20488	28703	4.05%	0.733%
22	13.507	1897	1899	1901	rBV3	10154	9182	1.29%	0.235%
23	14.183	2010	2014	2027	rBV2	345123	590281	83.20%	15.077%
24	15.742	2275	2279	2293	rVB2	177045	347130	48.93%	8.866%


Sum of corrected areas: 3915167

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF090418\
Data File : BF108768.D
Acq On : 5 Sep 2018 6:02
Operator : JU/SJ
Sample : J4741-14 10X
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
AOC10-01-B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

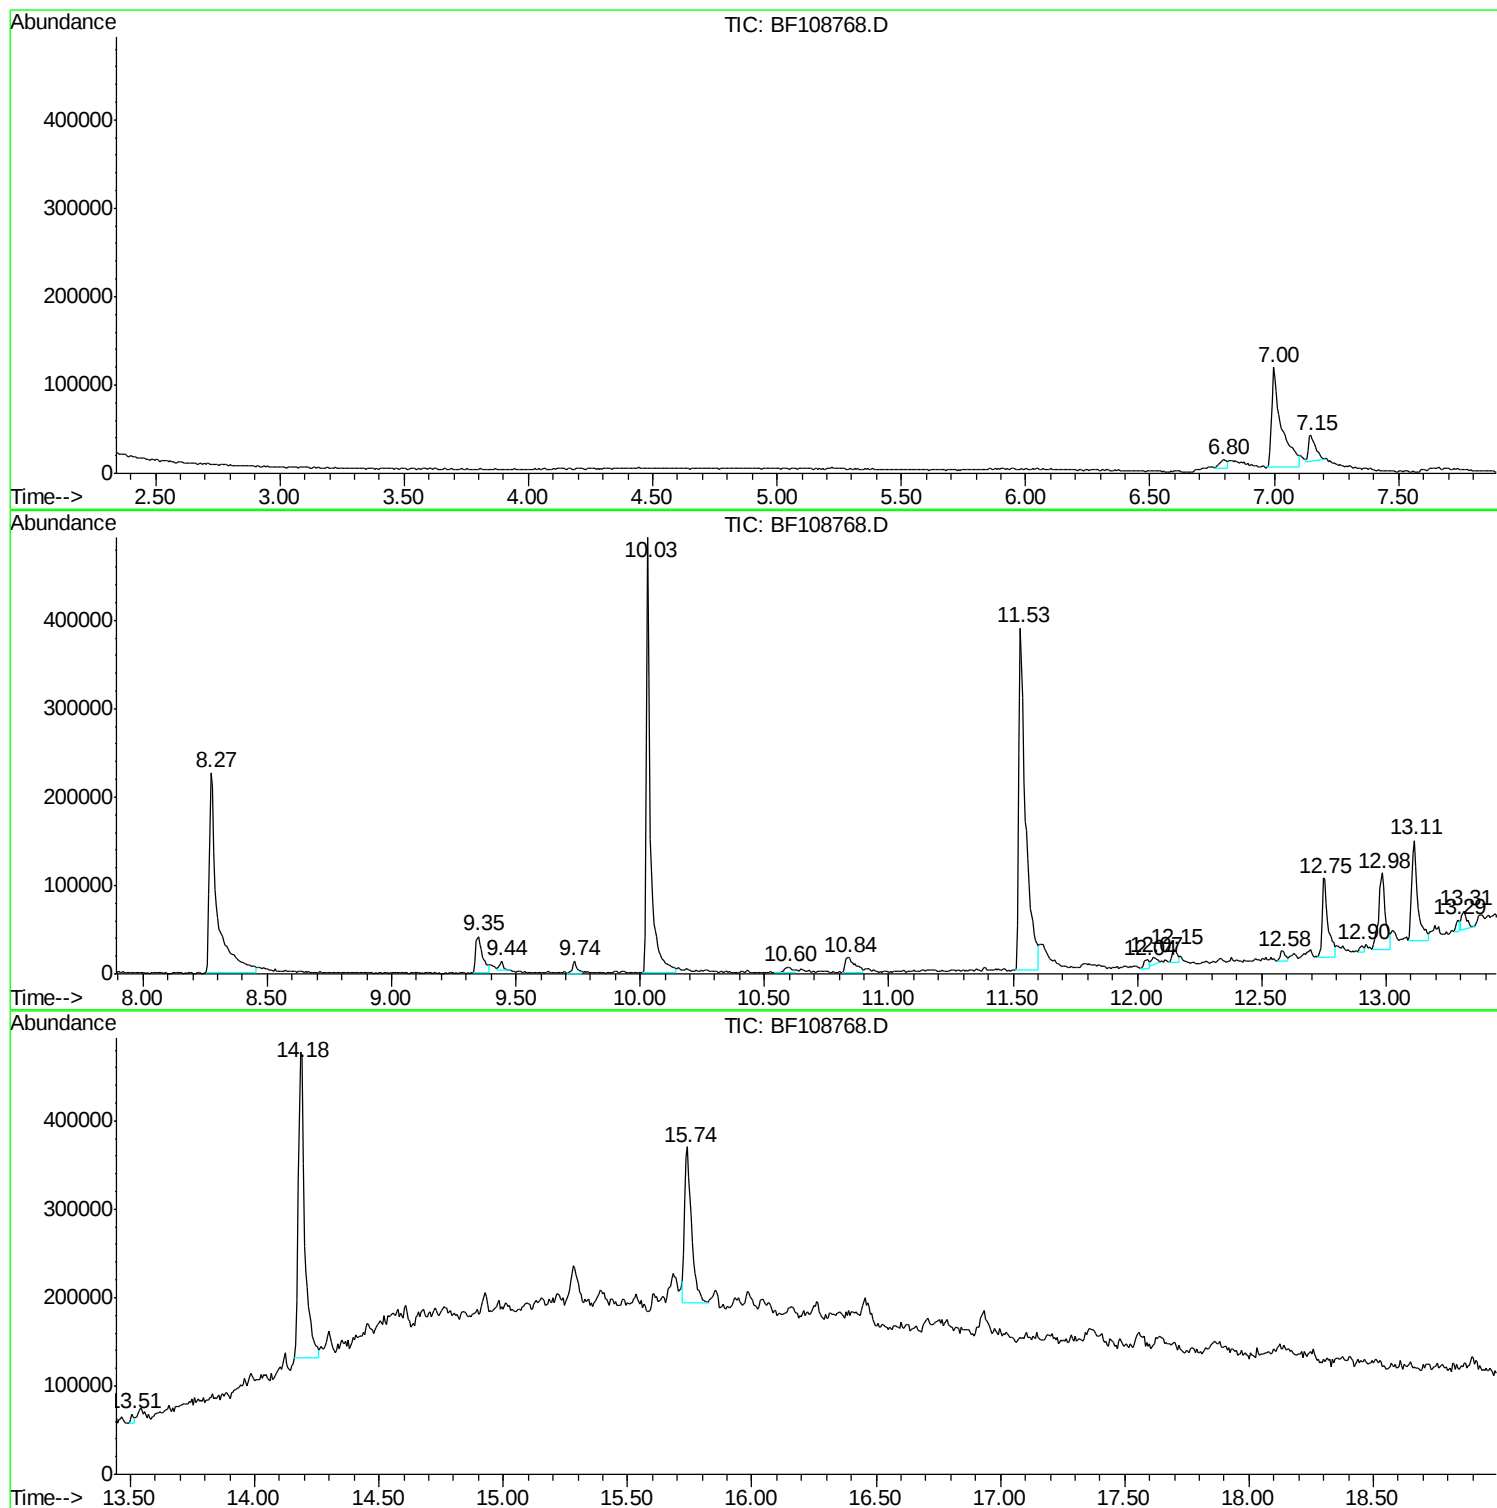

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF090418\
Data_File : BF108768.D
Acq_On : 5-Sep-2018 6:022
Operator : JU/SJJ
Sample : J4741-14 10XX
Misc :
ALS_Vial : 34 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
AOC10-01-B

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF083018.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
