

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF090418\
 Data File : BF108769.D
 Acq On : 5 Sep 2018 6:29
 Operator : JU/SJ
 Sample : J4741-06 10X
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 AOC2-04-B

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF083018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.807	753	760	761	rBV3	5594	9915	1.64%	0.296%
2	6.995	789	792	812	rBV	85622	269458	44.46%	8.051%
3	7.148	815	818	829	rVB	26321	56762	9.37%	1.696%
4	8.272	1006	1009	1035	rBV	178194	409297	67.53%	12.229%
5	9.348	1188	1192	1199	rBV	31769	57425	9.48%	1.716%
6	9.736	1254	1258	1263	rBV	12473	15351	2.53%	0.459%
7	10.031	1305	1308	1321	rBV	415602	478252	78.91%	14.290%
8	10.836	1441	1445	1452	rBV3	13041	28904	4.77%	0.864%
9	11.001	1468	1473	1475	rBV2	6268	9063	1.50%	0.271%
10	11.030	1475	1478	1481	rVB2	4786	6982	1.15%	0.209%
11	11.177	1500	1503	1507	rBV3	4386	6503	1.07%	0.194%
12	11.530	1559	1563	1582	rBV	326649	579782	95.66%	17.323%
13	12.583	1738	1742	1745	rBV4	9158	11882	1.96%	0.355%
14	12.754	1768	1771	1779	rBV	40313	70344	11.61%	2.102%
15	12.895	1794	1795	1797	rBV2	7026	6518	1.08%	0.195%
16	12.983	1803	1810	1816	rBV	52448	98563	16.26%	2.945%
17	13.113	1829	1832	1842	rBV	103000	162005	26.73%	4.841%
18	14.124	2001	2004	2008	rVB	45701	47603	7.85%	1.422%
19	14.189	2011	2015	2025	rVV	379521	606063	100.00%	18.109%
20	15.742	2275	2279	2292	rVB	212307	416156	68.67%	12.434%


Sum of corrected areas: 3346828

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF090418\
Data File : BF108769.D
Acq On : 5 Sep 2018 6:29
Operator : JU/SJ
Sample : J4741-06 10X
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
AOC2-04-B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

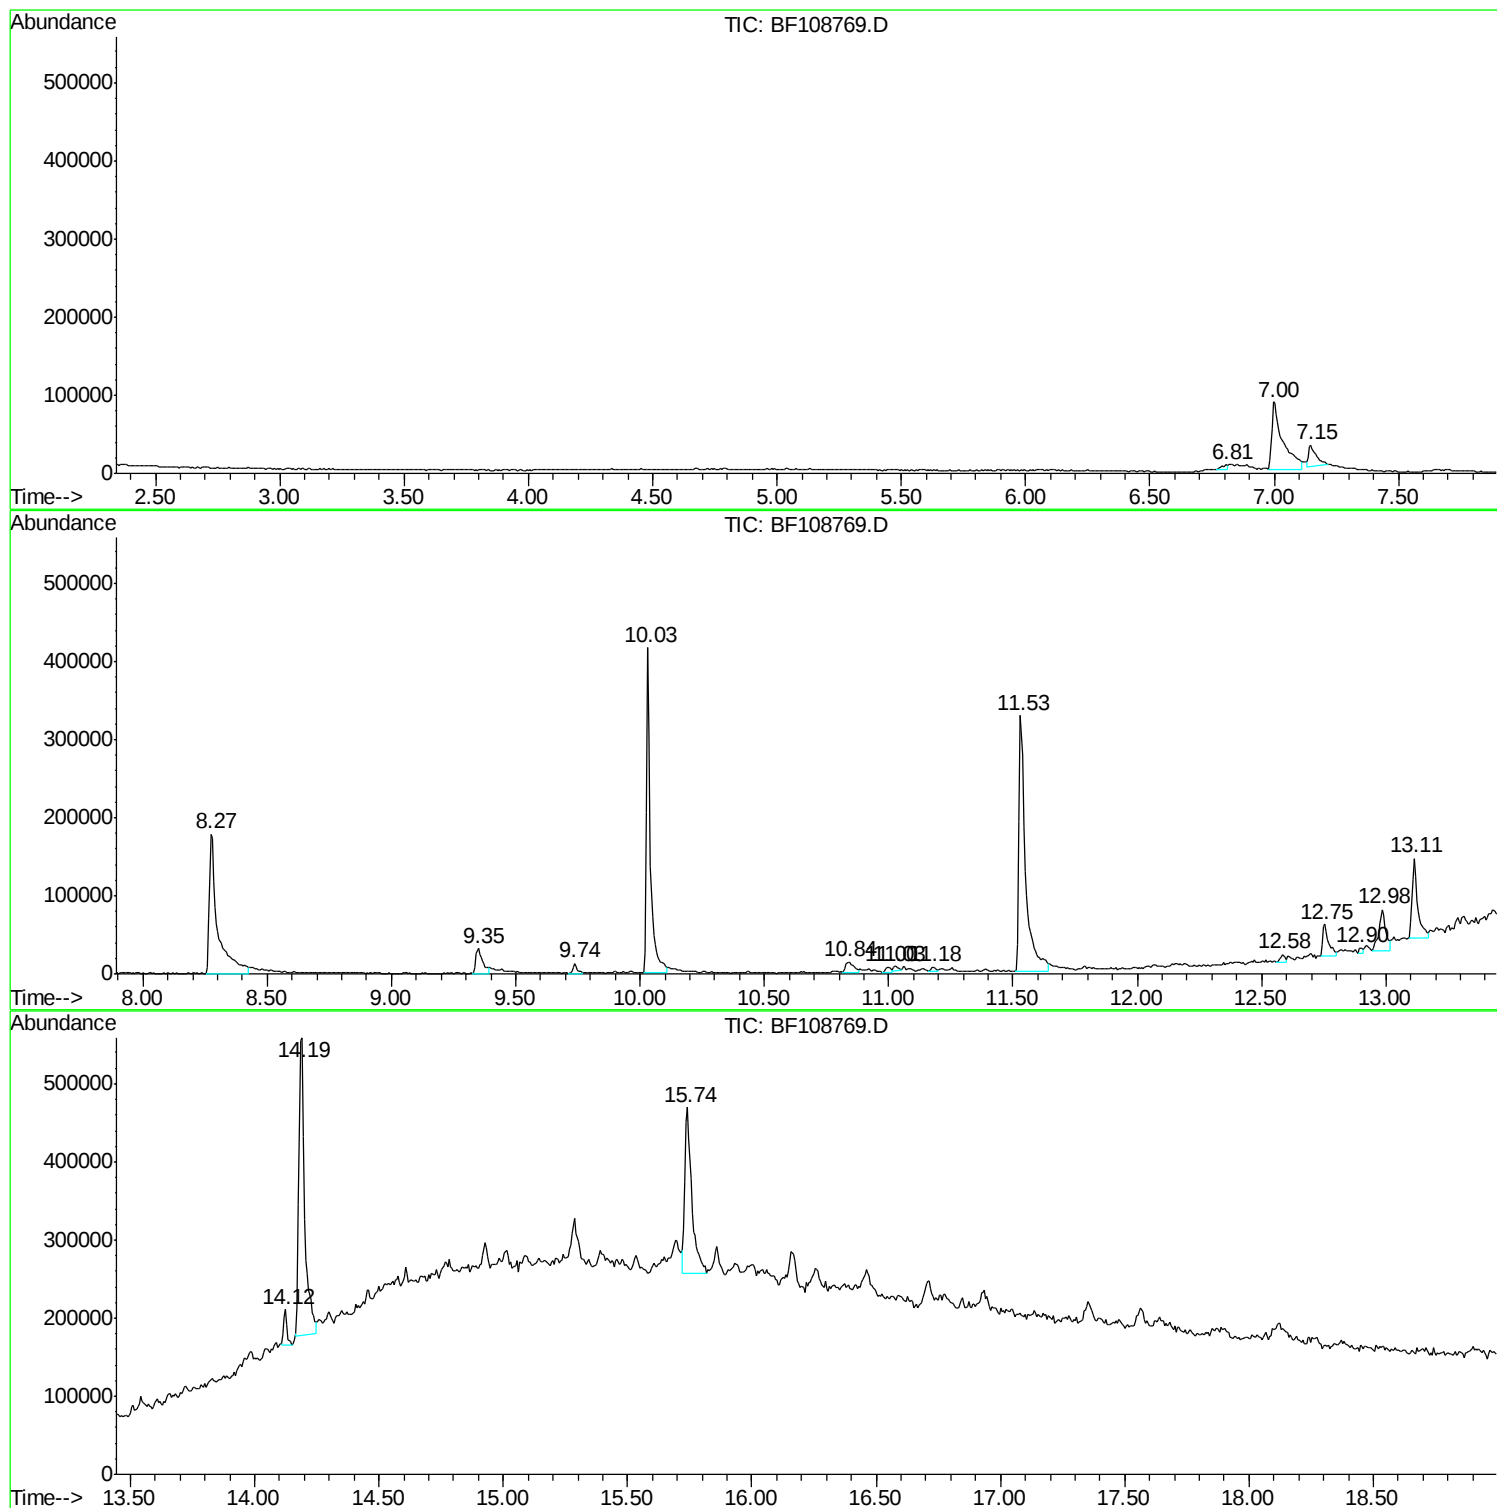

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF090418\
Data_File : BF108769.D
Acq_On : 5-Sep-2018 6:299
Operator : JU/SJJ
Sample : J4741-06-10XX
Misc :
ALS_Vial : 35 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
AOC2-04-B

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF083018.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
