

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF090418\
 Data File : BF108770.D
 Acq On : 5 Sep 2018 6:56
 Operator : JU/SJ
 Sample : J4741-08 10X
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 AOC2-04-D

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF083018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.995	788	792	813	rBV	105931	318467	47.53%	9.751%
2	7.148	815	818	828	rVB2	21358	45067	6.73%	1.380%
3	8.277	1006	1010	1026	rBV	226775	446264	66.60%	13.663%
4	9.348	1188	1192	1201	rBV	28567	54154	8.08%	1.658%
5	9.442	1205	1208	1215	rVB4	5312	9642	1.44%	0.295%
6	9.736	1253	1258	1264	rBV2	15341	23623	3.53%	0.723%
7	10.030	1305	1308	1328	rVV2	487315	574120	85.68%	17.578%
8	10.842	1441	1446	1454	rBV4	9879	23183	3.46%	0.710%
9	10.919	1457	1459	1464	rVB3	7893	7756	1.16%	0.237%
10	11.530	1559	1563	1585	rBV	372100	670062	100.00%	20.516%
11	12.154	1665	1669	1670	rBV4	5522	7090	1.06%	0.217%
12	12.460	1718	1721	1723	rBV4	6035	8970	1.34%	0.275%
13	12.583	1739	1742	1744	rBV3	19426	19234	2.87%	0.589%
14	12.754	1768	1771	1773	rBV	18468	22297	3.33%	0.683%
15	12.983	1807	1810	1816	rBV2	27572	42860	6.40%	1.312%
16	13.112	1829	1832	1842	rBV	76587	117068	17.47%	3.584%
17	14.124	2002	2004	2006	rVB	52577	38033	5.68%	1.164%
18	14.189	2011	2015	2027	rVV	300108	487103	72.70%	14.914%
19	15.742	2276	2279	2291	rVB	174793	351111	52.40%	10.750%


Sum of corrected areas: 3266104

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF090418\
Data File : BF108770.D
Acq On : 5 Sep 2018 6:56
Operator : JU/SJ
Sample : J4741-08 10X
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
AOC2-04-D

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF083018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

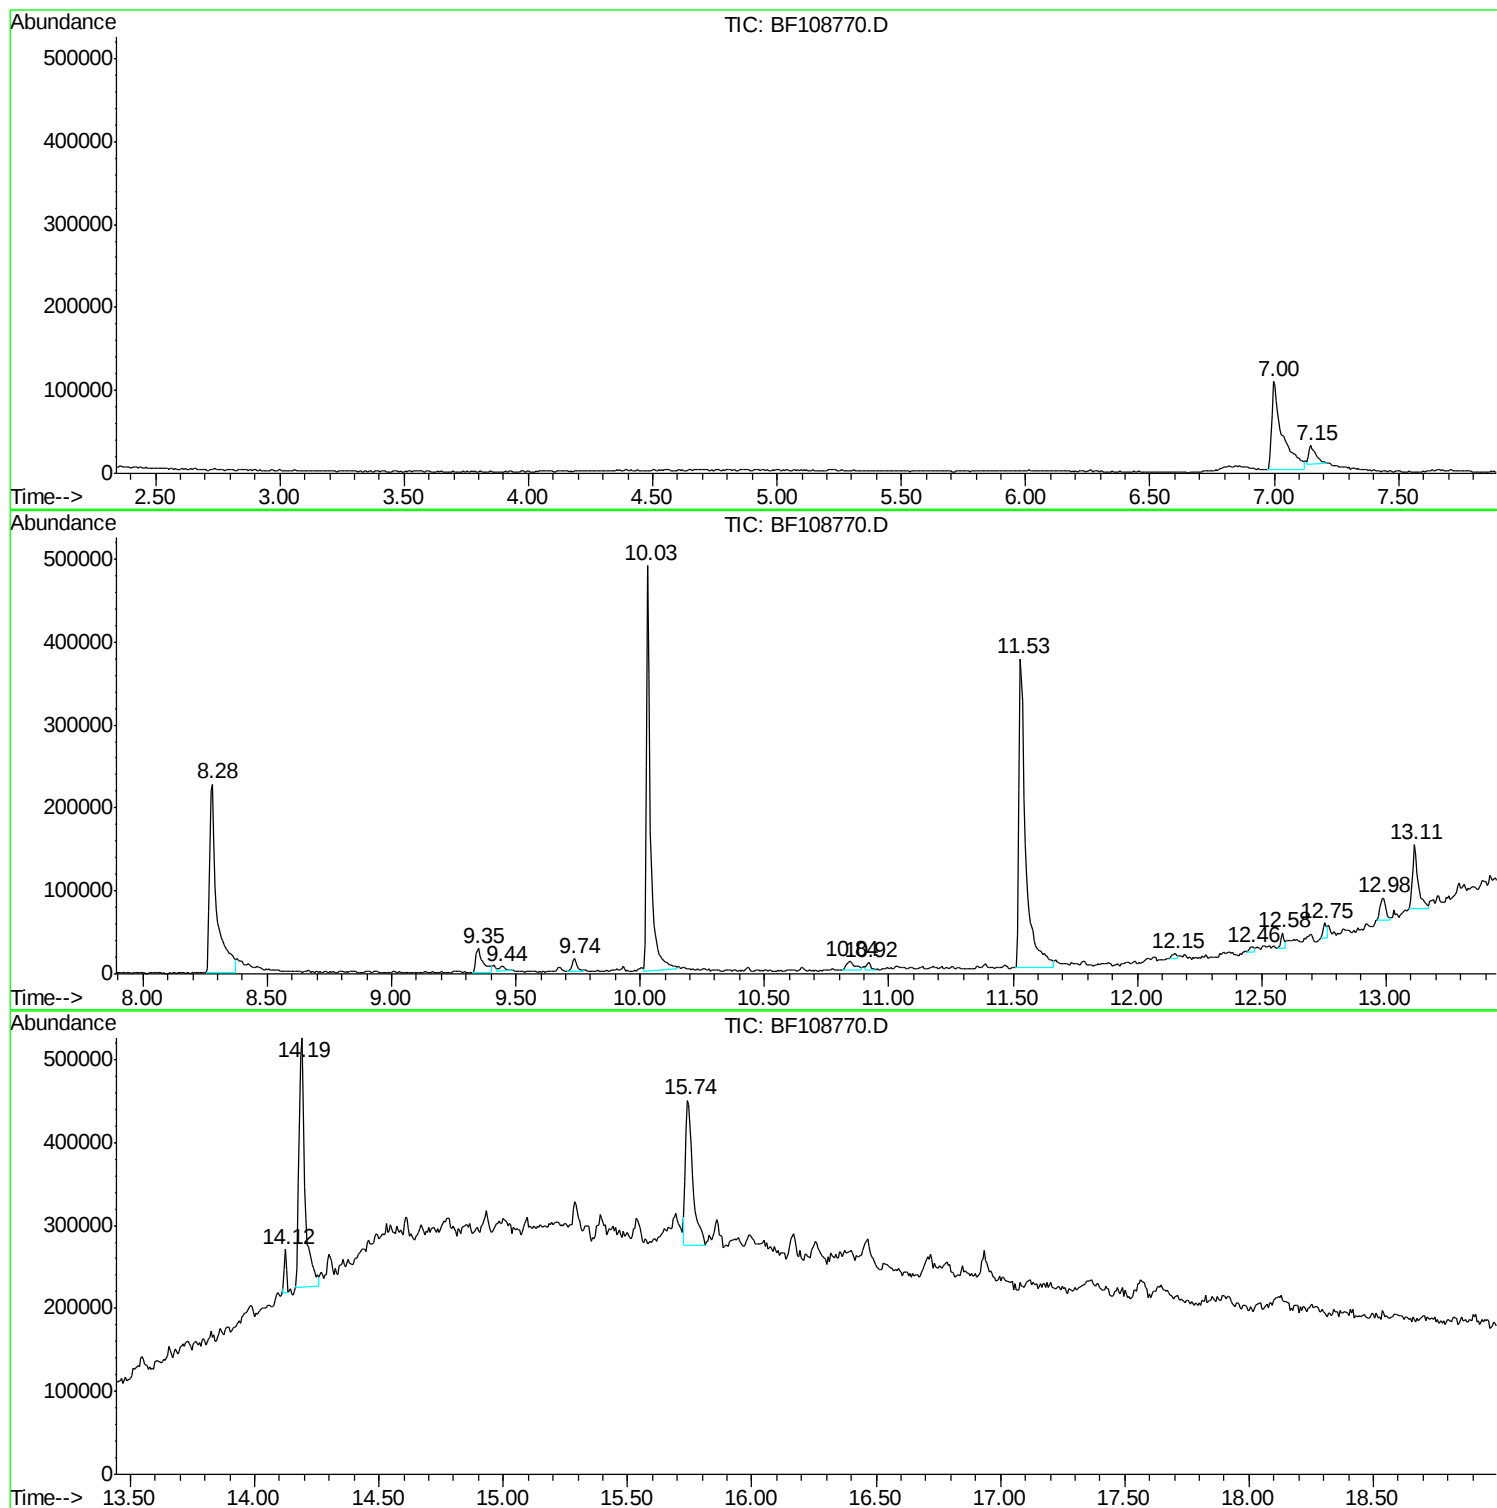

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF090418\
Data_File : BF108770.D
Acq_On : 5-Sep-2018 6:566
Operator : JU/SJJ
Sample : J4741-08-10XX
Misc :
ALS_Vial : 36 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
AOC2-04-D

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF083018.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
