
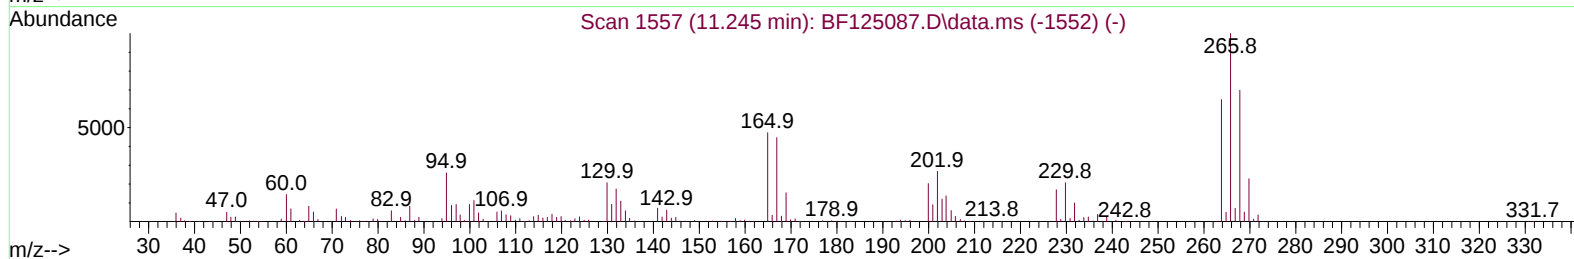
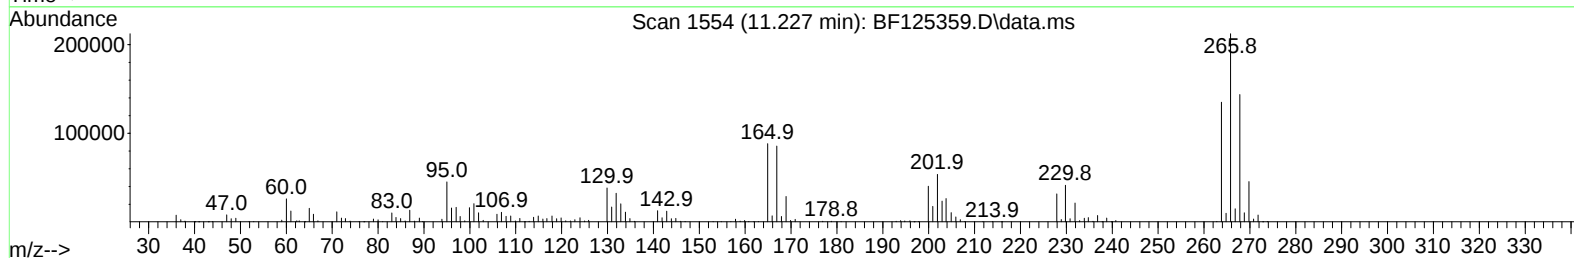


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090421\
Data File : BF125359.D
Acq On : 4 Sep 2021 9:36
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 06 09:16:47 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 03 11:56:34 2021
Response via : Initial Calibration

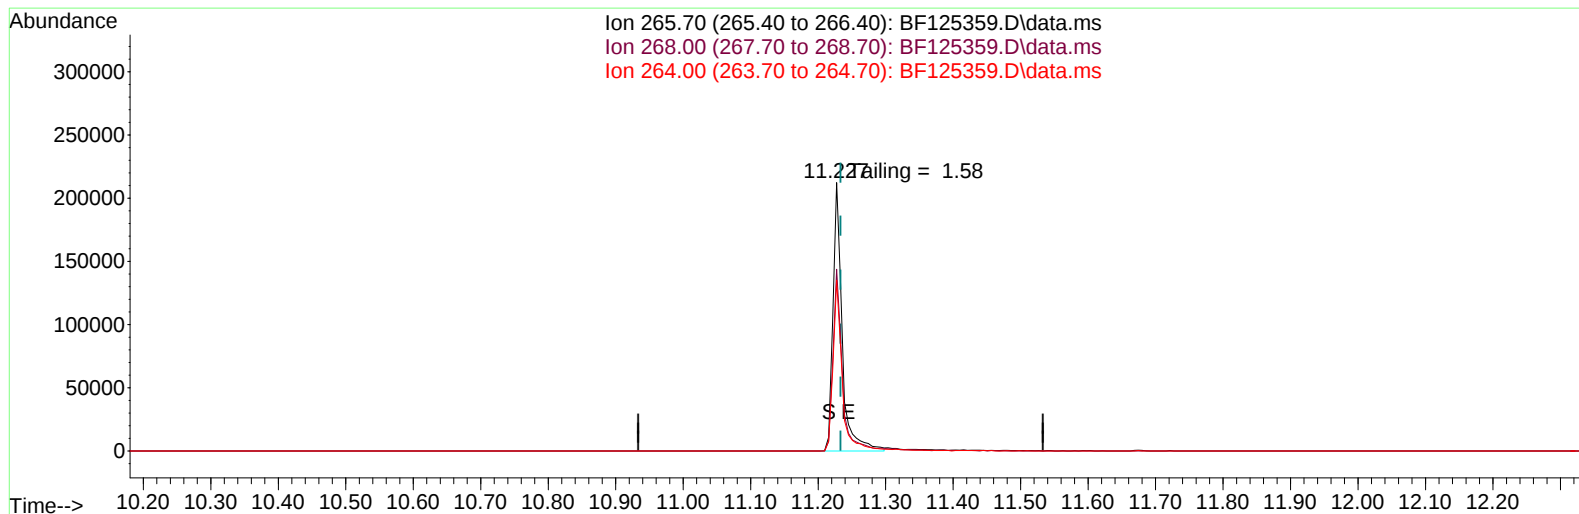

TIC: BF125359.D\data.ms

(70) Pentachlorophenol (C)




11.227min (-0.006) 24800.59 ng

response 205721

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	67.74
264.00	69.90	63.61
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090421\
Data File : BF125359.D
Acq On : 4 Sep 2021 9:36
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 06 09:16:47 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 03 11:56:34 2021
Response via : Initial Calibration

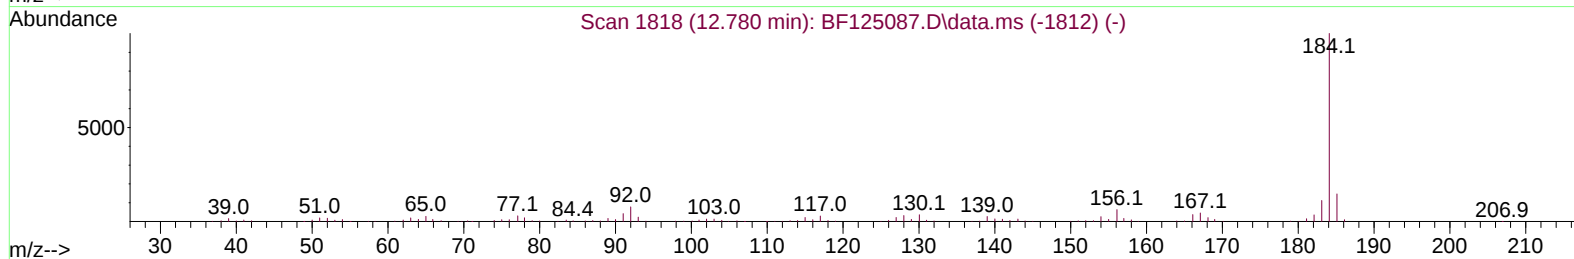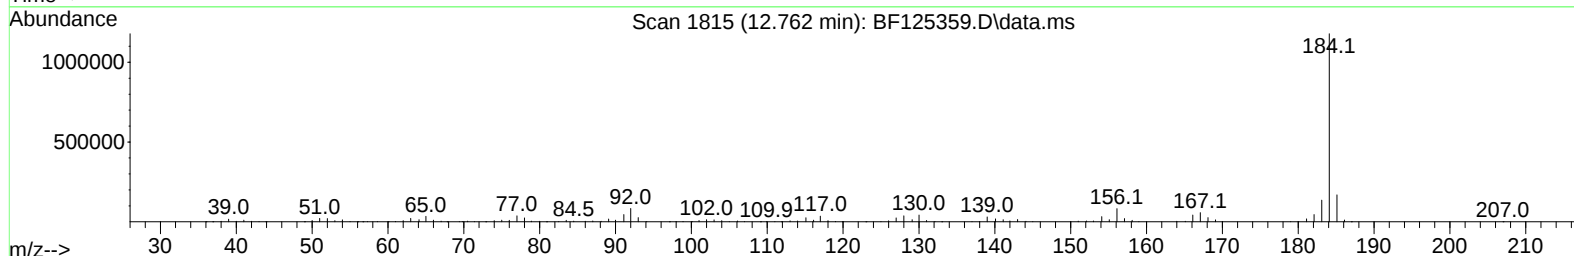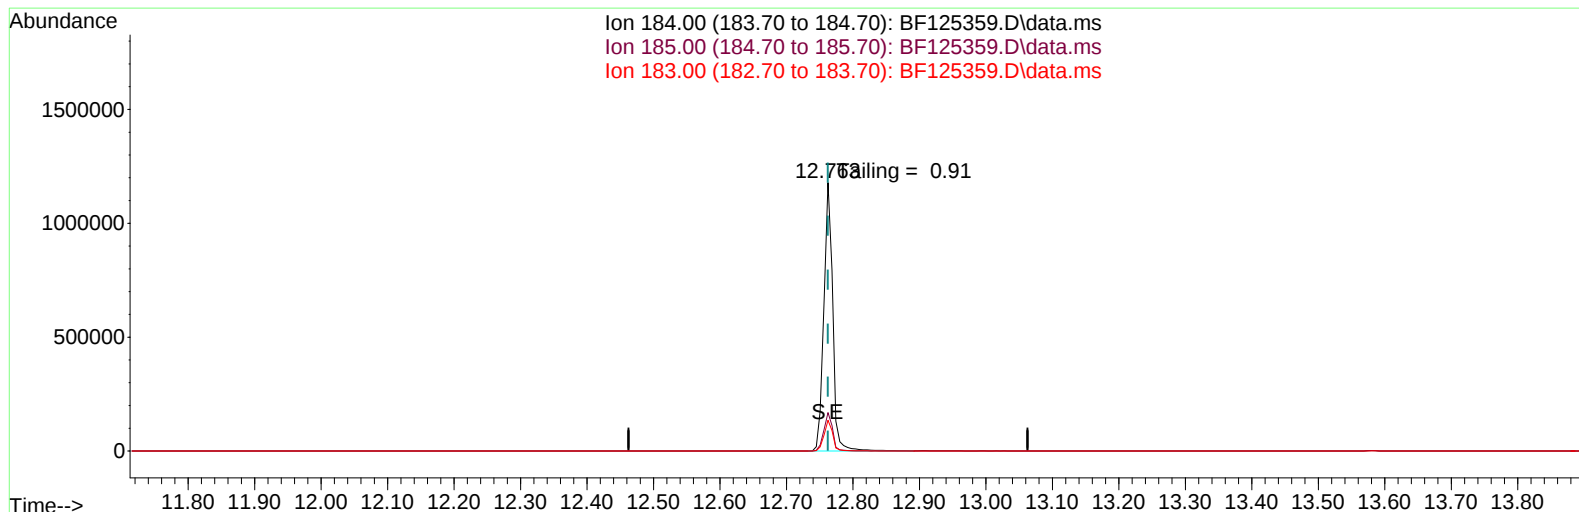

TIC: BF125359.D\data.ms

(77) Benzidine

12.762min (-0.000) 0.00 ng

response 1097141

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.35
183.00	10.10	11.48
0.00	0.00	0.00