
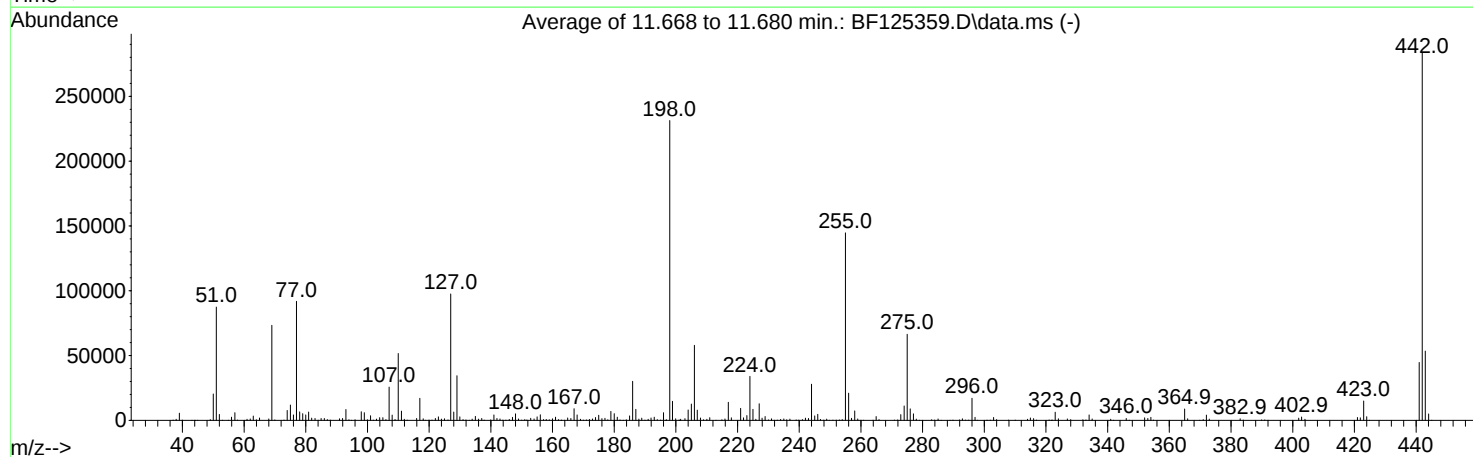


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090421\
 Data File : BF125359.D
 Acq On : 4 Sep 2021 9:36
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 03 11:56:34 2021

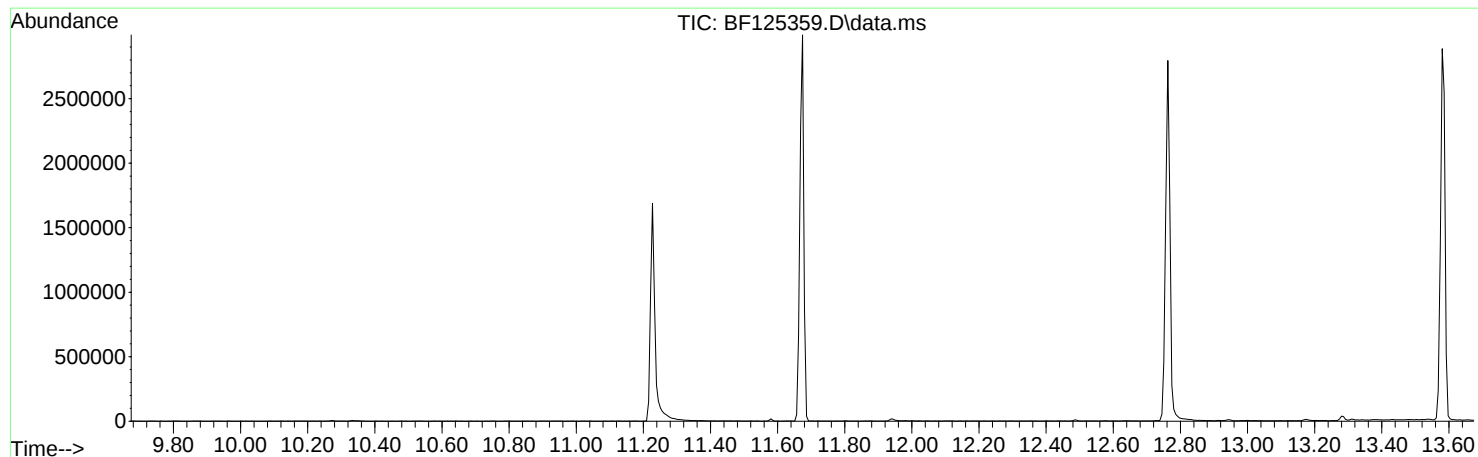

AutoFind: Scans 1629, 1630, 1631; Background Corrected with Scan 1624

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.8	87382	PASS
68	69	0.00	2	1.4	1058	PASS
69	198	0.00	100	31.7	73331	PASS
70	69	0.00	2	0.6	408	PASS
127	198	10	80	42.2	97539	PASS
197	198	0.00	2	0.2	509	PASS
198	198	100	100	100.0	231285	PASS
199	198	5	9	6.4	14758	PASS
275	198	10	60	28.7	66411	PASS
365	198	1	100	3.8	8829	PASS
441	198	0.01	100	19.3	44733	PASS
442	442	50	100	100.0	283776	PASS
443	442	15	24	18.9	53493	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
9/4/2021	BNA_F	<u>BF125359.D</u>
Compound Name	Response	Retention Time
DDT	558576	13.58
DDD	11159	13.286
DDE	1582	12.945
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12741	571317	2.23

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090421\
Data File : BF125359.D
Acq On : 4 Sep 2021 9:36
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 06 09:16:47 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 03 11:56:34 2021
Response via : Initial Calibration

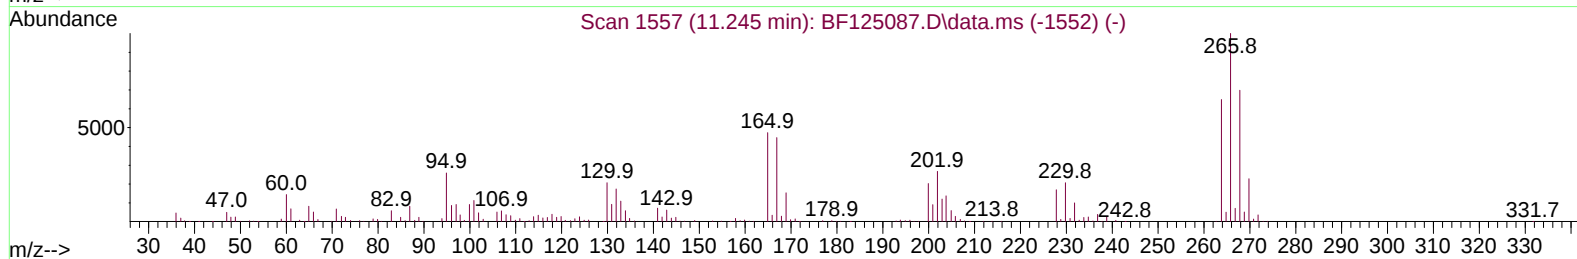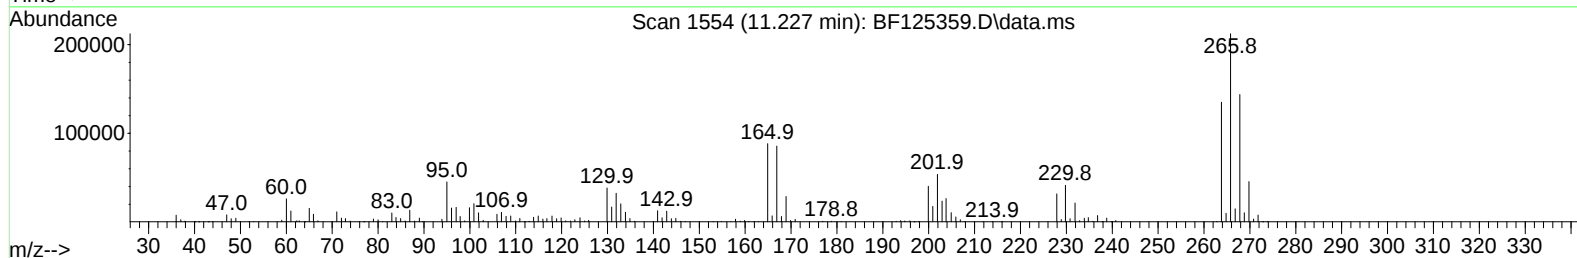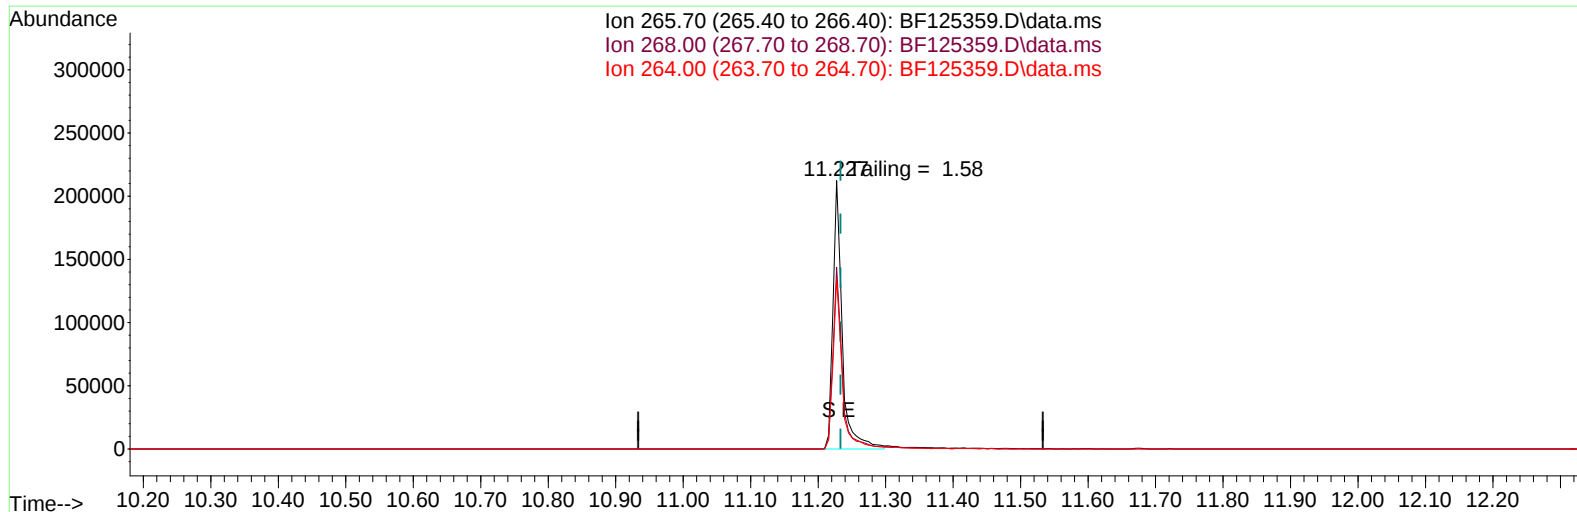

TIC: BF125359.D\data.ms

(70) Pentachlorophenol (C)

11.227min (-0.006) 24800.59 ng




response 205721

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	67.74
264.00	69.90	63.61
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090421\
 Data File : BF125359.D
 Acq On : 4 Sep 2021 9:36
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Sep 06 09:16:47 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 03 11:56:34 2021
 Response via : Initial Calibration

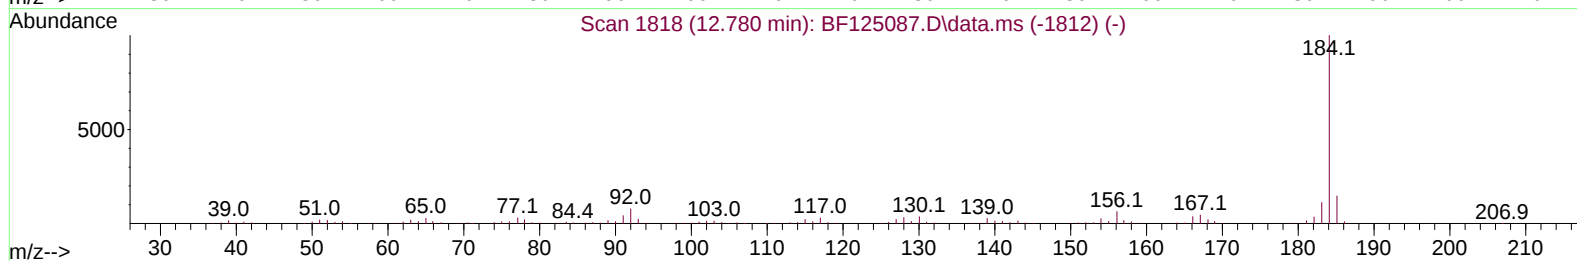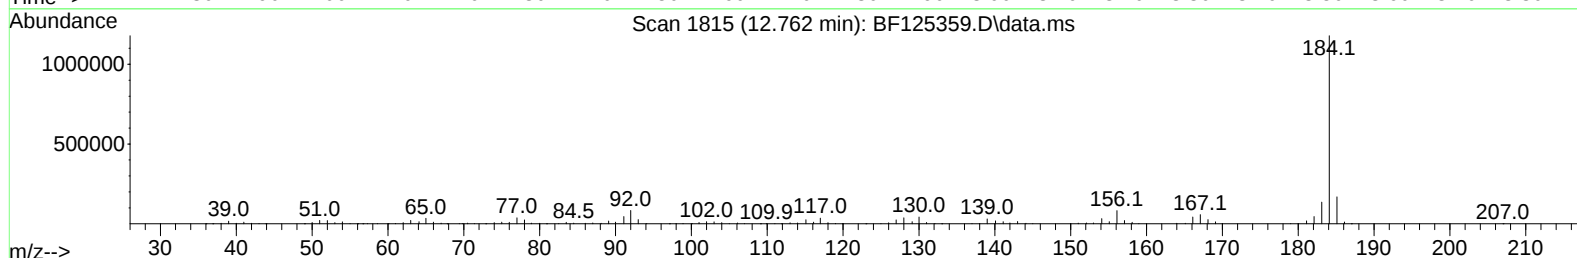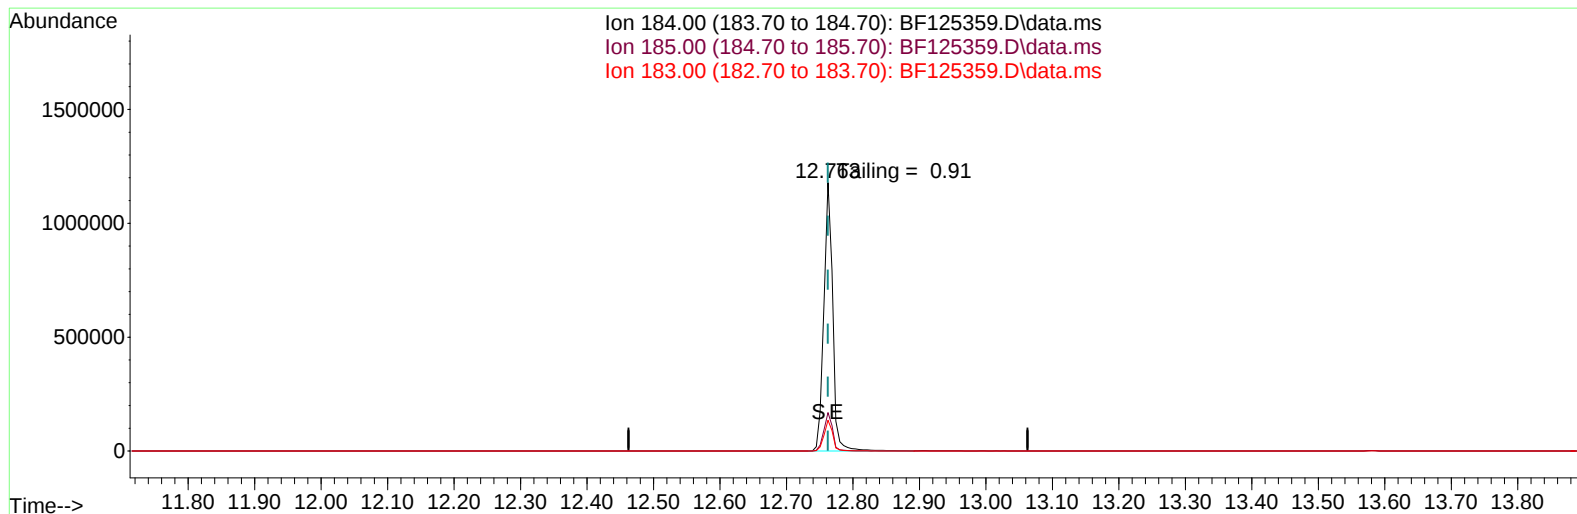

TIC: BF125359.D\data.ms

(77) Benzidine

12.762min (-0.000) 0.00 ng

response 1097141

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.35
183.00	10.10	11.48
0.00	0.00	0.00