
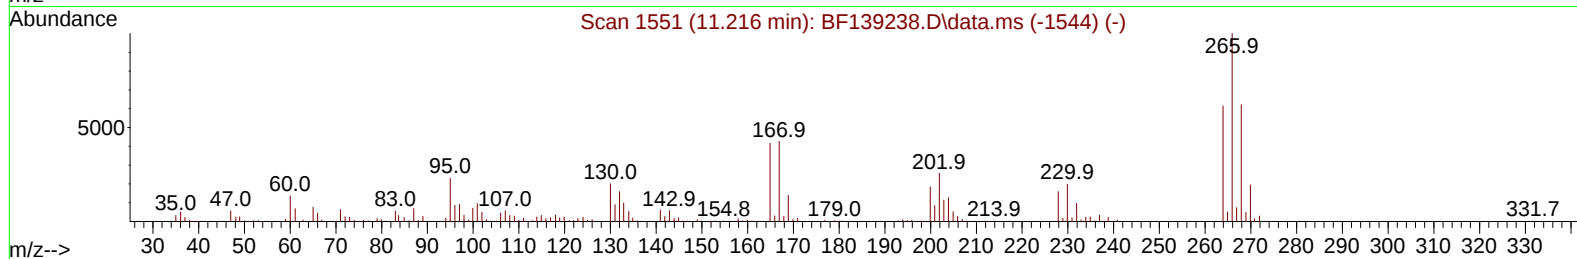
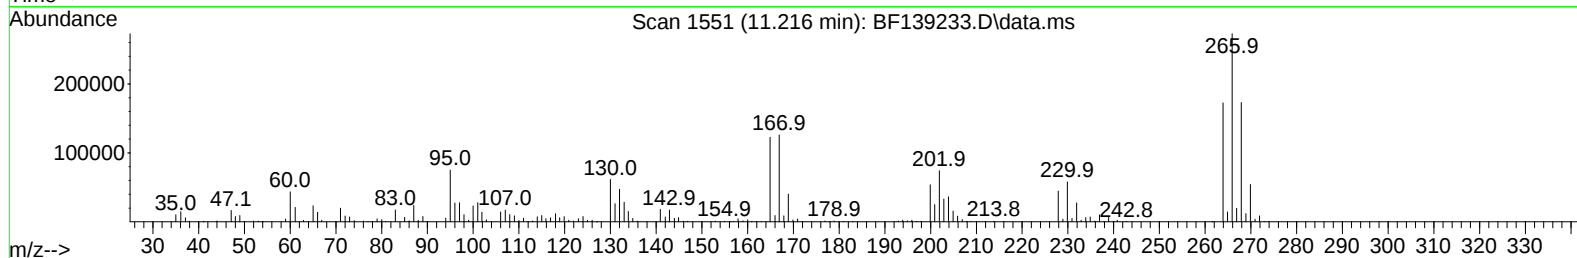


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090424\
Data File : BF139233.D
Acq On : 04 Sep 2024 11:09
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 04 13:35:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF090424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 04 13:35:04 2024
Response via : Initial Calibration

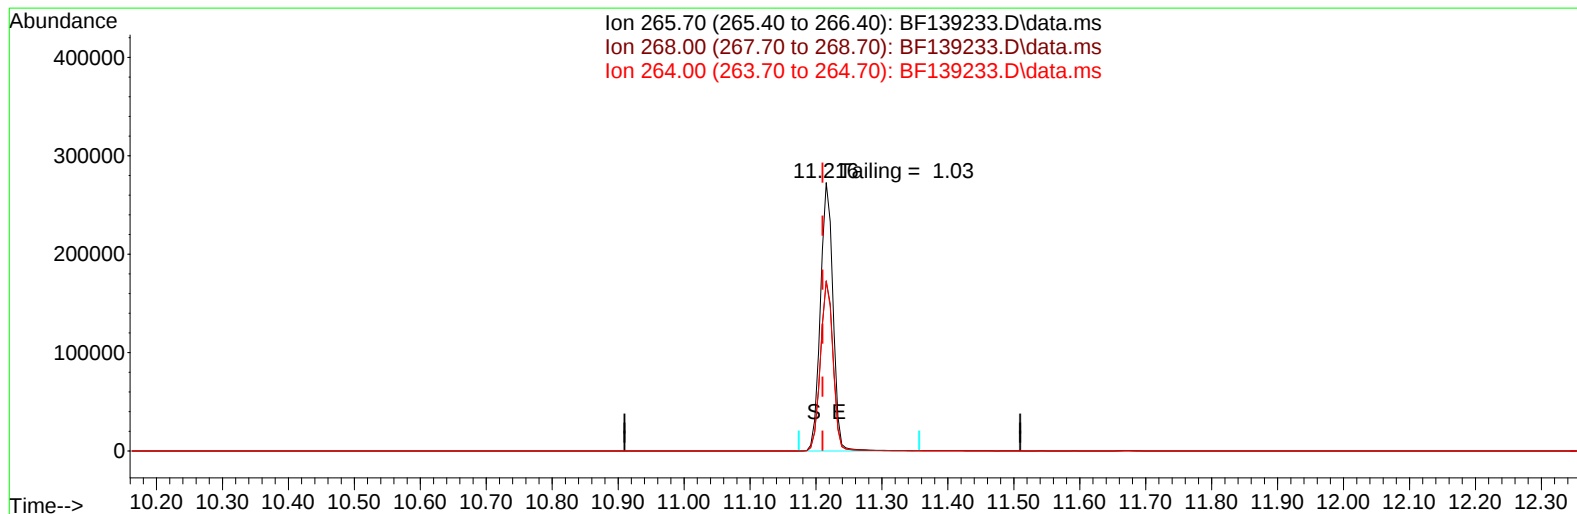

TIC: BF139233.D\data.ms

(70) Pentachlorophenol (C)




11.216min (+ 0.006) 32762.20 ng

response 363720

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	63.42
264.00	62.80	63.23
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090424\
Data File : BF139233.D
Acq On : 04 Sep 2024 11:09
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 04 13:35:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF090424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 04 13:35:04 2024
Response via : Initial Calibration

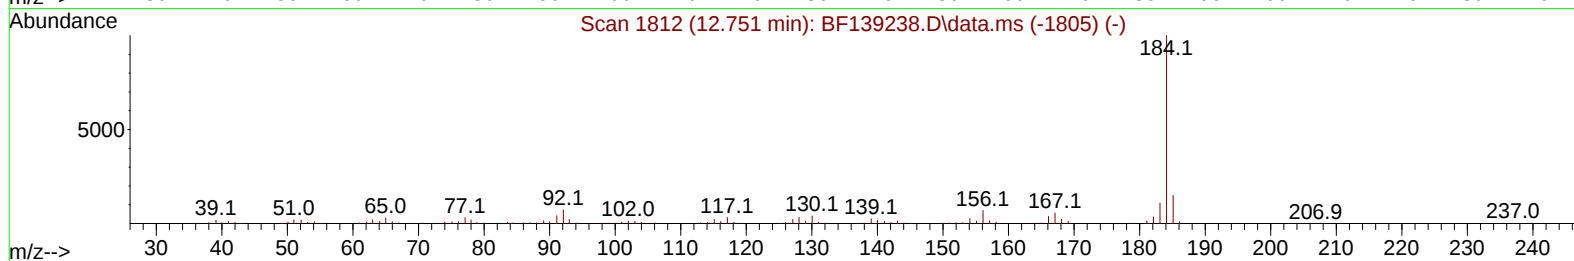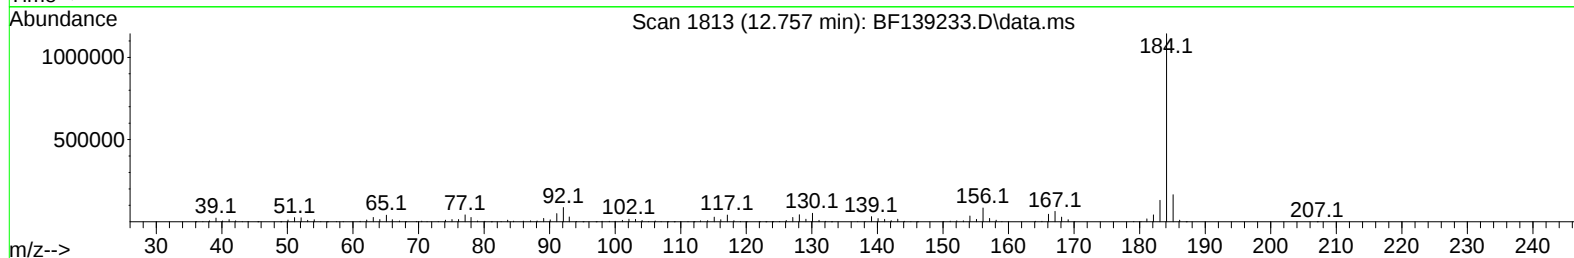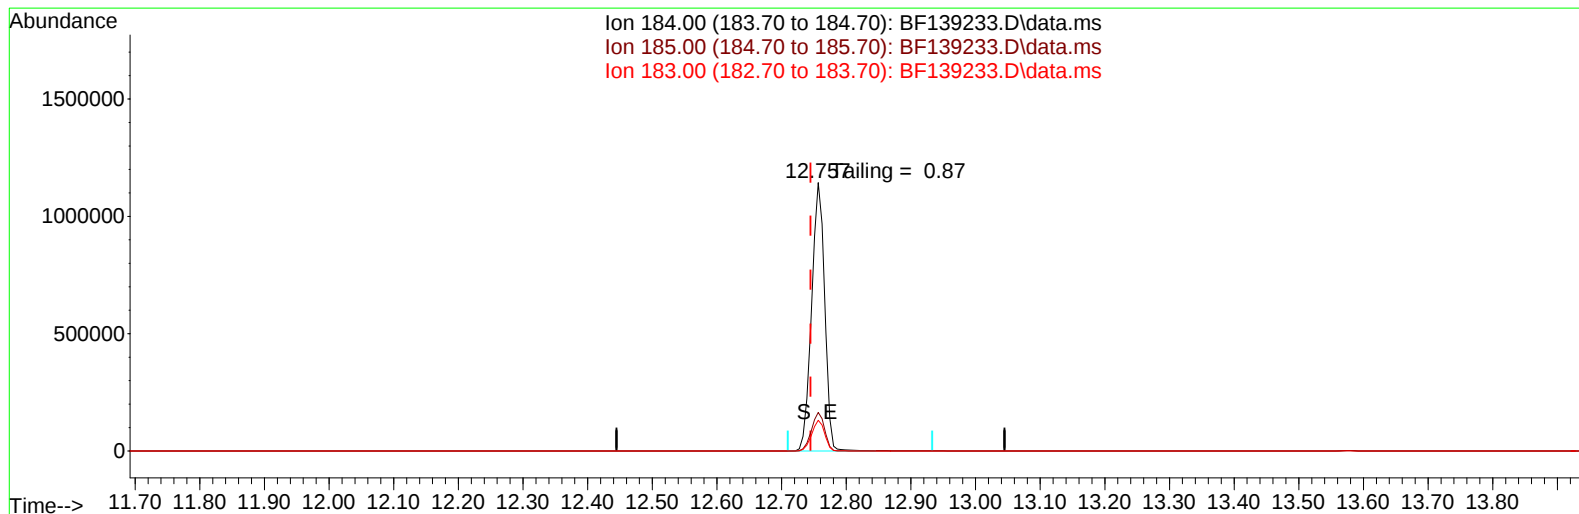

TIC: BF139233.D\data.ms

(77) Benzidine

12.757min (+ 0.012) 0.00 ng

response 1614907

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.39
183.00	11.90	11.45
0.00	0.00	0.00